

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120920\
 Data File : FB025313.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2020 16:18
 Operator : DD/AJ
 Sample : L4880-06MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 KENS-B4-112320-0-2MSD

Integration File: Calibration.e
 Quant Time: Dec 10 00:11:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	390250	18.563 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	797112	26.514 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	754644	25.080 ng/ml
3) t n-Heptane	7.759	243382	8.219 ng/ml
4) t Benzene	7.893	355479	9.611 ng/ml
6) t Toluene	10.632	1002906	28.540 ng/ml
7) t Ethylbenzene	13.073	296515	9.078 ng/ml
8) t m-Xylene	13.205	588878	18.194 ng/ml
9) t O-Xylene	13.933	572941	18.124 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	464399	17.102 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120920\
Data File : FB025313.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2020 16:18
Operator : DD/AJ
Sample : L4880-06MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-B4-112320-0-2MSD

Integration File: Calibration.e
Quant Time: Dec 10 00:11:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

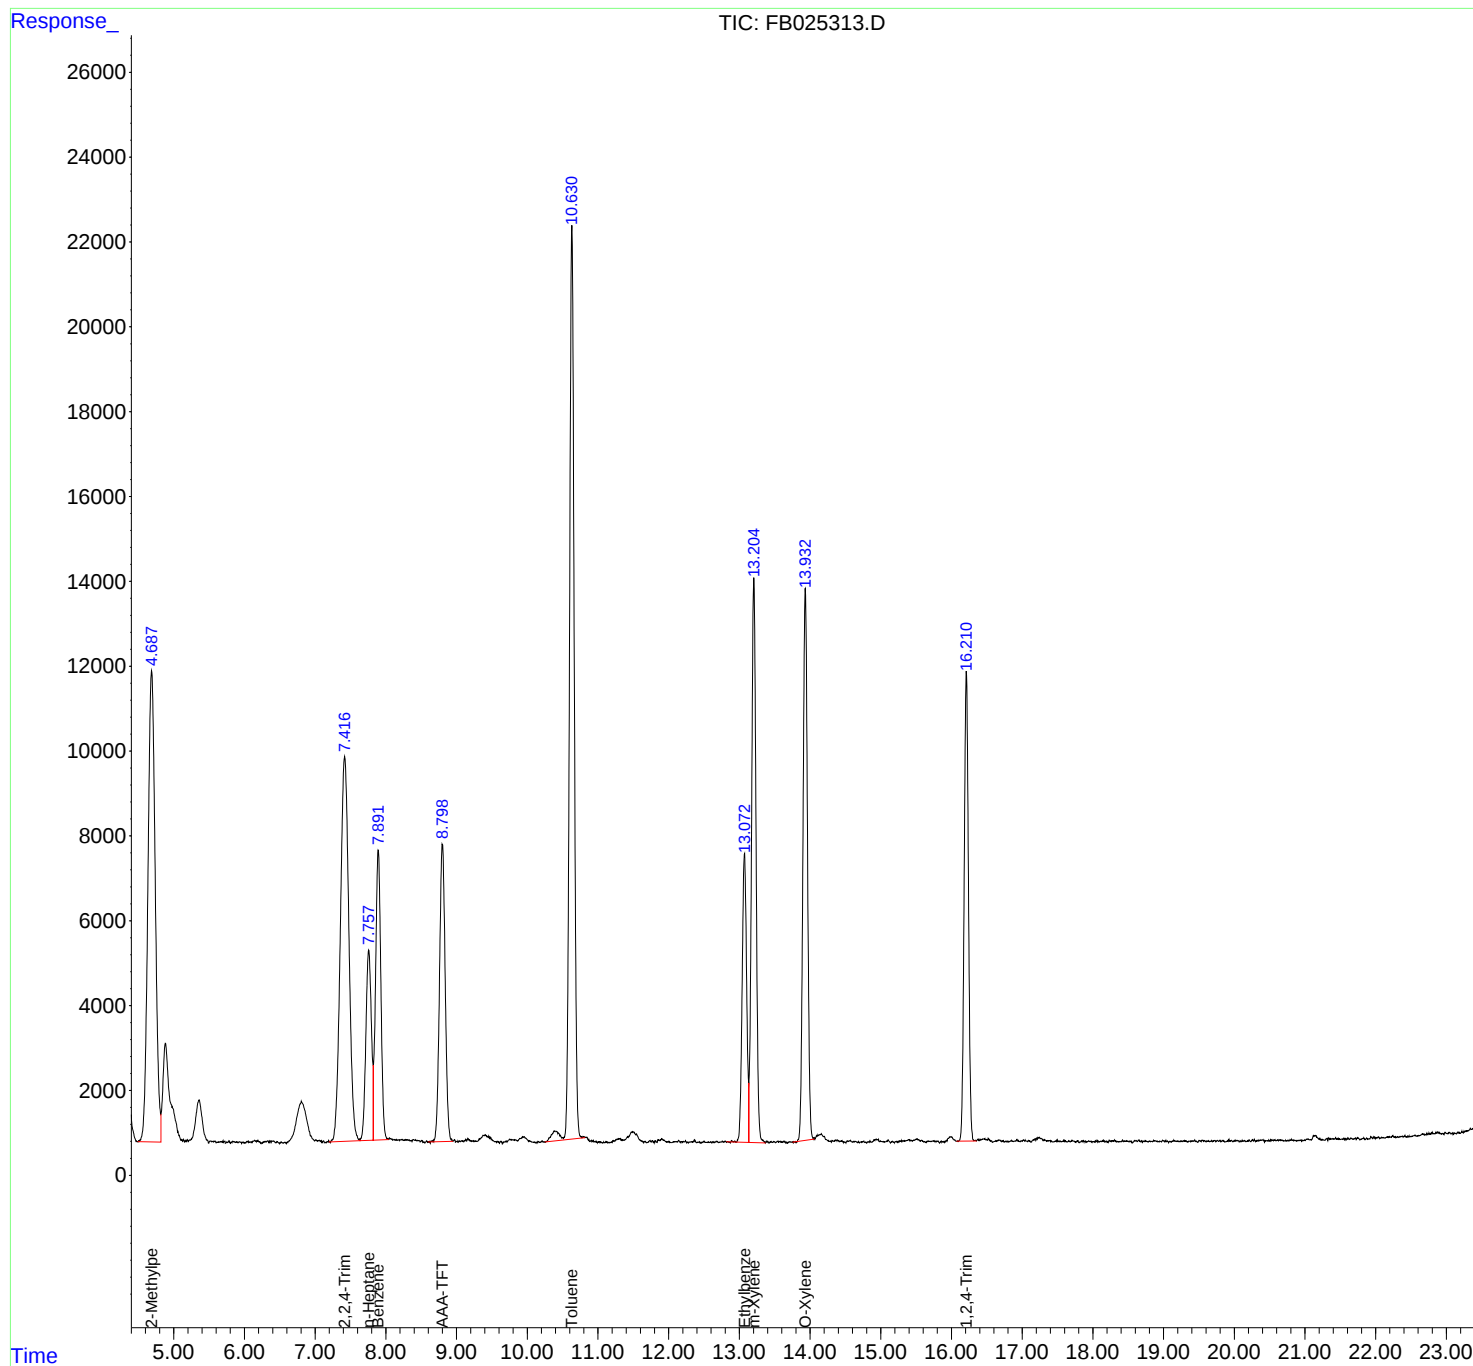


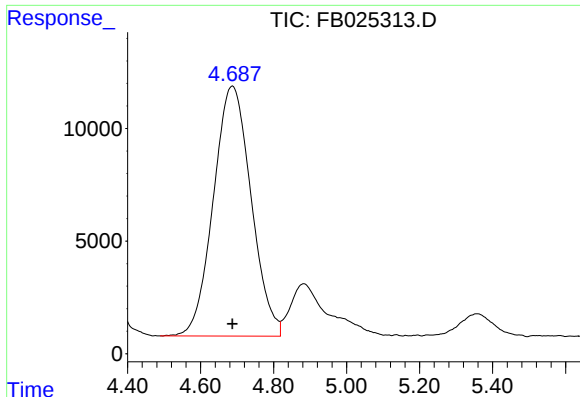

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 797112
Conc: 26.51 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B4-112320-0-2MSD

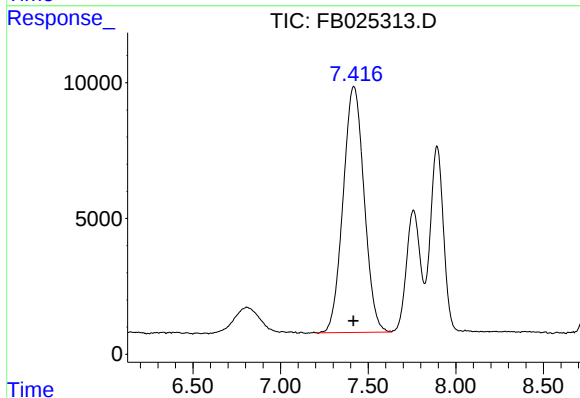


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 754644
Conc: 25.08 ng/ml

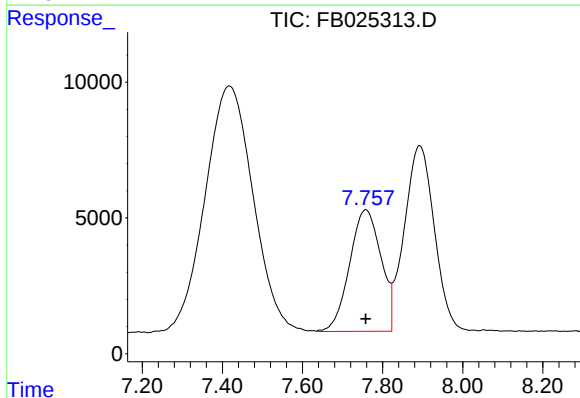


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 243382
Conc: 8.22 ng/ml

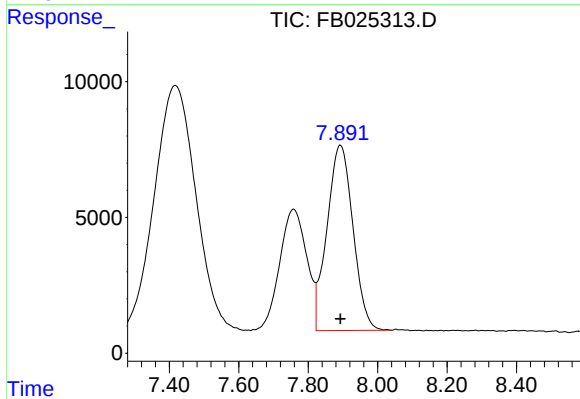

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 355479
Conc: 9.61 ng/ml

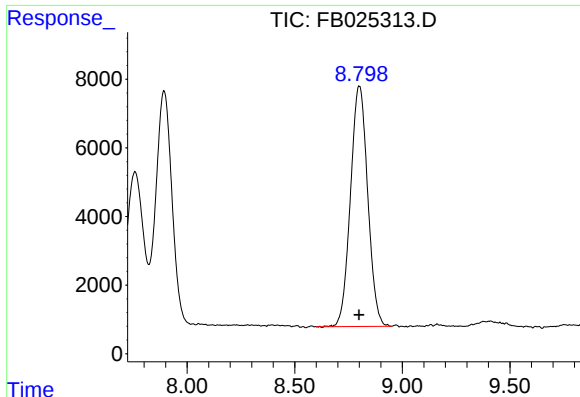

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.001 min
Response: 390250
Conc: 18.56 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B4-112320-0-2MSD

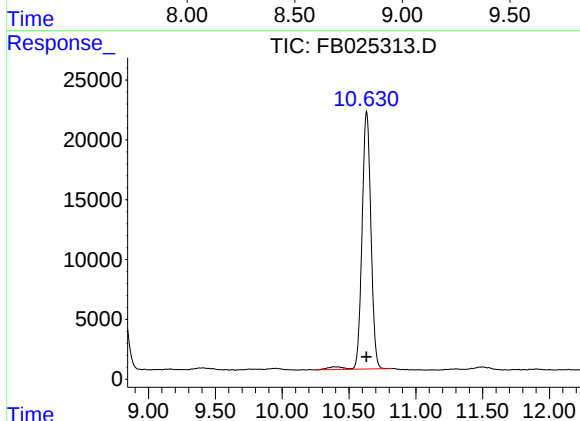


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.002 min
Response: 1002906
Conc: 28.54 ng/ml

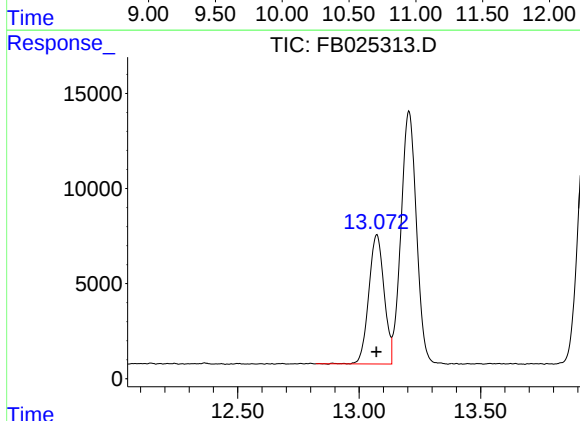


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.002 min
Response: 296515
Conc: 9.08 ng/ml

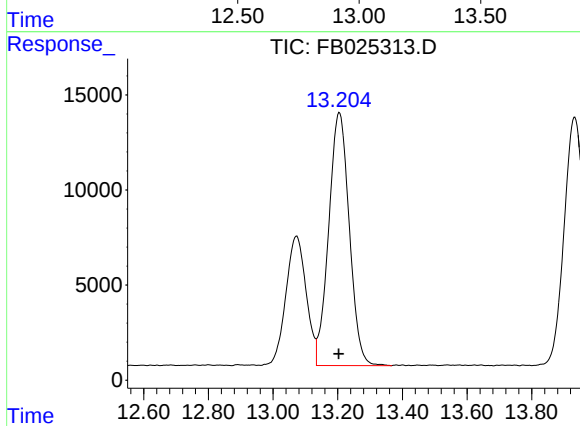

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.002 min
Response: 588878
Conc: 18.19 ng/ml

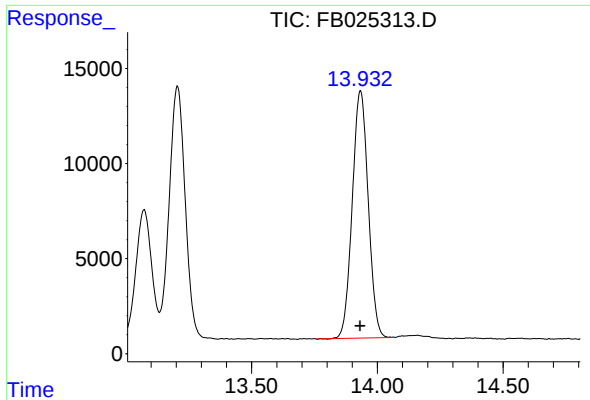

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.002 min
Response: 572941
Conc: 18.12 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B4-112320-0-2MSD

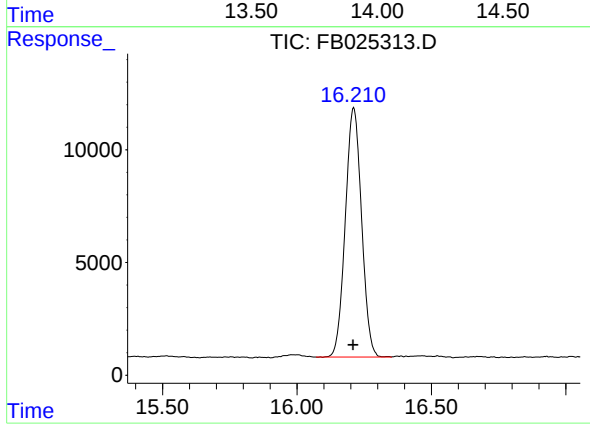

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.002 min
Response: 464399
Conc: 17.10 ng/ml