

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120920\
 Data File : FB025315.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2020 17:18
 Operator : DD/AJ
 Sample : BSF1209S2
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1209S2

Integration File: Calibration.e
 Quant Time: Dec 10 00:12:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	329321	15.665 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	722550	24.034 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	737050	24.495 ng/ml
3) t n-Heptane	7.759	241341	8.150 ng/ml
4) t Benzene	7.893	315884	8.540 ng/ml
6) t Toluene	10.632	908353	25.849 ng/ml
7) t Ethylbenzene	13.072	277295	8.489 ng/ml
8) t m-Xylene	13.205	553542	17.102 ng/ml
9) t O-Xylene	13.933	545011	17.240 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	468855	17.266 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120920\
Data File : FB025315.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2020 17:18
Operator : DD/AJ
Sample : BSF1209S2
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1209S2

Integration File: Calibration.e
Quant Time: Dec 10 00:12:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

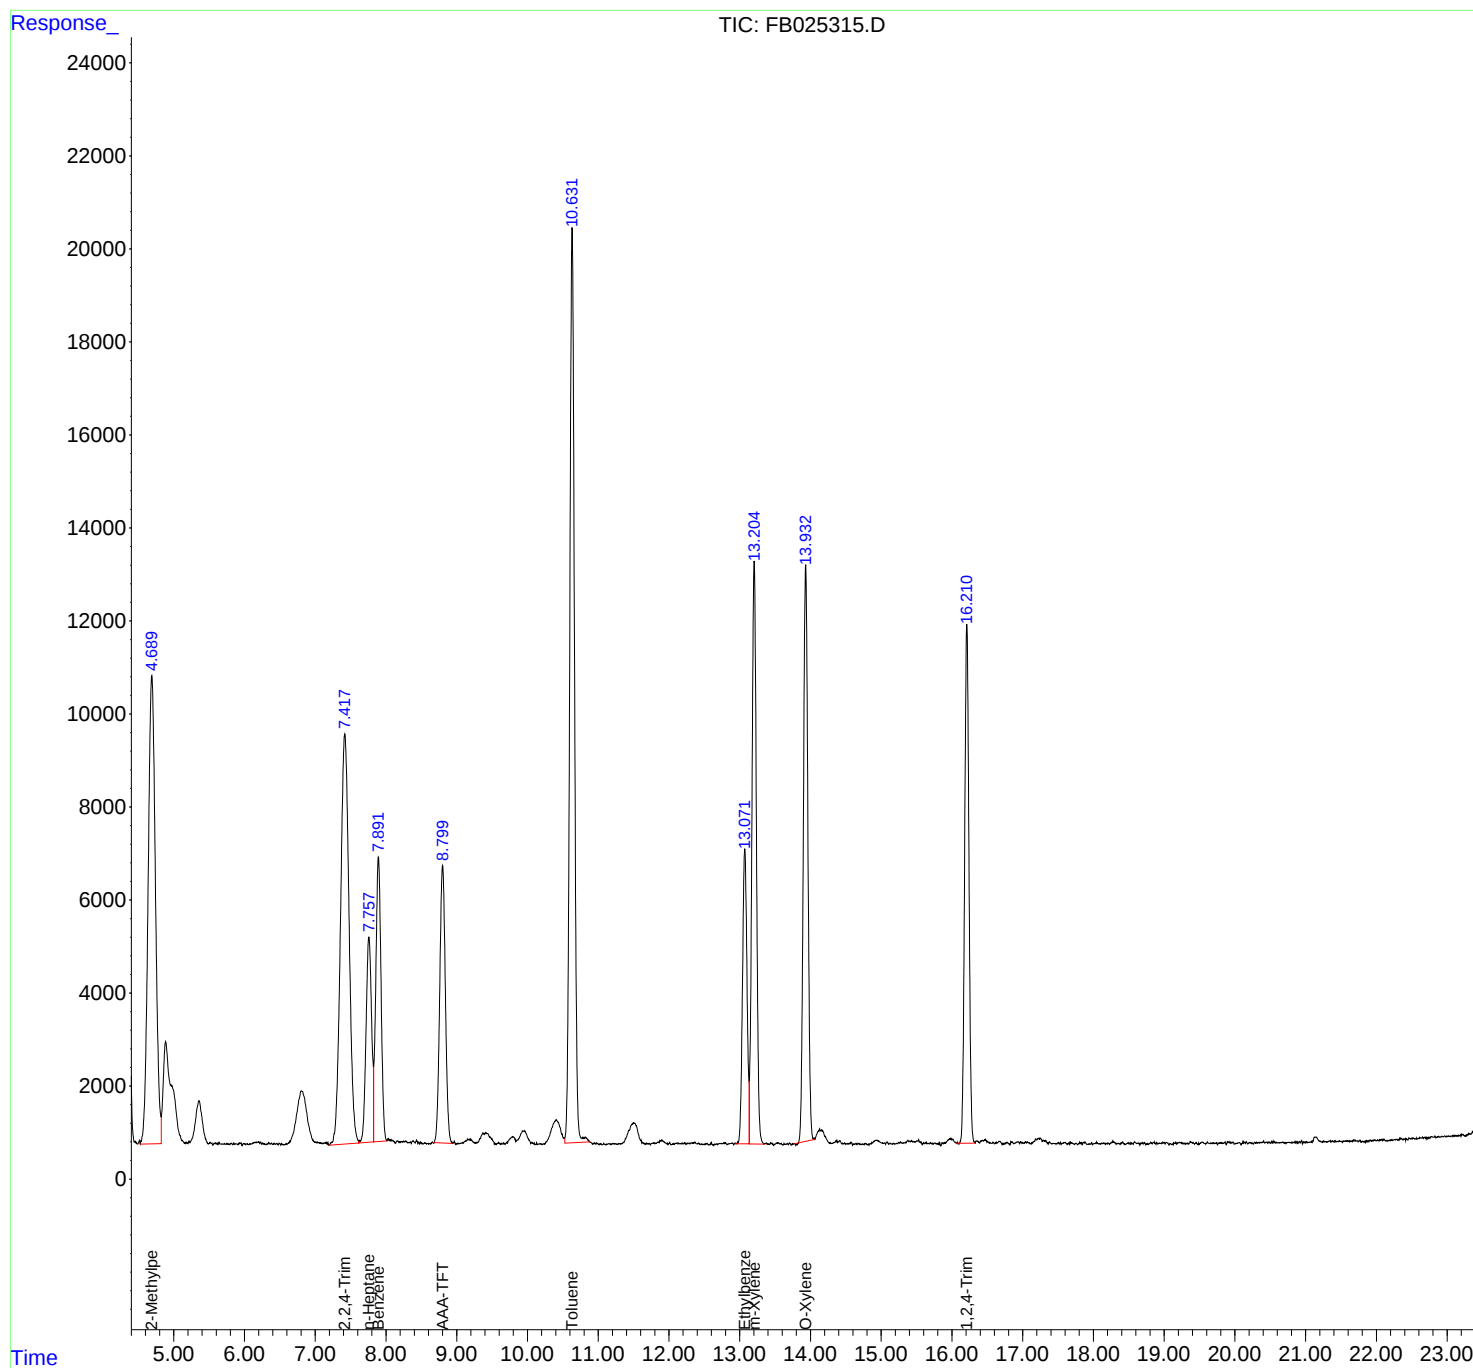


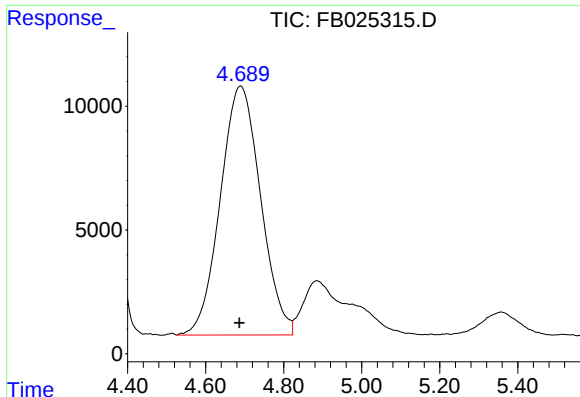

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.004 min
Response: 722550
Conc: 24.03 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1209S2

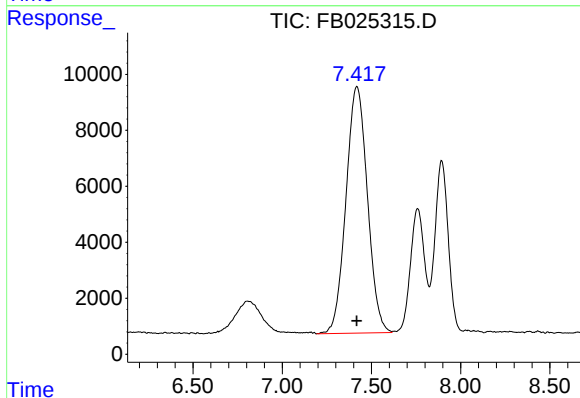


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.002 min
Response: 737050
Conc: 24.50 ng/ml

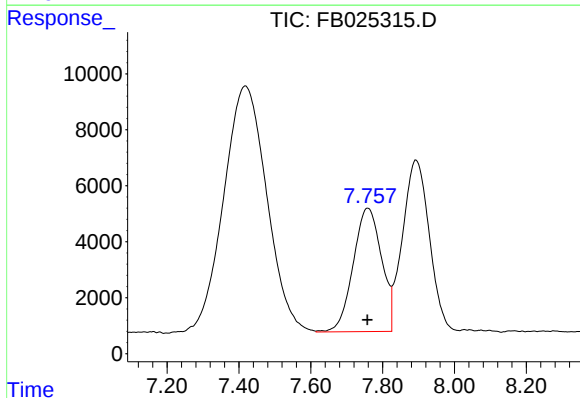


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.001 min
Response: 241341
Conc: 8.15 ng/ml

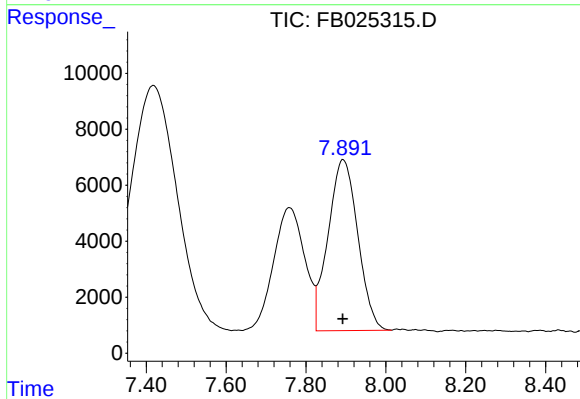

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 315884
Conc: 8.54 ng/ml

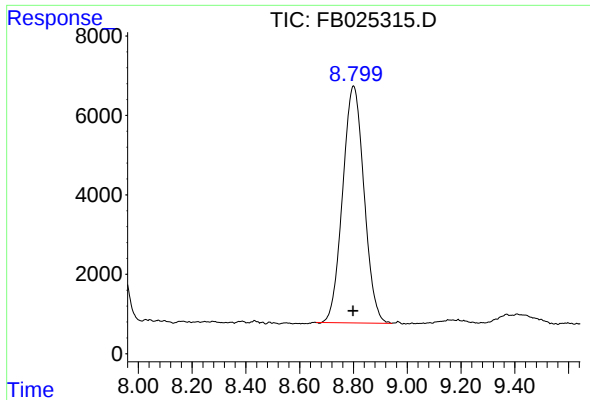

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.002 min
Response: 329321
Conc: 15.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1209S2

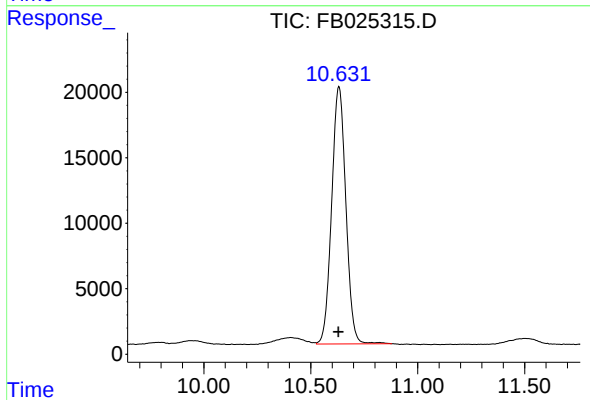


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.002 min
Response: 908353
Conc: 25.85 ng/ml

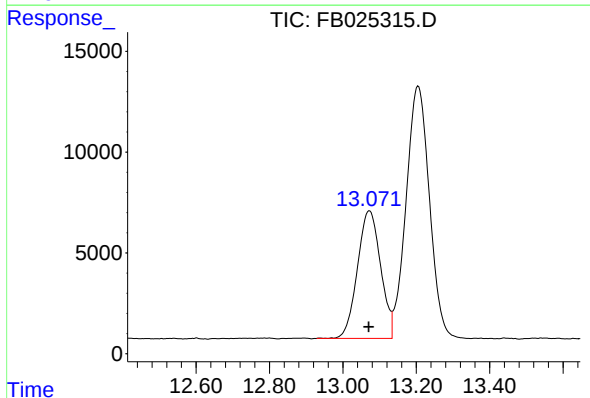


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.002 min
Response: 277295
Conc: 8.49 ng/ml

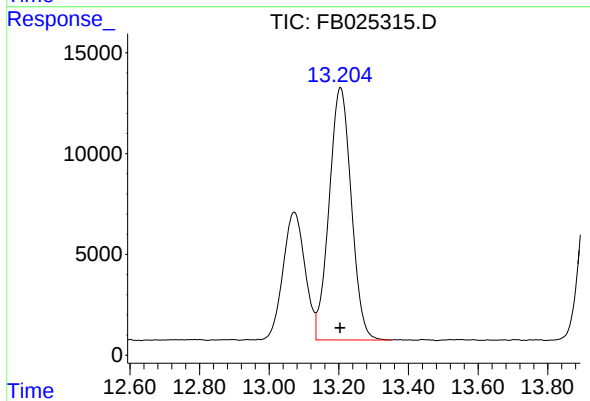

#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.002 min
Response: 553542
Conc: 17.10 ng/ml

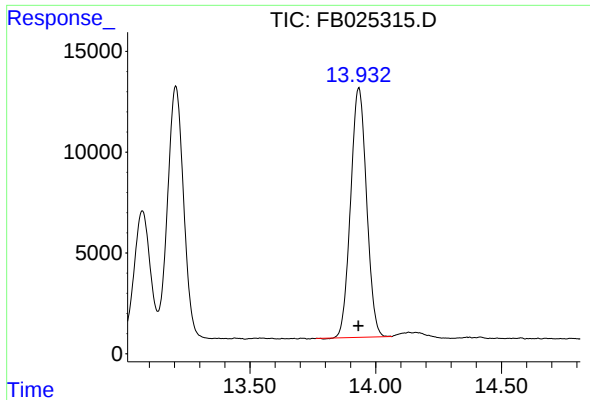

#9 O-Xylene


R.T.: 13.933 min

Delta R.T.: 0.002 min

Response: 545011

Conc: 17.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1209S2

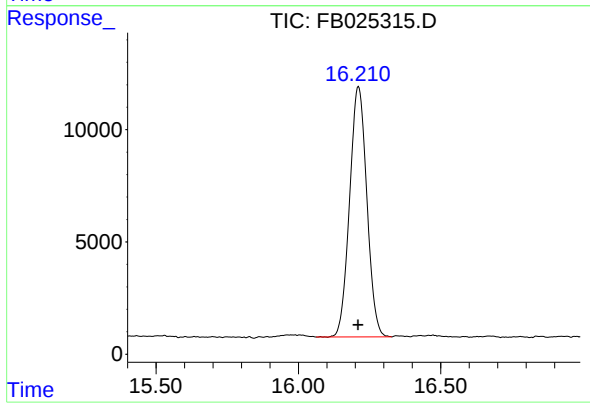

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min

Delta R.T.: 0.002 min

Response: 468855

Conc: 17.27 ng/ml