

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120924\
 Data File : FB031275.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2024 10:50
 Operator : YP/AJ
 Sample : VBF1209S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 10 00:47:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
 Quant Title :
 QLast Update : Thu Nov 21 12:34:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	444288	15.784 ng/ml
Target Compounds			
6) t Toluene	10.601	920	0.018 ng/ml
8) t m-Xylene	13.180	5581	0.118 ng/ml
9) t O-Xylene	13.905	6552	0.150 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	8310	0.233 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120924\
Data File : FB031275.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2024 10:50
Operator : YP/AJ
Sample : VBF1209S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 10 00:47:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
Quant Title :
QLast Update : Thu Nov 21 12:34:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

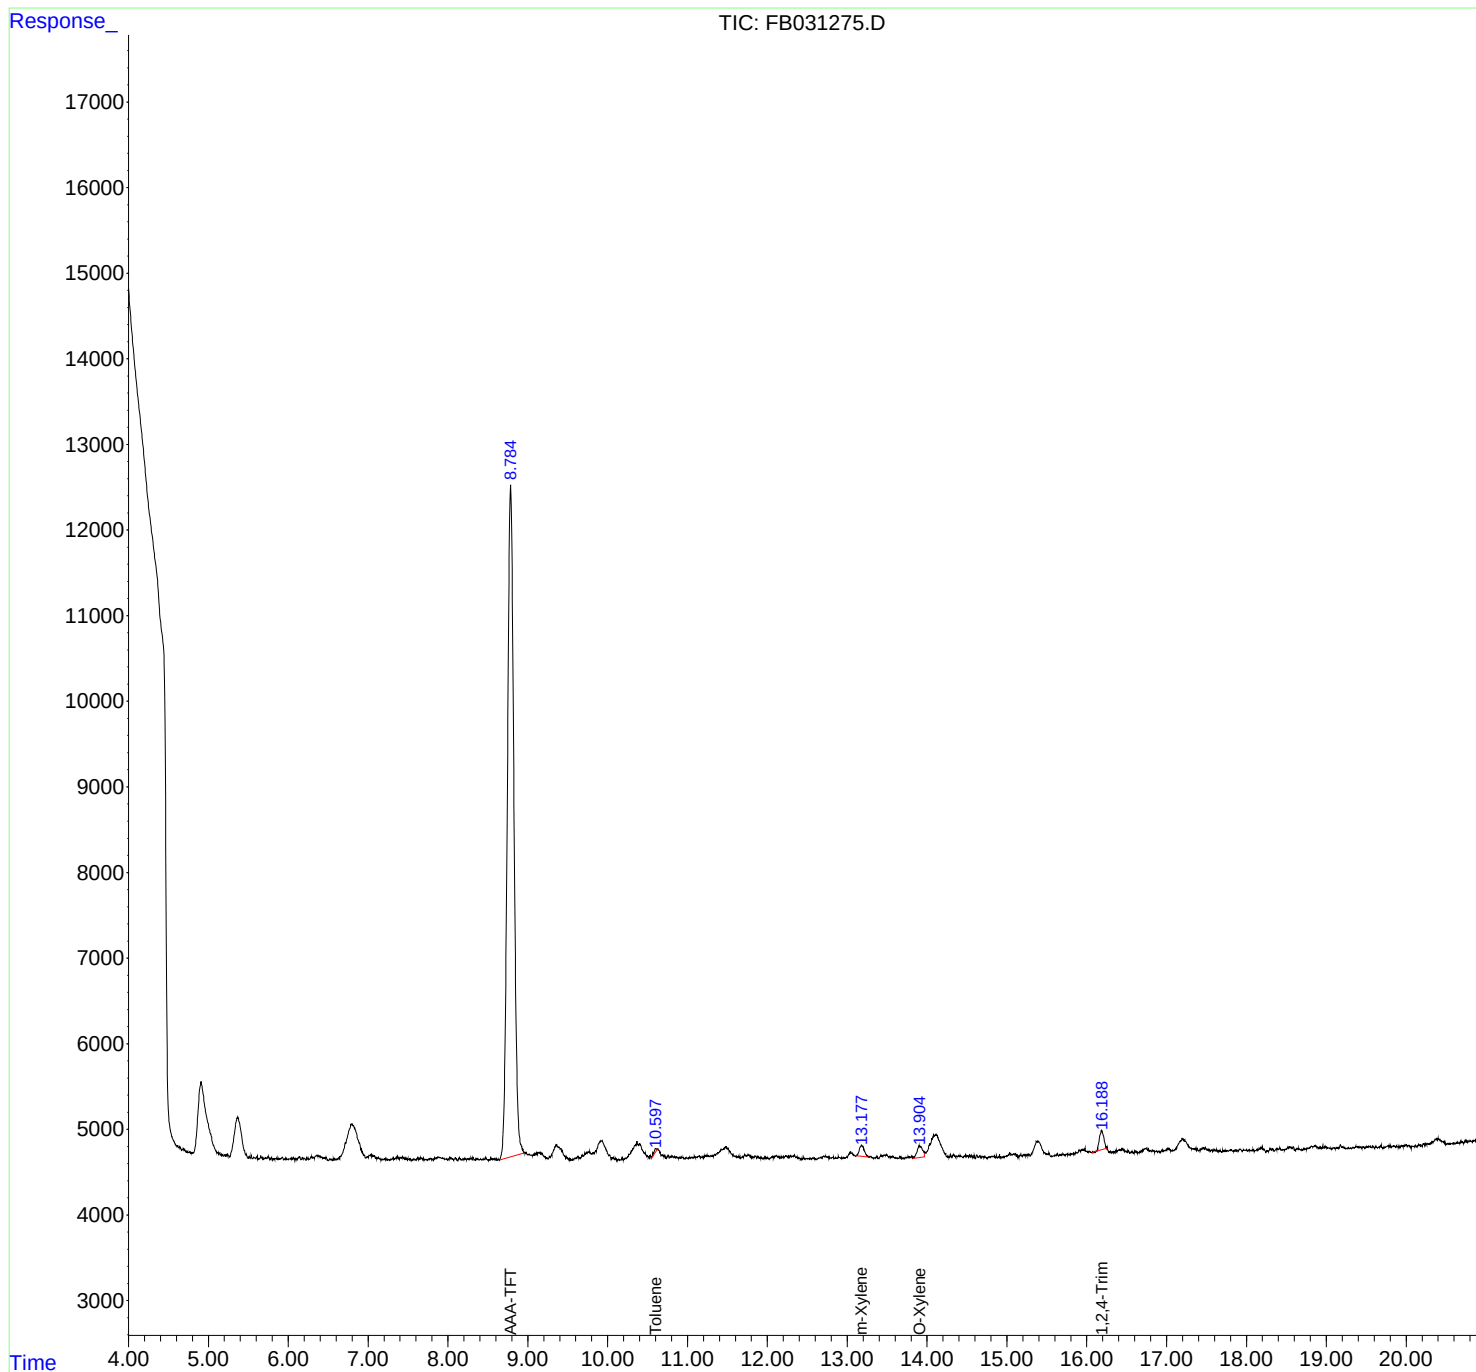


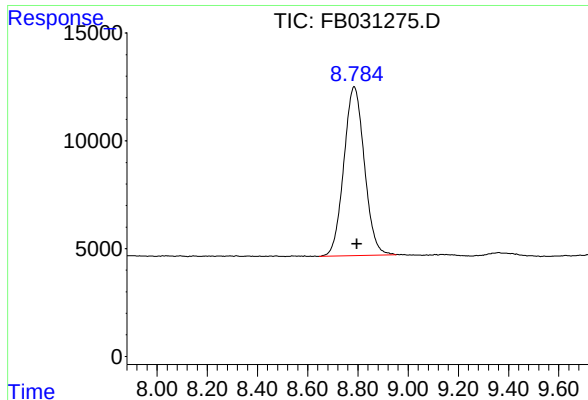

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.011 min
Response: 444288
Conc: 15.78 ng/ml

Instrument :
FID_B
ClientSampleId :

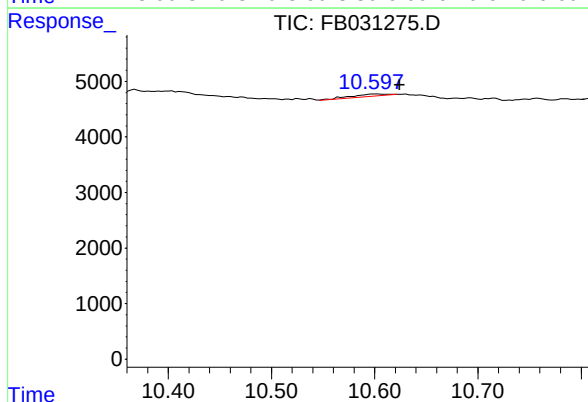


#6 Toluene

R.T.: 10.601 min
Delta R.T.: -0.023 min
Response: 920
Conc: 0.02 ng/ml

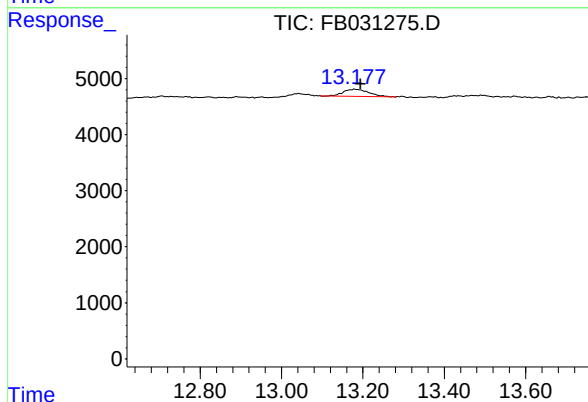


#8 m-Xylene

R.T.: 13.180 min
Delta R.T.: -0.015 min
Response: 5581
Conc: 0.12 ng/ml

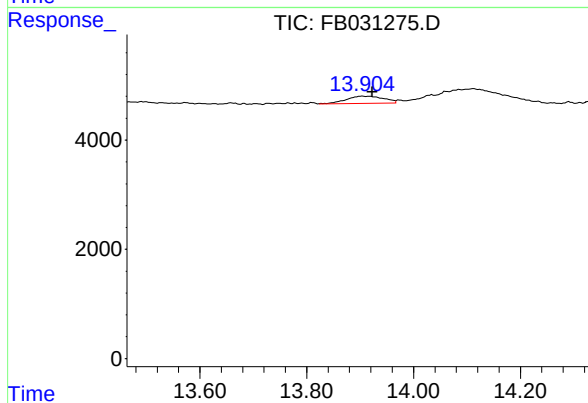

#9 O-Xylene

R.T.: 13.905 min
Delta R.T.: -0.017 min
Response: 6552
Conc: 0.15 ng/ml

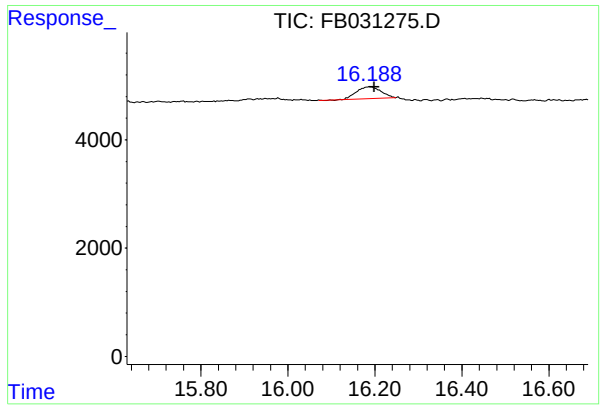

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min

Delta R.T.: -0.010 min

Response: 8310

Conc: 0.23 ng/ml

Instrument :

FID_B

ClientSampleId :