

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120924\
 Data File : FB031277.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2024 11:43
 Operator : YP/AJ
 Sample : BSF1209S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 10 00:47:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
 Quant Title :
 QLast Update : Thu Nov 21 12:34:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	555024	19.719 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	869864	22.057 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1078704	22.811 ng/ml
3) t n-Heptane	7.751	329205	7.049 ng/ml
4) t Benzene	7.890	399625	7.373 ng/ml
6) t Toluene	10.617	1118711	22.371 ng/ml
7) t Ethylbenzene	13.053	325400	7.417 ng/ml
8) t m-Xylene	13.186	696309	14.769 ng/ml
9) t O-Xylene	13.914	648761	14.896 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	527443	14.776 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120924\
Data File : FB031277.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2024 11:43
Operator : YP/AJ
Sample : BSF1209S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 10 00:47:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112124.M
Quant Title :
QLast Update : Thu Nov 21 12:34:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

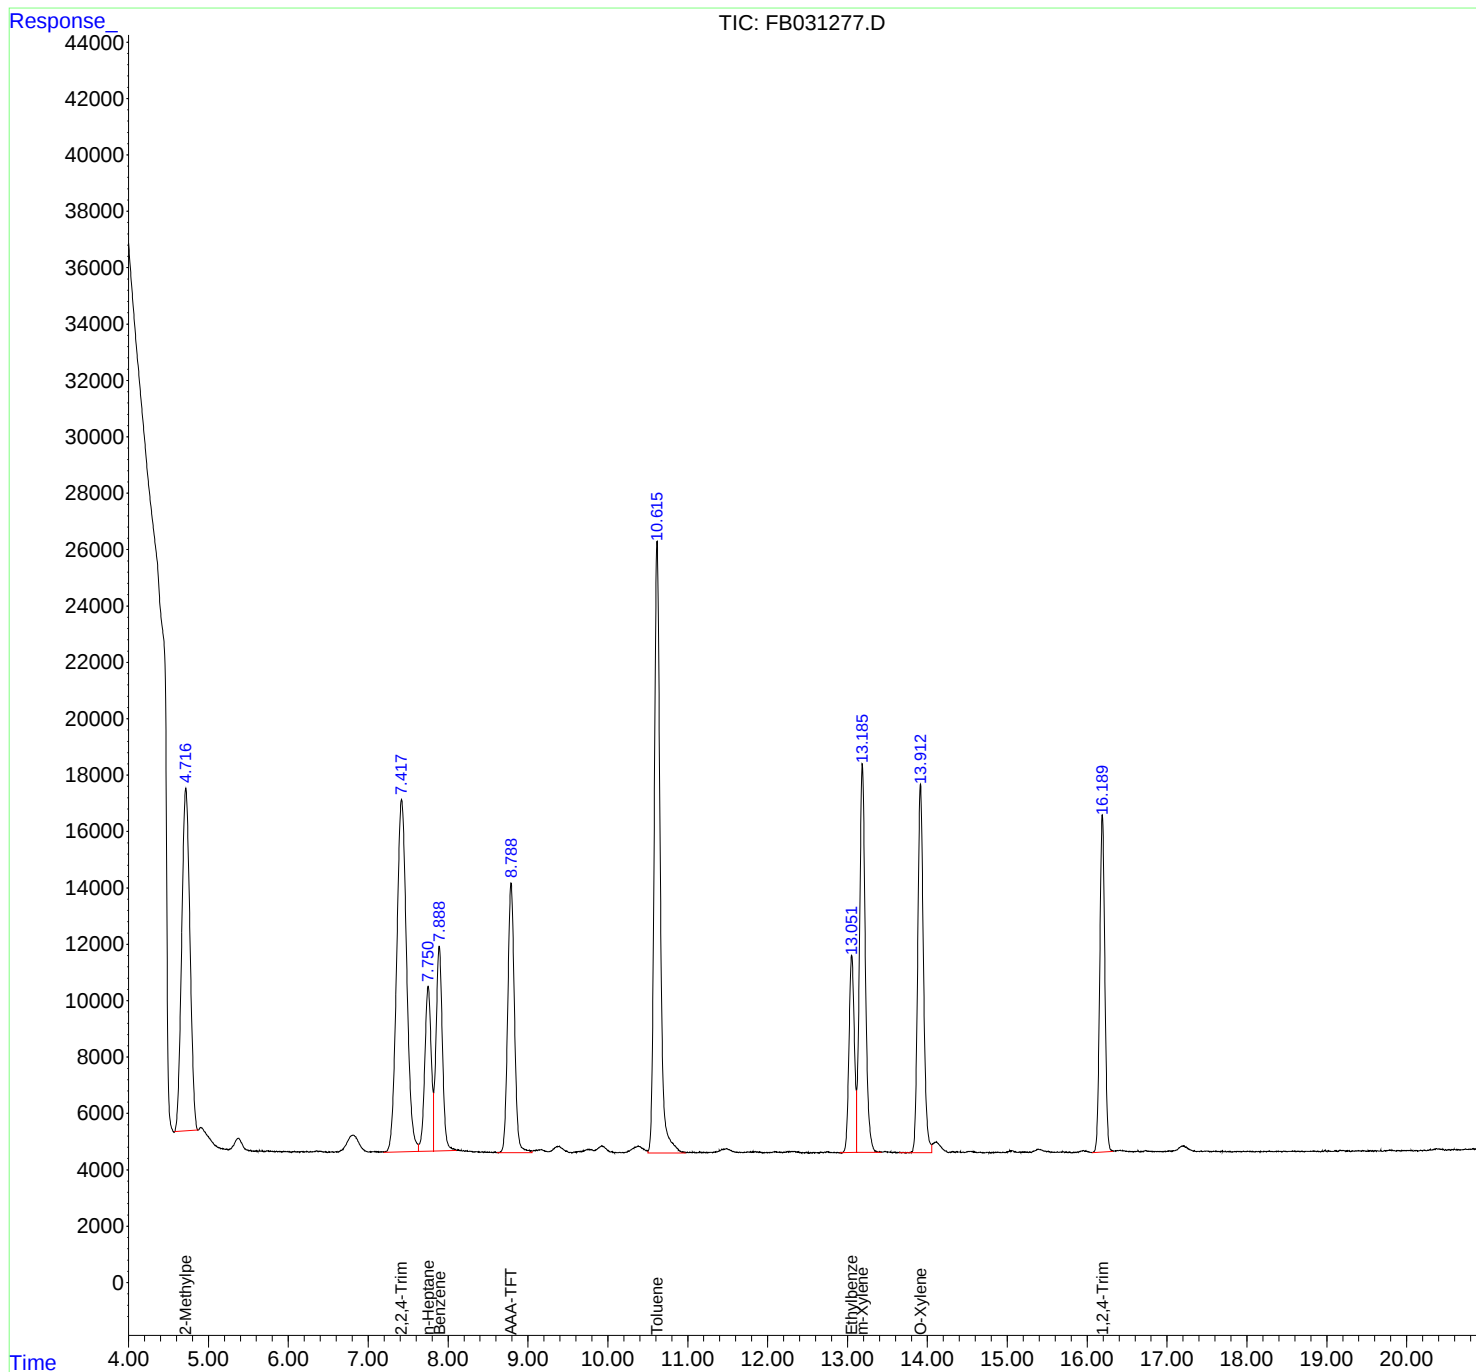

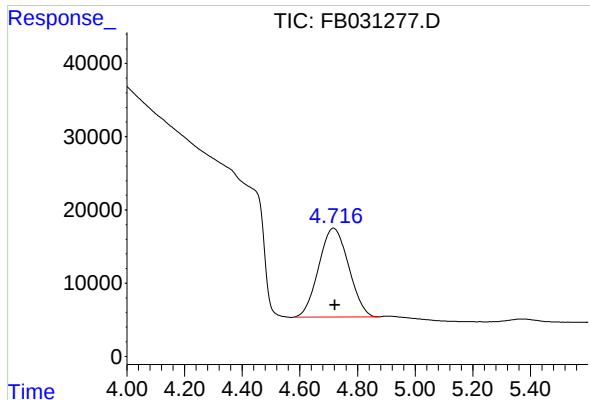


#1 2-Methylpentane

R.T.: 4.718 min
Delta R.T.: -0.004 min
Response: 869864
Conc: 22.06 ng/ml


Instrument : FID_B

ClientSampleId :

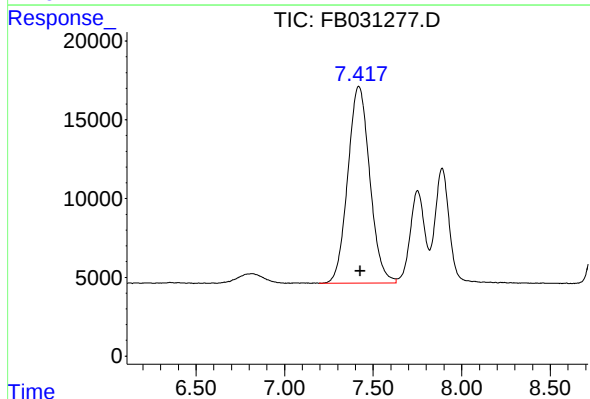


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.009 min
Response: 1078704
Conc: 22.81 ng/ml

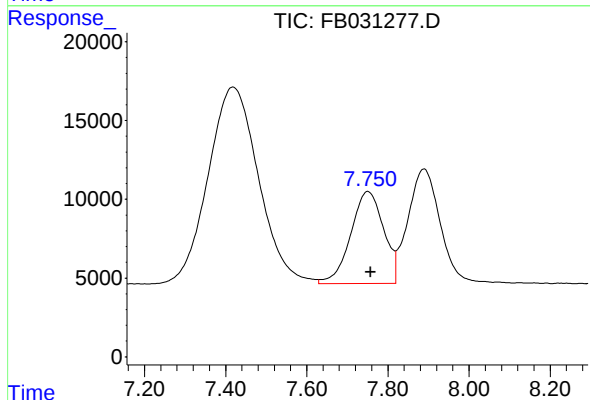


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.006 min
Response: 329205
Conc: 7.05 ng/ml

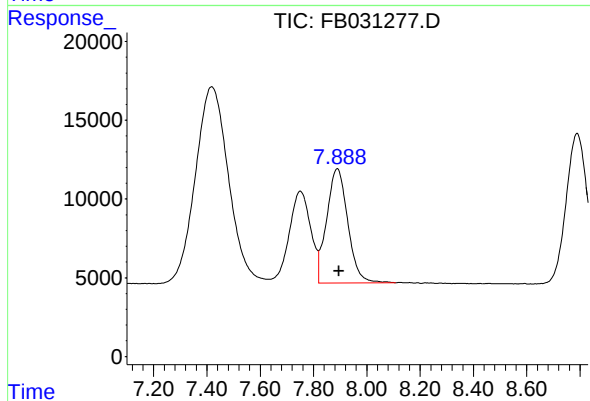

#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.006 min
Response: 399625
Conc: 7.37 ng/ml

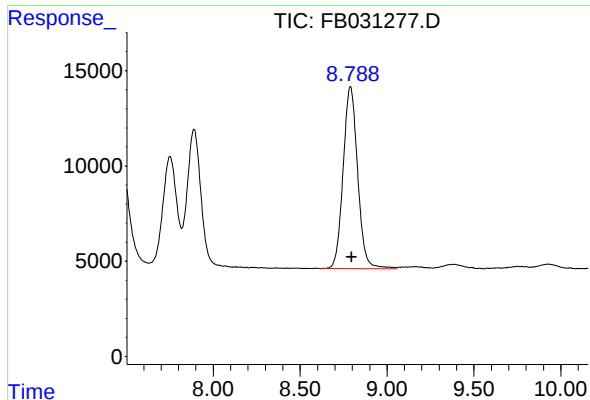


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: -0.007 min
Response: 555024
Conc: 19.72 ng/ml

Instrument :


FID_B

ClientSampleId :

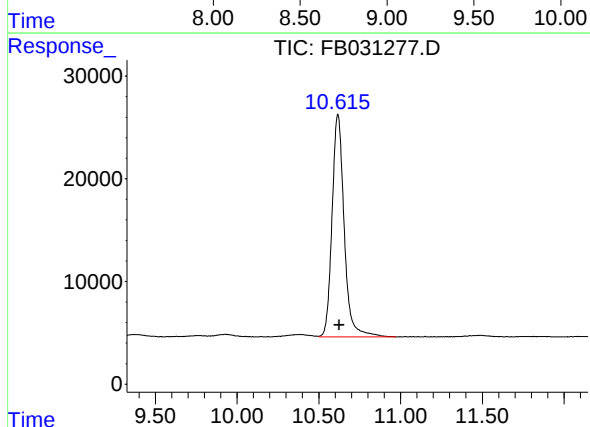


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.008 min
Response: 1118711
Conc: 22.37 ng/ml

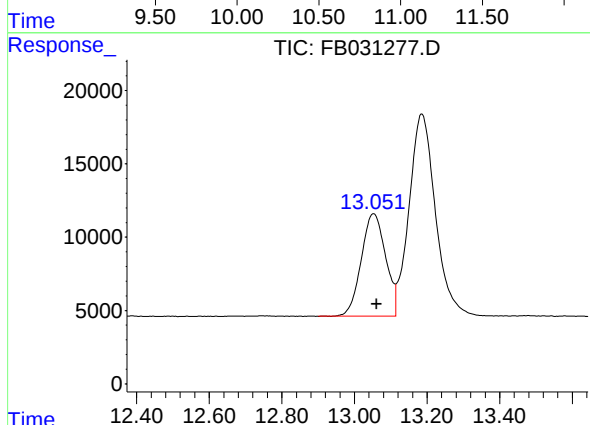


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.008 min
Response: 325400
Conc: 7.42 ng/ml

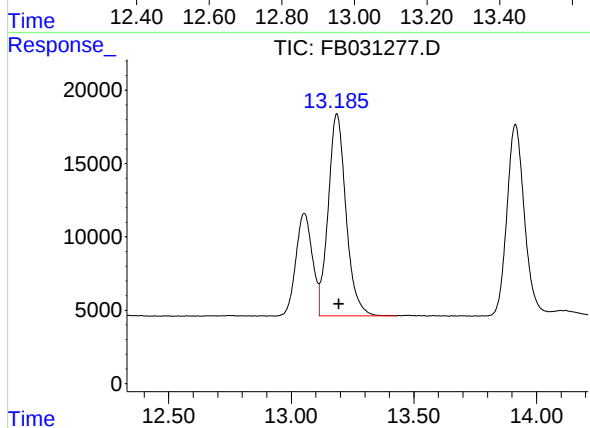

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.008 min
Response: 696309
Conc: 14.77 ng/ml

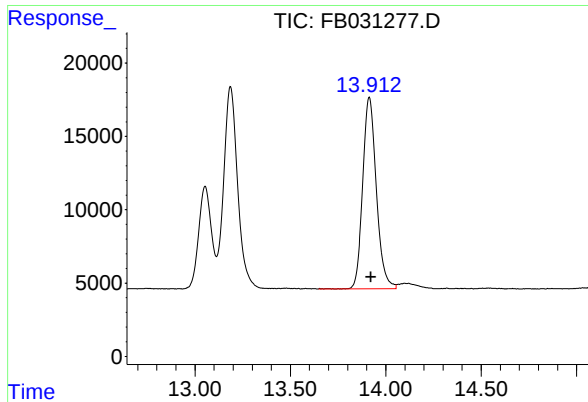

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.009 min
Response: 648761
Conc: 14.90 ng/ml

Instrument :
FID_B
ClientSampleId :

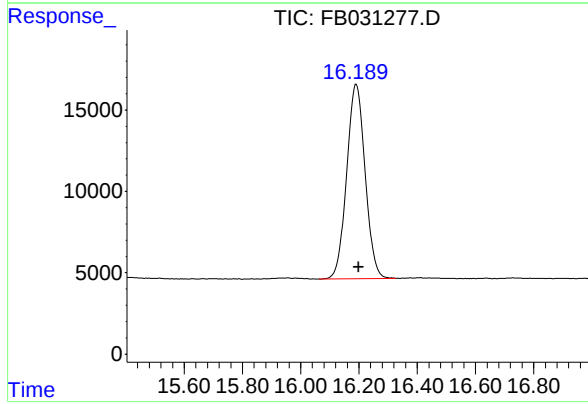

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.009 min
Response: 527443
Conc: 14.78 ng/ml