

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032417.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 10:37
Operator : YP/AJ
Sample : VBF1209S1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 10 00:39:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	430824	19.123 ng/ml
Target Compounds			
6) t Toluene	10.620	8608	0.188 ng/ml
8) t m-Xylene	13.190	9083	0.211 ng/ml
9) t O-Xylene	13.917	9660	0.233 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	30712	0.873 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032417.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 10:37
Operator : YP/AJ
Sample : VBF1209S1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 10 00:39:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

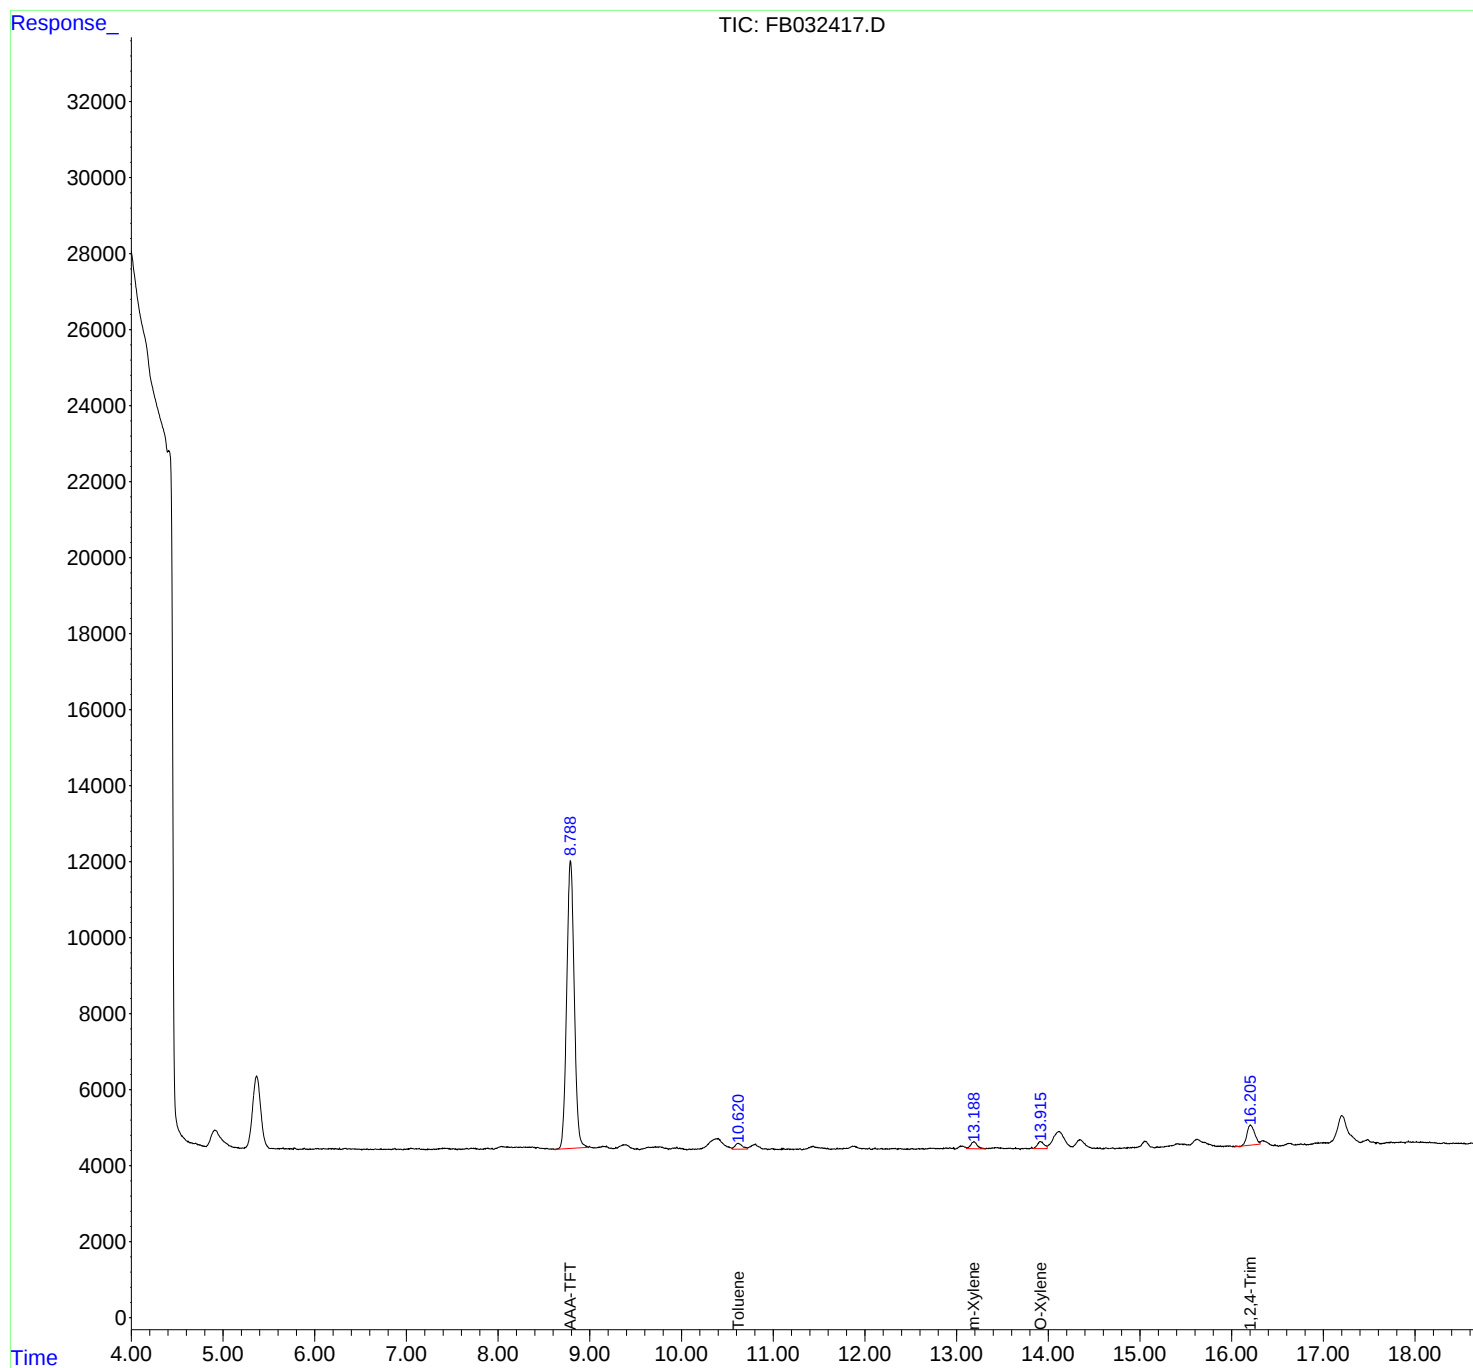


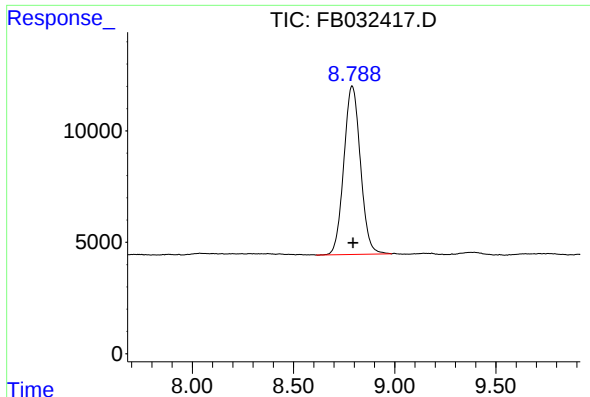

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.005 min
Response: 430824
Conc: 19.12 ng/ml

Instrument :
FID_B
ClientSampleId :

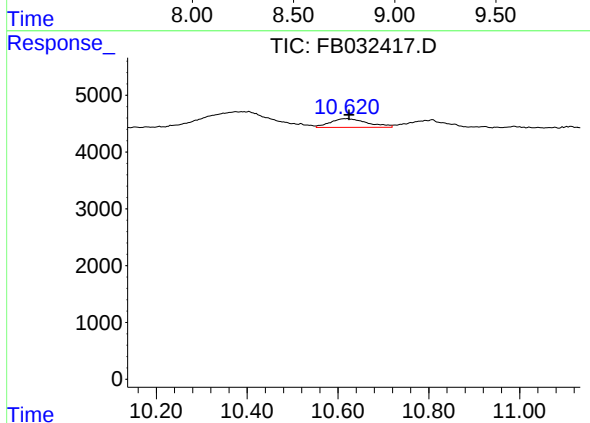


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.004 min
Response: 8608
Conc: 0.19 ng/ml

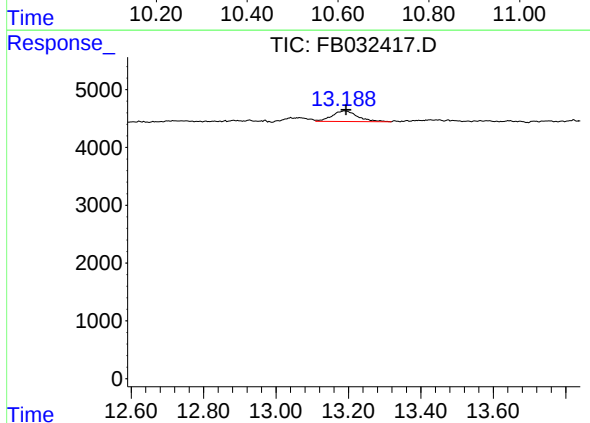


#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: -0.004 min
Response: 9083
Conc: 0.21 ng/ml

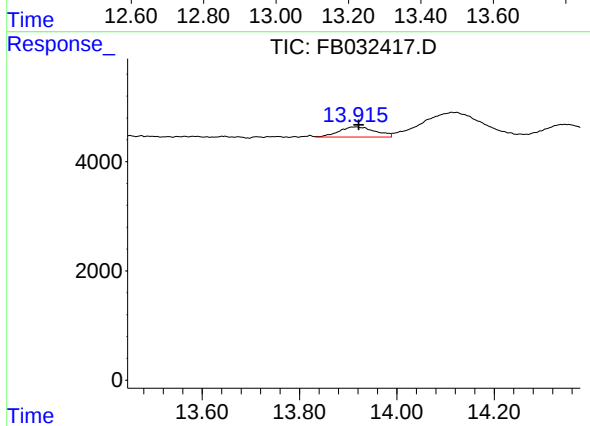

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.005 min
Response: 9660
Conc: 0.23 ng/ml

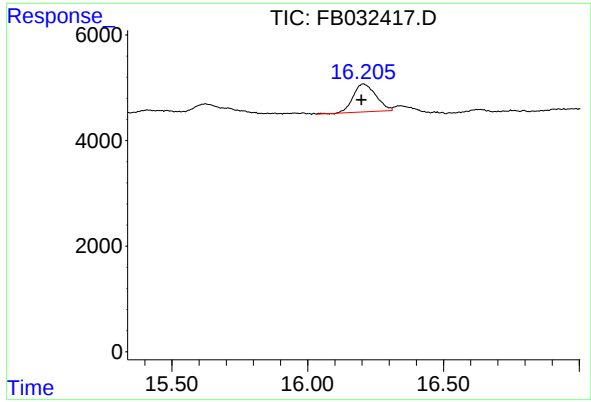

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.008 min
Response: 30712
Conc: 0.87 ng/ml

Instrument :
FID_B
ClientSampleId :