

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
 Data File : FB032420.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2025 12:25
 Operator : YP/AJ
 Sample : Q3741-05 50X
 Misc : 5.43G/5.00 ML MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 10 00:39:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Quant Title :
 QLast Update : Fri Dec 05 17:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	564270	25.046 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.379	25034	0.626 ng/ml
3) t n-Heptane	7.749	25204	0.638 ng/ml
4) t Benzene	7.890	21052	0.468 ng/ml
6) t Toluene	10.624	113708	2.489 ng/ml
7) t Ethylbenzene	13.059	76435	1.877 ng/ml
8) t m-Xylene	13.191	272136	6.320 ng/ml
9) t O-Xylene	13.922	98265	2.374 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	340757	9.681 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032420.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 12:25
Operator : YP/AJ
Sample : Q3741-05 50X
Misc : 5.43G/5.00 ML MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 10 00:39:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

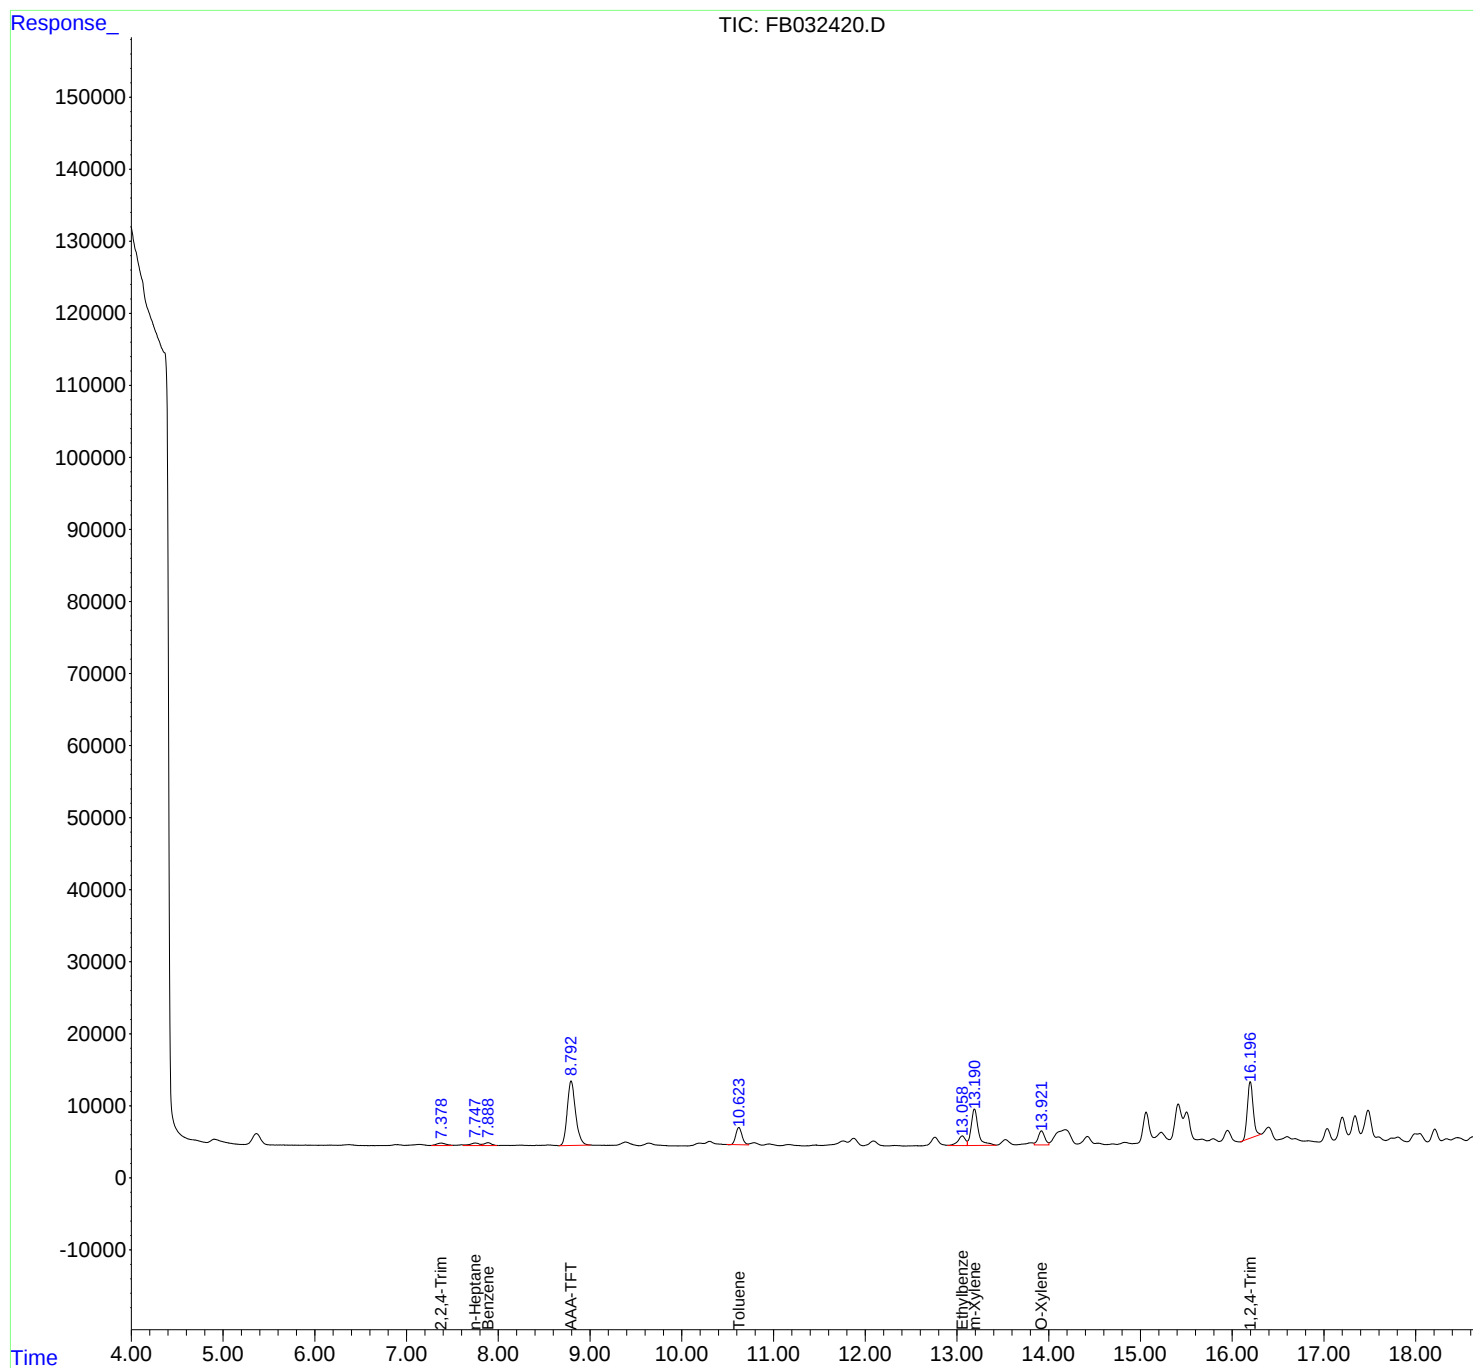


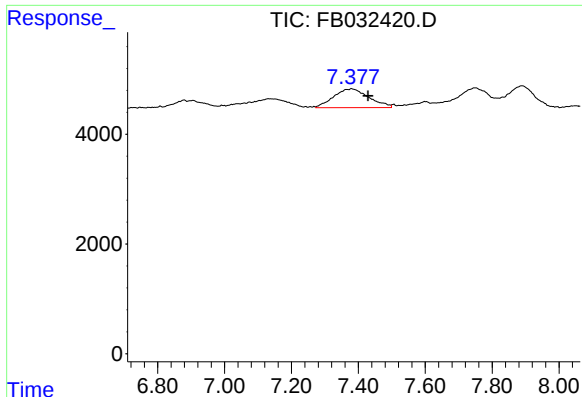

#2 2,2,4-Trimethylpentane


R.T.: 7.379 min
Delta R.T.: -0.050 min
Response: 25034
Conc: 0.63 ng/ml

Instrument :
FID_B
ClientSampleId :

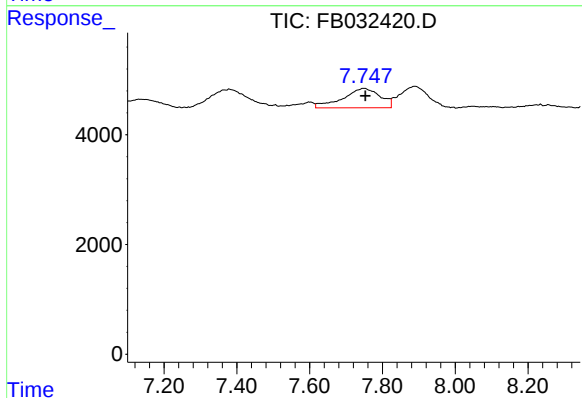


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.004 min
Response: 25204
Conc: 0.64 ng/ml

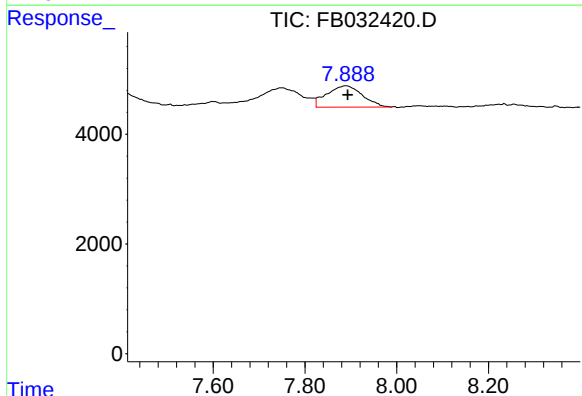


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 21052
Conc: 0.47 ng/ml

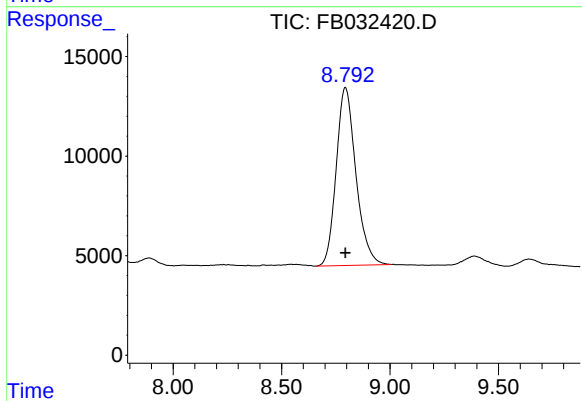

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 564270
Conc: 25.05 ng/ml

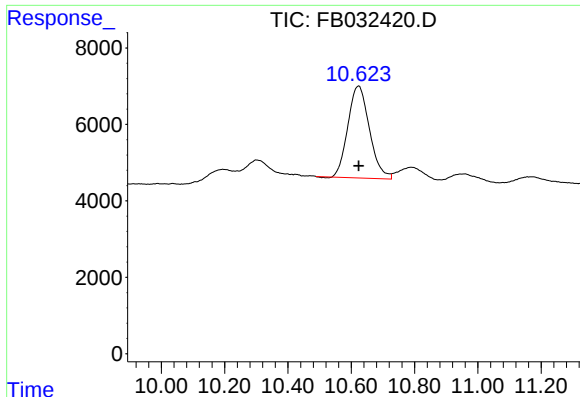

#6 Toluene


R.T.: 10.624 min
Delta R.T.: 0.000 min
Response: 113708
Conc: 2.49 ng/ml

Instrument :
FID_B
ClientSampleId :

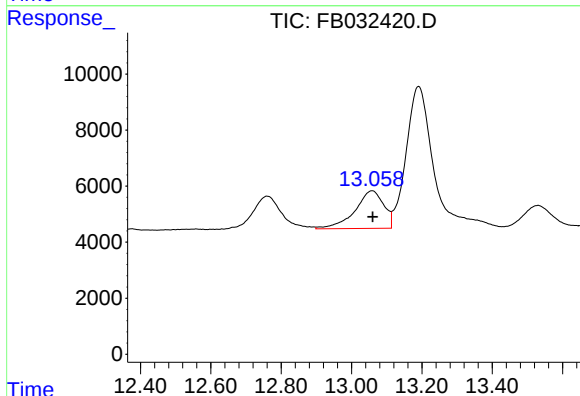


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: -0.001 min
Response: 76435
Conc: 1.88 ng/ml

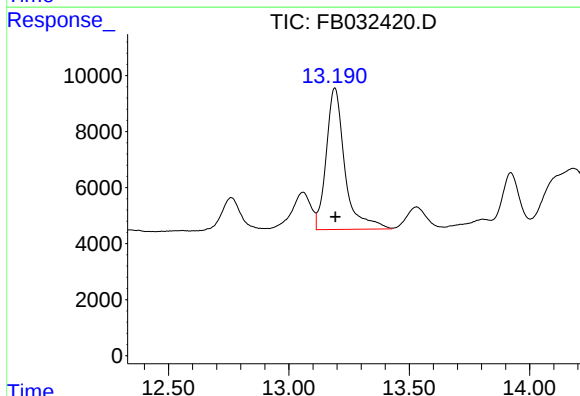


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: -0.003 min
Response: 272136
Conc: 6.32 ng/ml

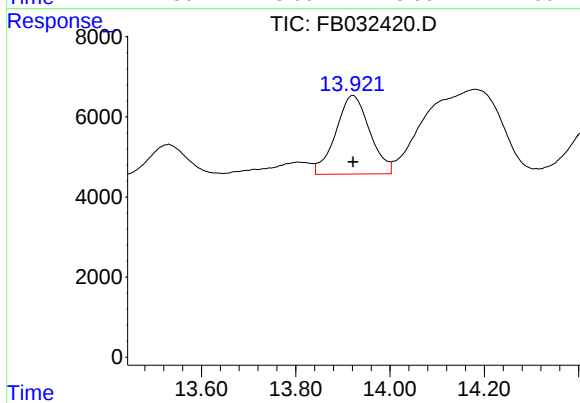

#9 o-Xylene

R.T.: 13.922 min
Delta R.T.: 0.000 min
Response: 98265
Conc: 2.37 ng/ml

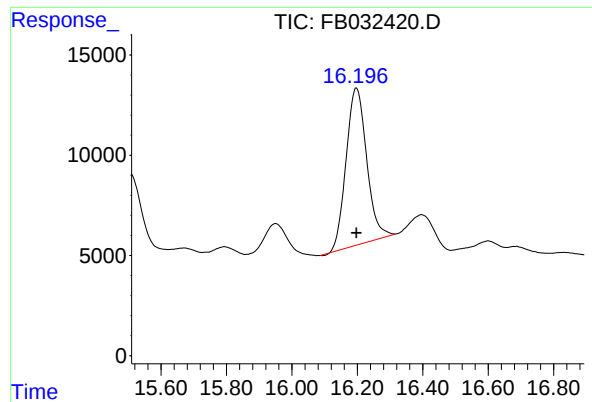

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.000 min
Response: 340757
Conc: 9.68 ng/ml

Instrument :

FID_B

ClientSampleId :