

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
 Data File : FB032421.D
 Signal(s) : FID2B.CH
 Acq On : 9 Dec 2025 13:16
 Operator : YP/AJ
 Sample : BSF1209S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1209S2

Integration File: Calibration.e
 Quant Time: Dec 10 00:39:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
 Quant Title :
 QLast Update : Fri Dec 05 17:59:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	484856	21.521 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	973028	28.045 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	1181119	29.526 ng/ml
3) t n-Heptane	7.753	386821	9.790 ng/ml
4) t Benzene	7.893	462897	10.282 ng/ml
6) t Toluene	10.622	1375187	30.100 ng/ml
7) t Ethylbenzene	13.059	403417	9.905 ng/ml
8) t m-Xylene	13.192	852790	19.803 ng/ml
9) t O-Xylene	13.920	804629	19.436 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	692789	19.683 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB120925\
Data File : FB032421.D
Signal(s) : FID2B.CH
Acq On : 9 Dec 2025 13:16
Operator : YP/AJ
Sample : BSF1209S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1209S2

Integration File: Calibration.e
Quant Time: Dec 10 00:39:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

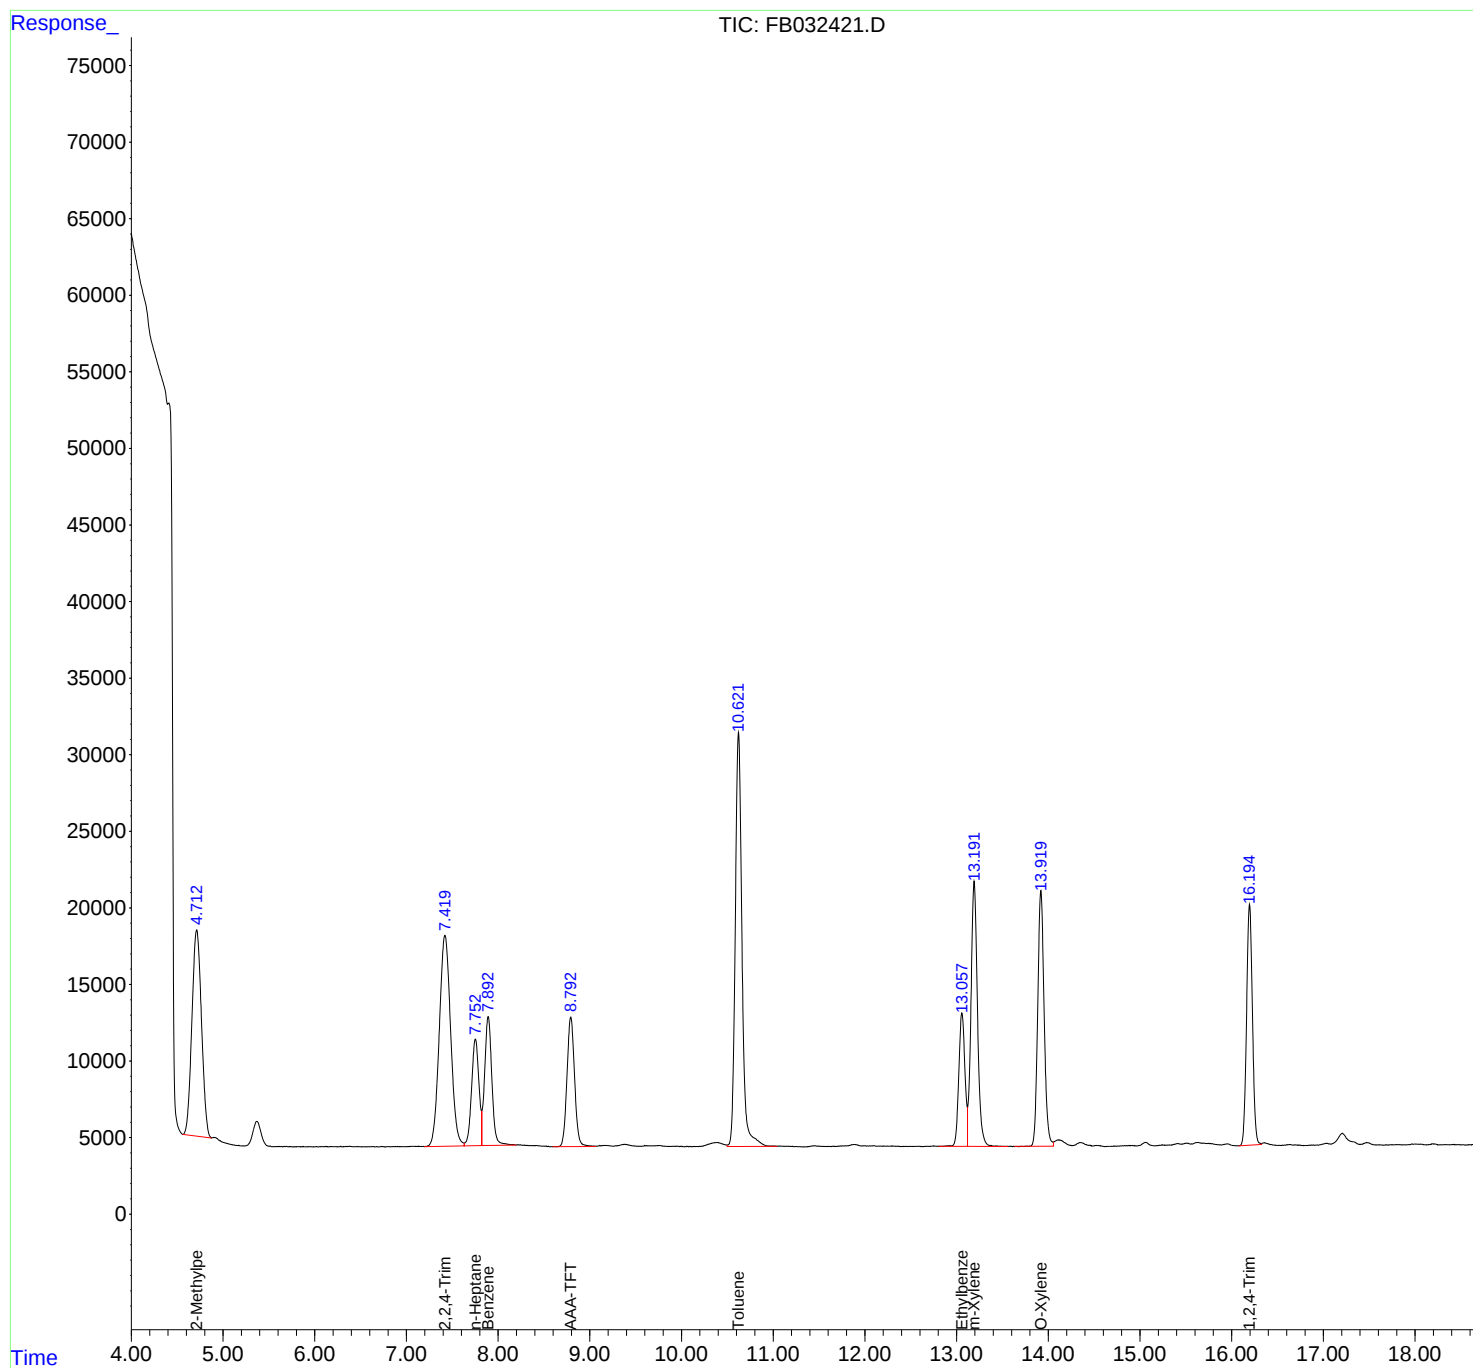


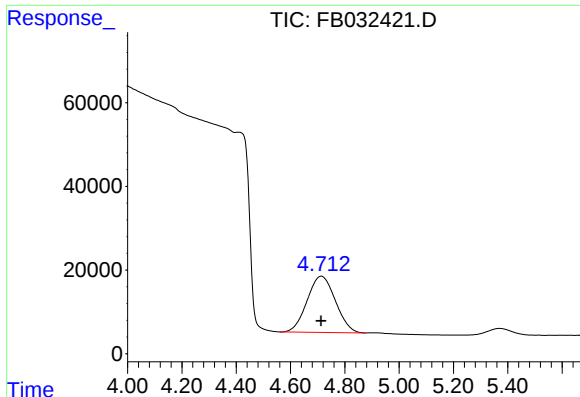

#1 2-Methylpentane


R.T.: 4.714 min
Delta R.T.: 0.002 min
Response: 973028
Conc: 28.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1209S2

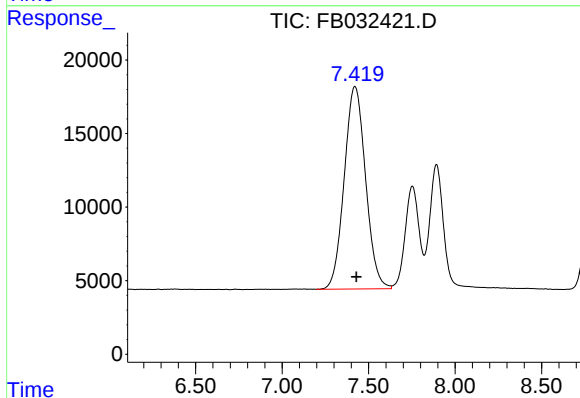


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: -0.008 min
Response: 1181119
Conc: 29.53 ng/ml

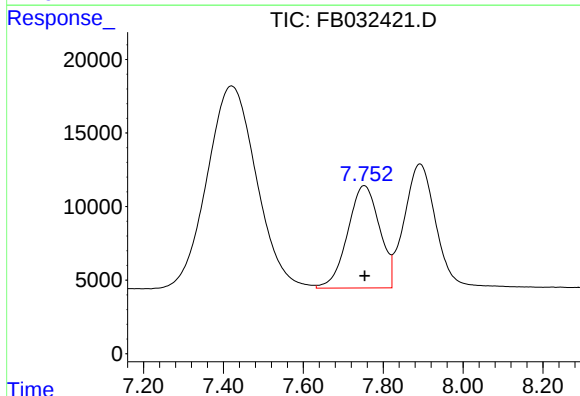


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.000 min
Response: 386821
Conc: 9.79 ng/ml

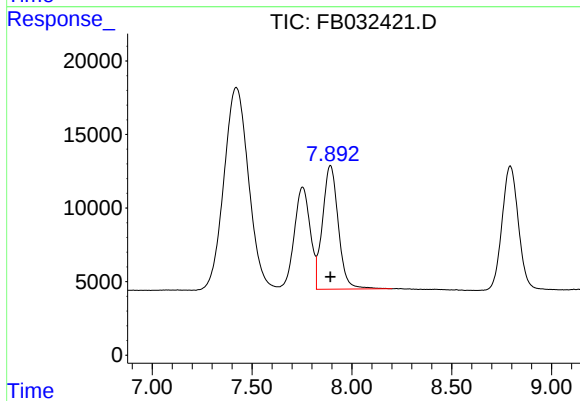

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 462897
Conc: 10.28 ng/ml

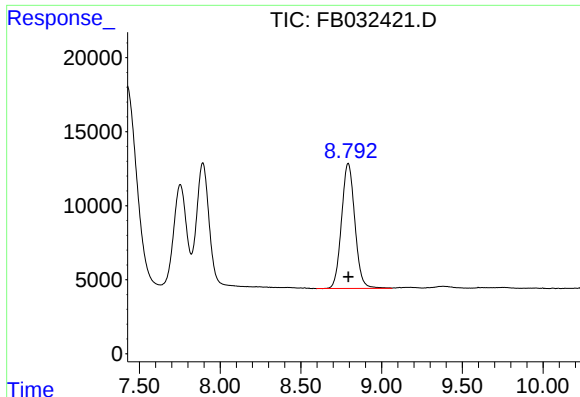

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.001 min
Response: 484856
Conc: 21.52 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1209S2

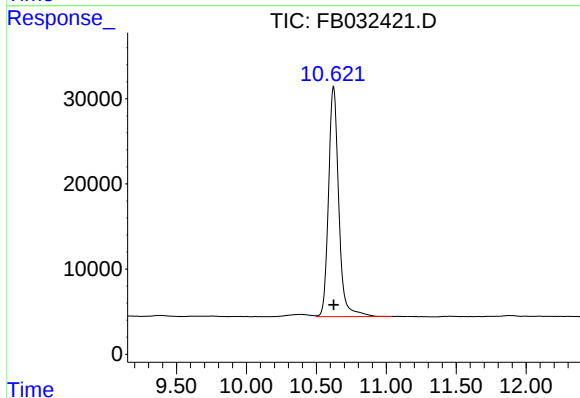


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.002 min
Response: 1375187
Conc: 30.10 ng/ml

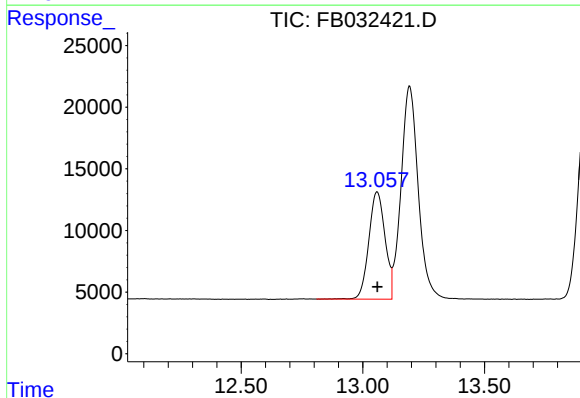


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: -0.002 min
Response: 403417
Conc: 9.91 ng/ml

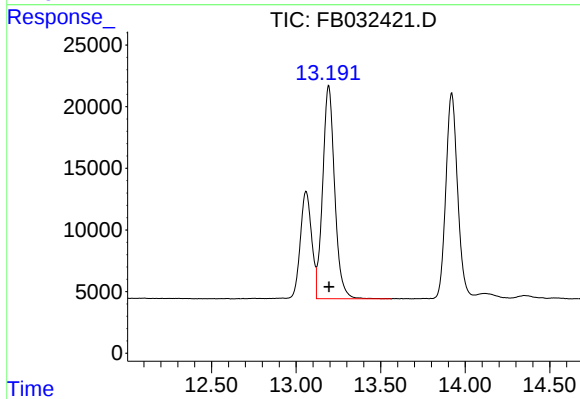

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: -0.001 min
Response: 852790
Conc: 19.80 ng/ml

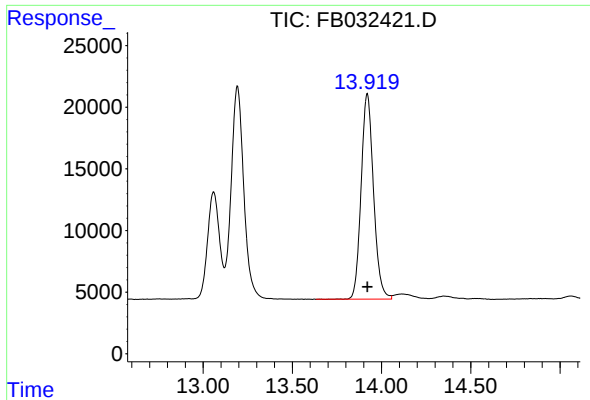

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.001 min
Response: 804629
Conc: 19.44 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1209S2

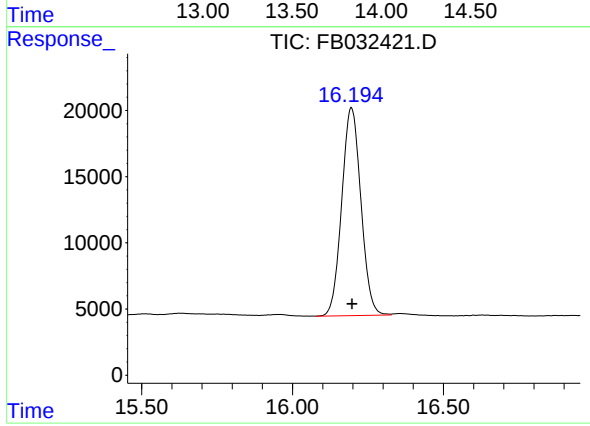

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: -0.002 min
Response: 692789
Conc: 19.68 ng/ml