

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121018\
 Data File : FB018988.D
 Signal(s) : FID2B.CH
 Acq On : 10 Dec 2018 18:11
 Operator : MJ/SJ
 Sample : J6269-01 200X
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 11 03:55:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.175	499389	57.134 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.966	47625	3.115 ng/ml
2) t 2,2,4-Trimethylpentane	7.681	93238	6.052 ng/ml
3) t n-Heptane	8.069	293813	19.768 ng/ml
6) t Toluene	11.007	49624	3.269 ng/ml
7) t Ethylbenzene	13.373	415826	26.765 ng/ml
8) t m-Xylene	13.528	90197	5.536 ng/ml
9) t O-Xylene	14.288	63564	3.759 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	878154	43.392 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121018\
Data File : FB018988.D
Signal(s) : FID2B.CH
Acq On : 10 Dec 2018 18:11
Operator : MJ/SJ
Sample : J6269-01 200X
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 11 03:55:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

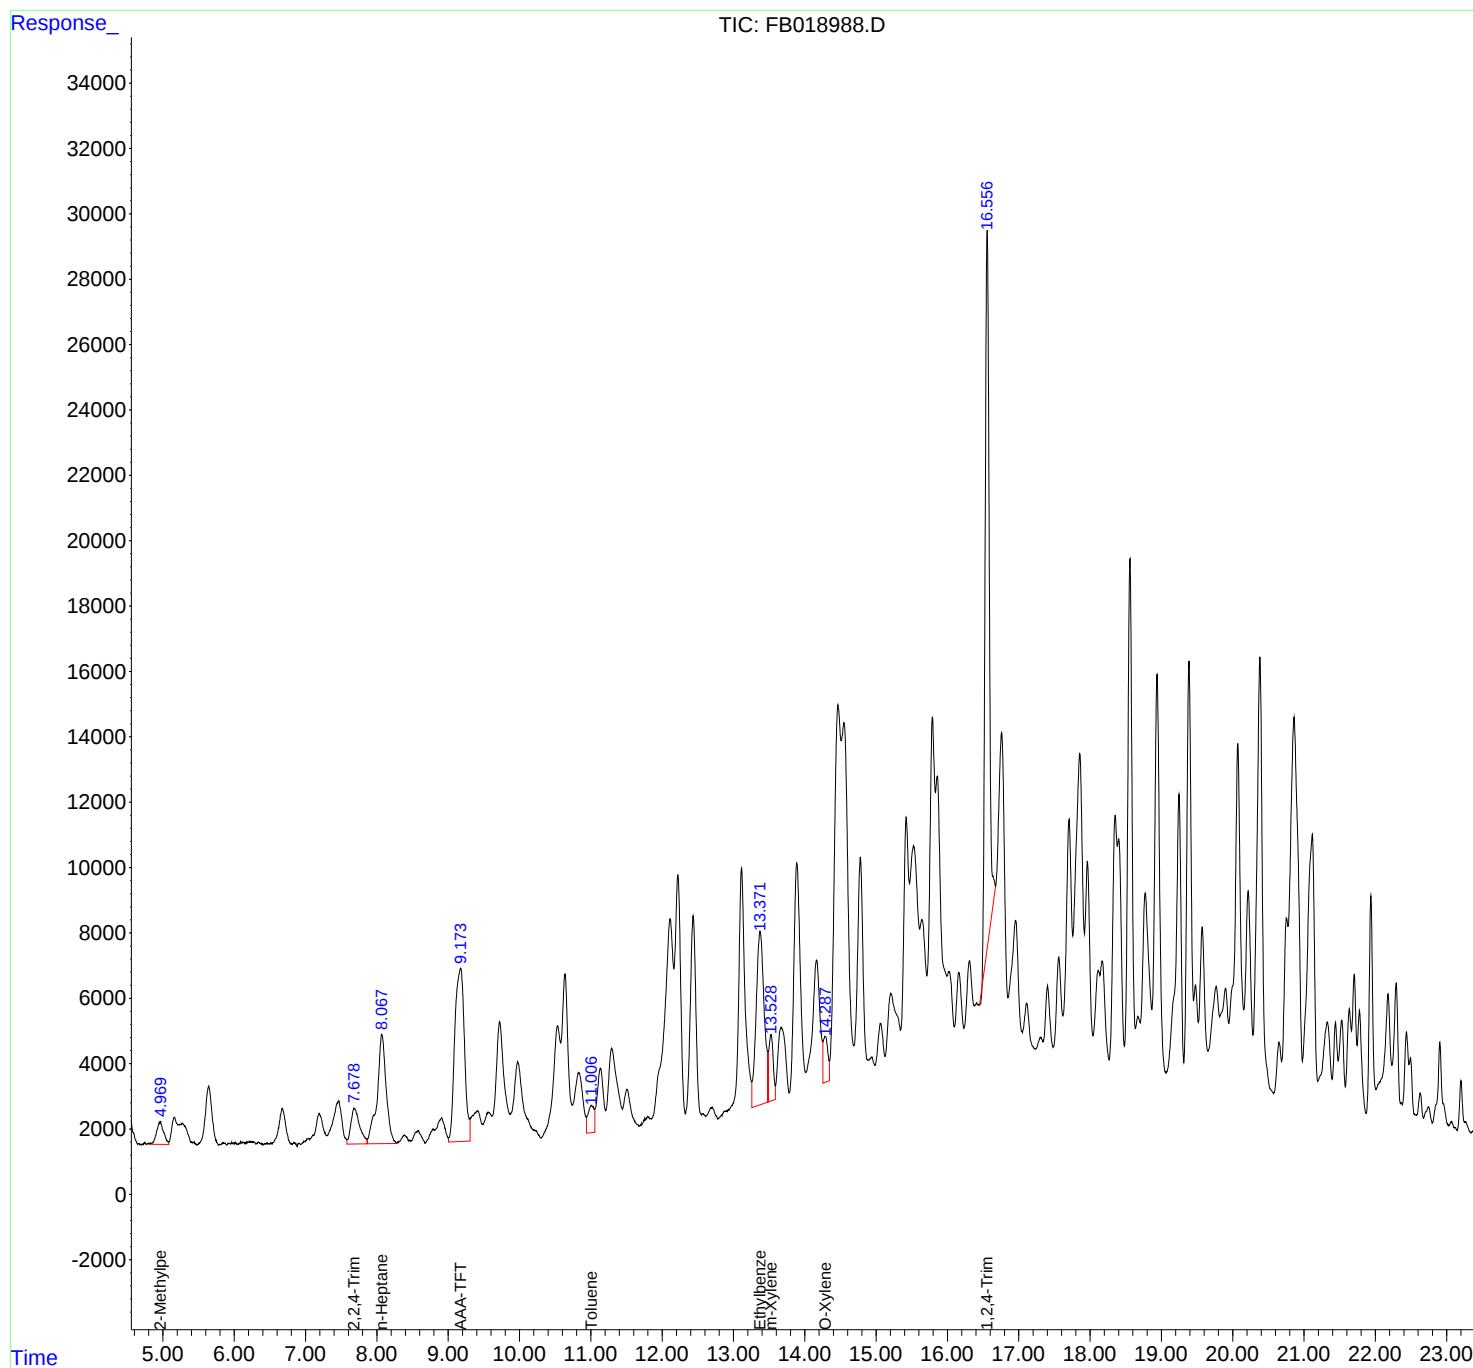


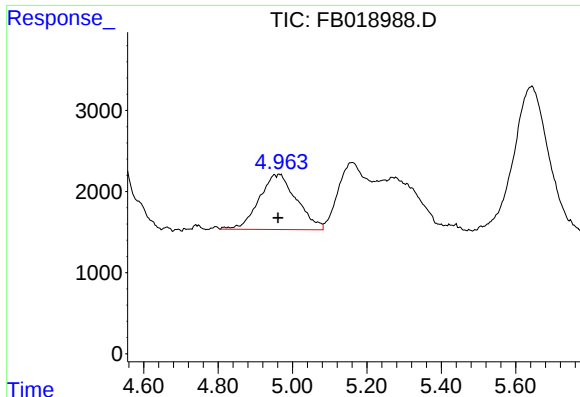

#1 2-Methylpentane


R.T.: 4.966 min
Delta R.T.: 0.005 min
Response: 47625
Conc: 3.12 ng/ml

Instrument :
FID_B
ClientSampleId :

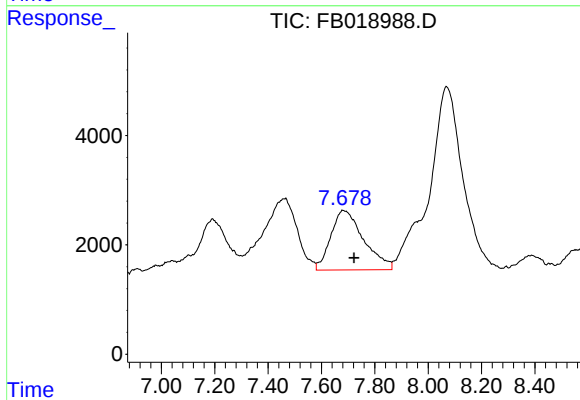


#2 2,2,4-Trimethylpentane

R.T.: 7.681 min
Delta R.T.: -0.042 min
Response: 93238
Conc: 6.05 ng/ml

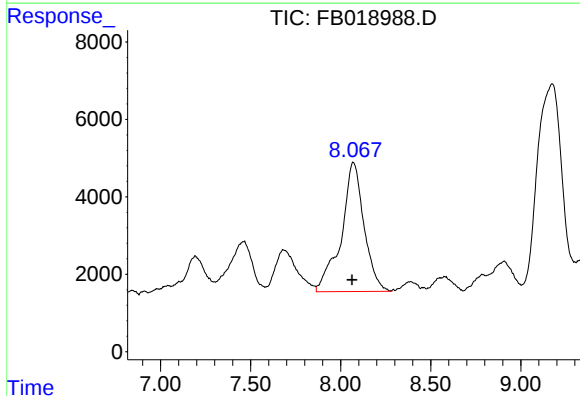


#3 n-Heptane

R.T.: 8.069 min
Delta R.T.: 0.007 min
Response: 293813
Conc: 19.77 ng/ml

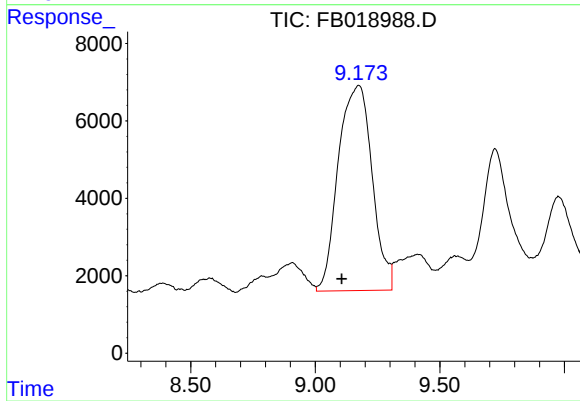

#5 AAA-TFT


R.T.: 9.175 min
Delta R.T.: 0.068 min
Response: 499389
Conc: 57.13 ng/ml

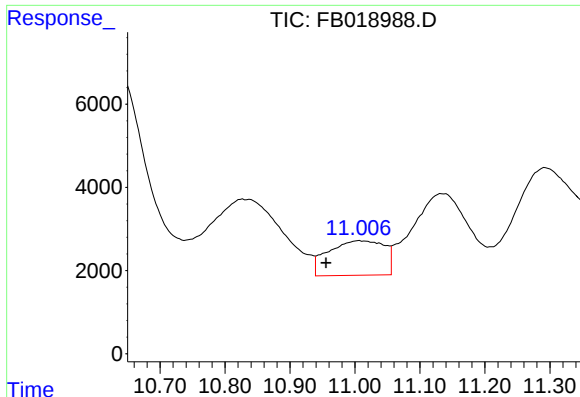

#6 Toluene


R.T.: 11.007 min
Delta R.T.: 0.052 min
Response: 49624
Conc: 3.27 ng/ml

Instrument :
FID_B
ClientSampleId :

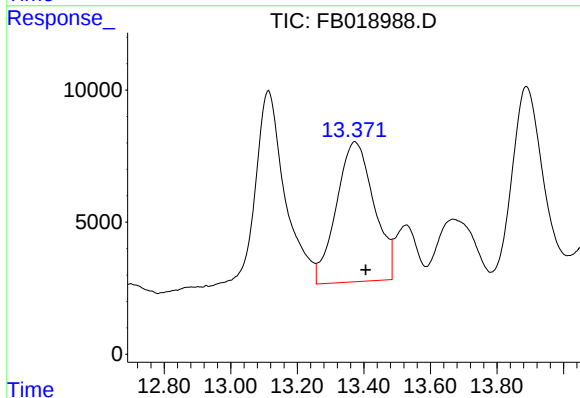


#7 Ethylbenzene

R.T.: 13.373 min
Delta R.T.: -0.032 min
Response: 415826
Conc: 26.77 ng/ml

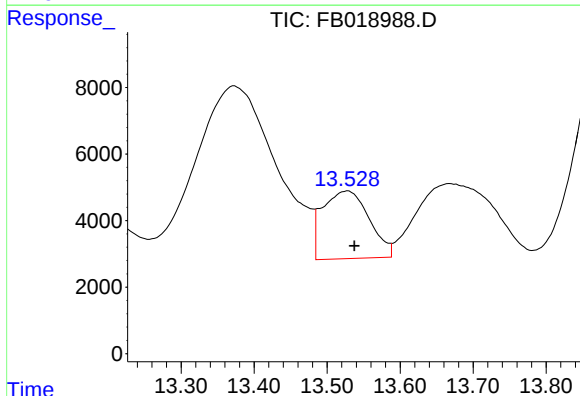


#8 m-Xylene

R.T.: 13.528 min
Delta R.T.: -0.010 min
Response: 90197
Conc: 5.54 ng/ml

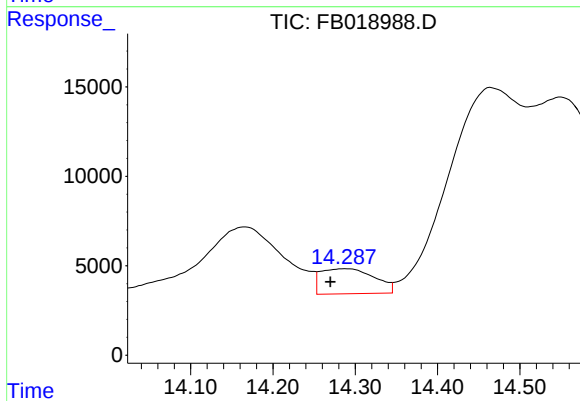

#9 O-Xylene

R.T.: 14.288 min
Delta R.T.: 0.019 min
Response: 63564
Conc: 3.76 ng/ml

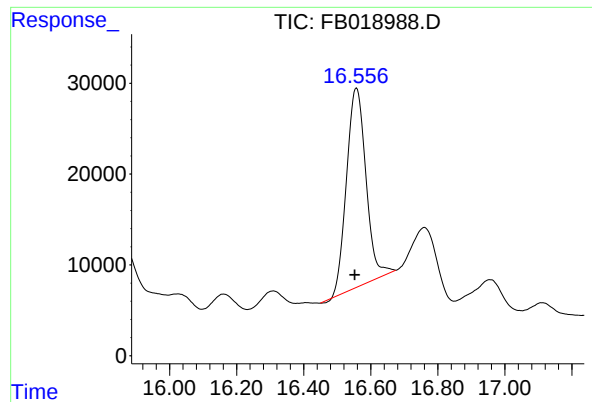

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.005 min
Response: 878154
Conc: 43.39 ng/ml

Instrument :
FID_B
ClientSampleId :