

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121018\
 Data File : FB018973.D
 Signal(s) : FID2B.CH
 Acq On : 10 Dec 2018 9:35
 Operator : MJ/SJ
 Sample : BSF1210S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1210S1

Integration File: Calibration.e
 Quant Time: Dec 11 03:53:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.107	162618	18.605 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.960	455685	29.808 ng/ml
2) t 2,2,4-Trimethylpentane	7.723	470316	30.528 ng/ml
3) t n-Heptane	8.062	151648	10.203 ng/ml
4) t Benzene	8.202	186670	10.363 ng/ml
6) t Toluene	10.955	456116	30.049 ng/ml
7) t Ethylbenzene	13.405	157007	10.106 ng/ml
8) t m-Xylene	13.538	331990	20.378 ng/ml
9) t O-Xylene	14.269	345967	20.461 ng/ml
10) t 1,2,4-Trimethylbenzene	16.553	408278	20.174 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121018\
Data File : FB018973.D
Signal(s) : FID2B.CH
Acq On : 10 Dec 2018 9:35
Operator : MJ/SJ
Sample : BSF1210S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1210S1

Integration File: Calibration.e
Quant Time: Dec 11 03:53:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

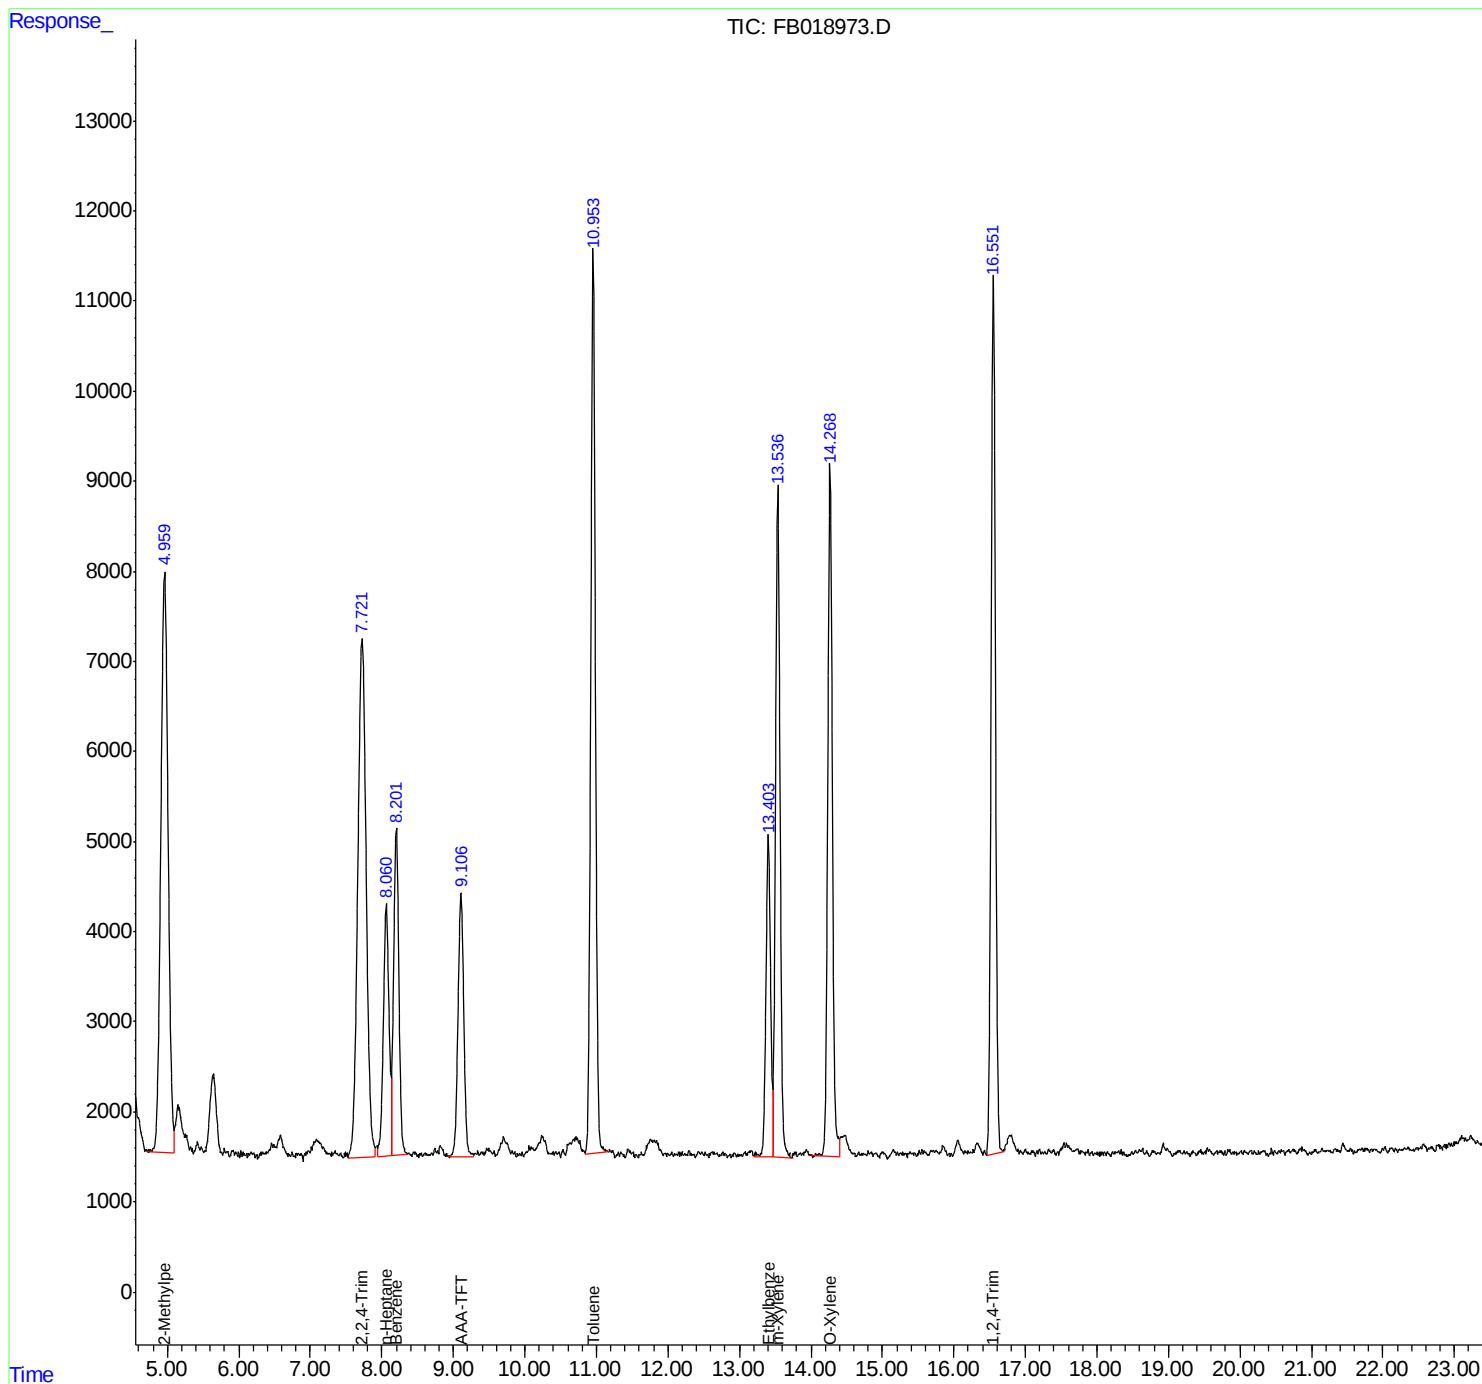


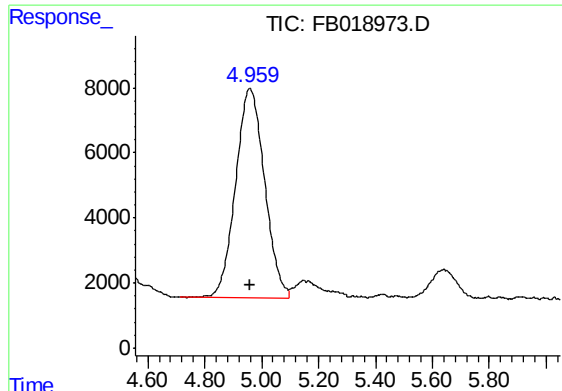

#1 2-Methylpentane


R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 455685
Conc: 29.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1210S1

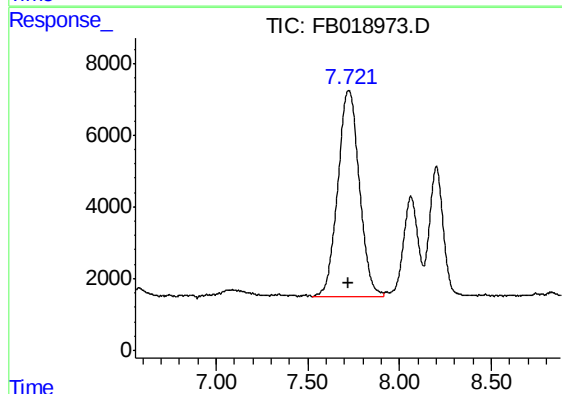


#2 2,2,4-Trimethylpentane

R.T.: 7.723 min
Delta R.T.: 0.000 min
Response: 470316
Conc: 30.53 ng/ml

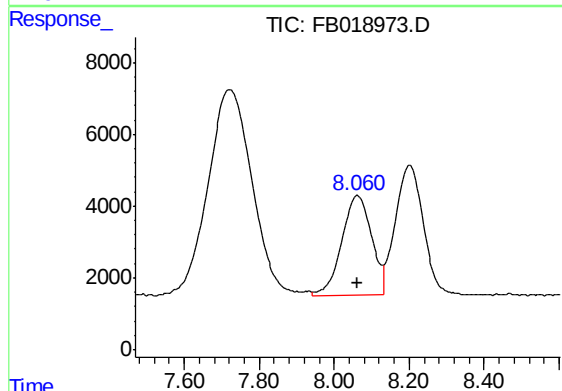


#3 n-Heptane

R.T.: 8.062 min
Delta R.T.: 0.000 min
Response: 151648
Conc: 10.20 ng/ml

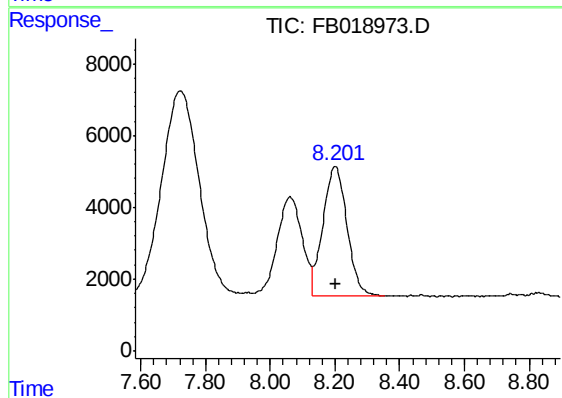

#4 Benzene


R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 186670
Conc: 10.36 ng/ml

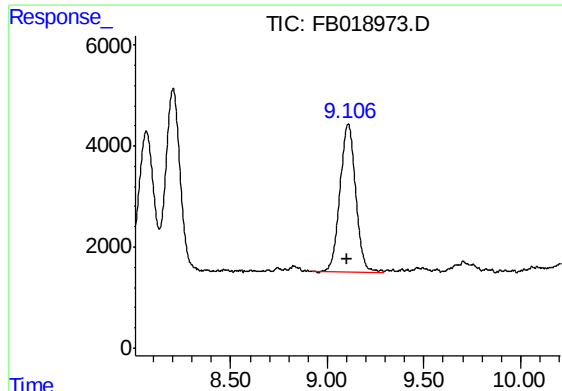

#5 AAA-TFT


R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 162618
Conc: 18.60 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1210S1

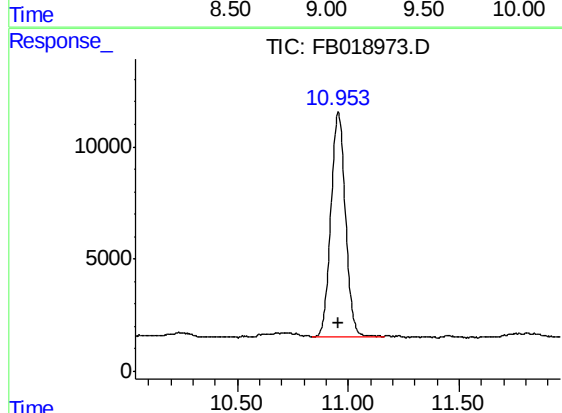


#6 Toluene

R.T.: 10.955 min
Delta R.T.: 0.000 min
Response: 456116
Conc: 30.05 ng/ml

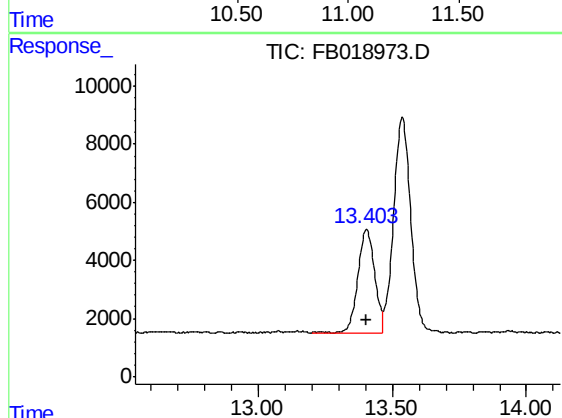


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: 0.000 min
Response: 157007
Conc: 10.11 ng/ml

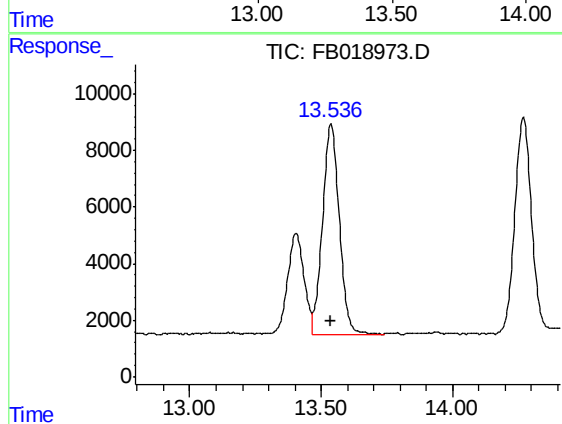

#8 m-Xylene


R.T.: 13.538 min
Delta R.T.: 0.000 min
Response: 331990
Conc: 20.38 ng/ml

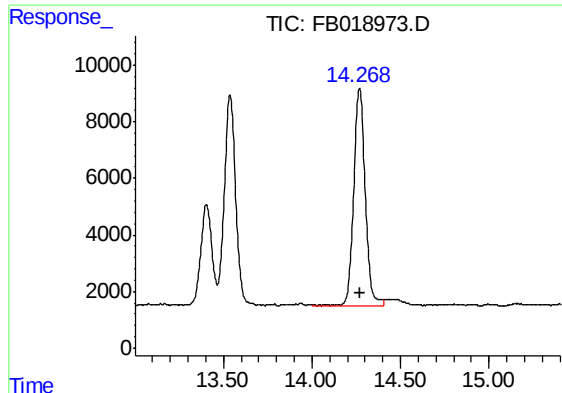

#9 O-Xylene

R.T.: 14.269 min
Delta R.T.: 0.000 min
Response: 345967
Conc: 20.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1210S1

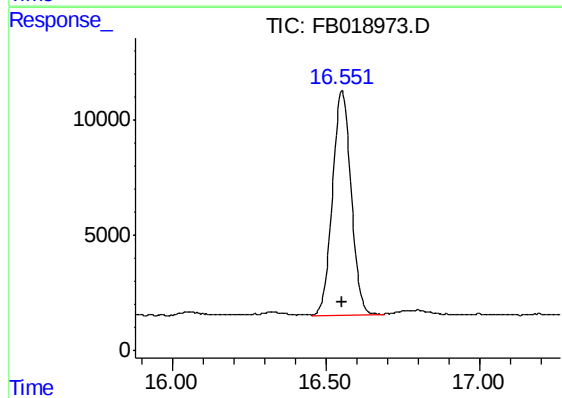

#10 1,2,4-Trimethylbenzene

R.T.: 16.553 min
Delta R.T.: 0.000 min
Response: 408278
Conc: 20.17 ng/ml