

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121020\
 Data File : FB025319.D
 Signal(s) : FID2B.CH
 Acq On : 10 Dec 2020 10:18
 Operator : DD/AJ
 Sample : BSF1210S2
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1210S2

Integration File: Calibration.e
 Quant Time: Dec 11 00:19:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	380589	18.103 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	857155	28.511 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	891666	29.634 ng/ml
3) t n-Heptane	7.757	293624	9.916 ng/ml
4) t Benzene	7.891	348781	9.430 ng/ml
6) t Toluene	10.629	990988	28.201 ng/ml
7) t Ethylbenzene	13.069	303680	9.297 ng/ml
8) t m-Xylene	13.202	608383	18.797 ng/ml
9) t O-Xylene	13.930	587492	18.584 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	510860	18.813 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121020\
Data File : FB025319.D
Signal(s) : FID2B.CH
Acq On : 10 Dec 2020 10:18
Operator : DD/AJ
Sample : BSF1210S2
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1210S2

Integration File: Calibration.e
Quant Time: Dec 11 00:19:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

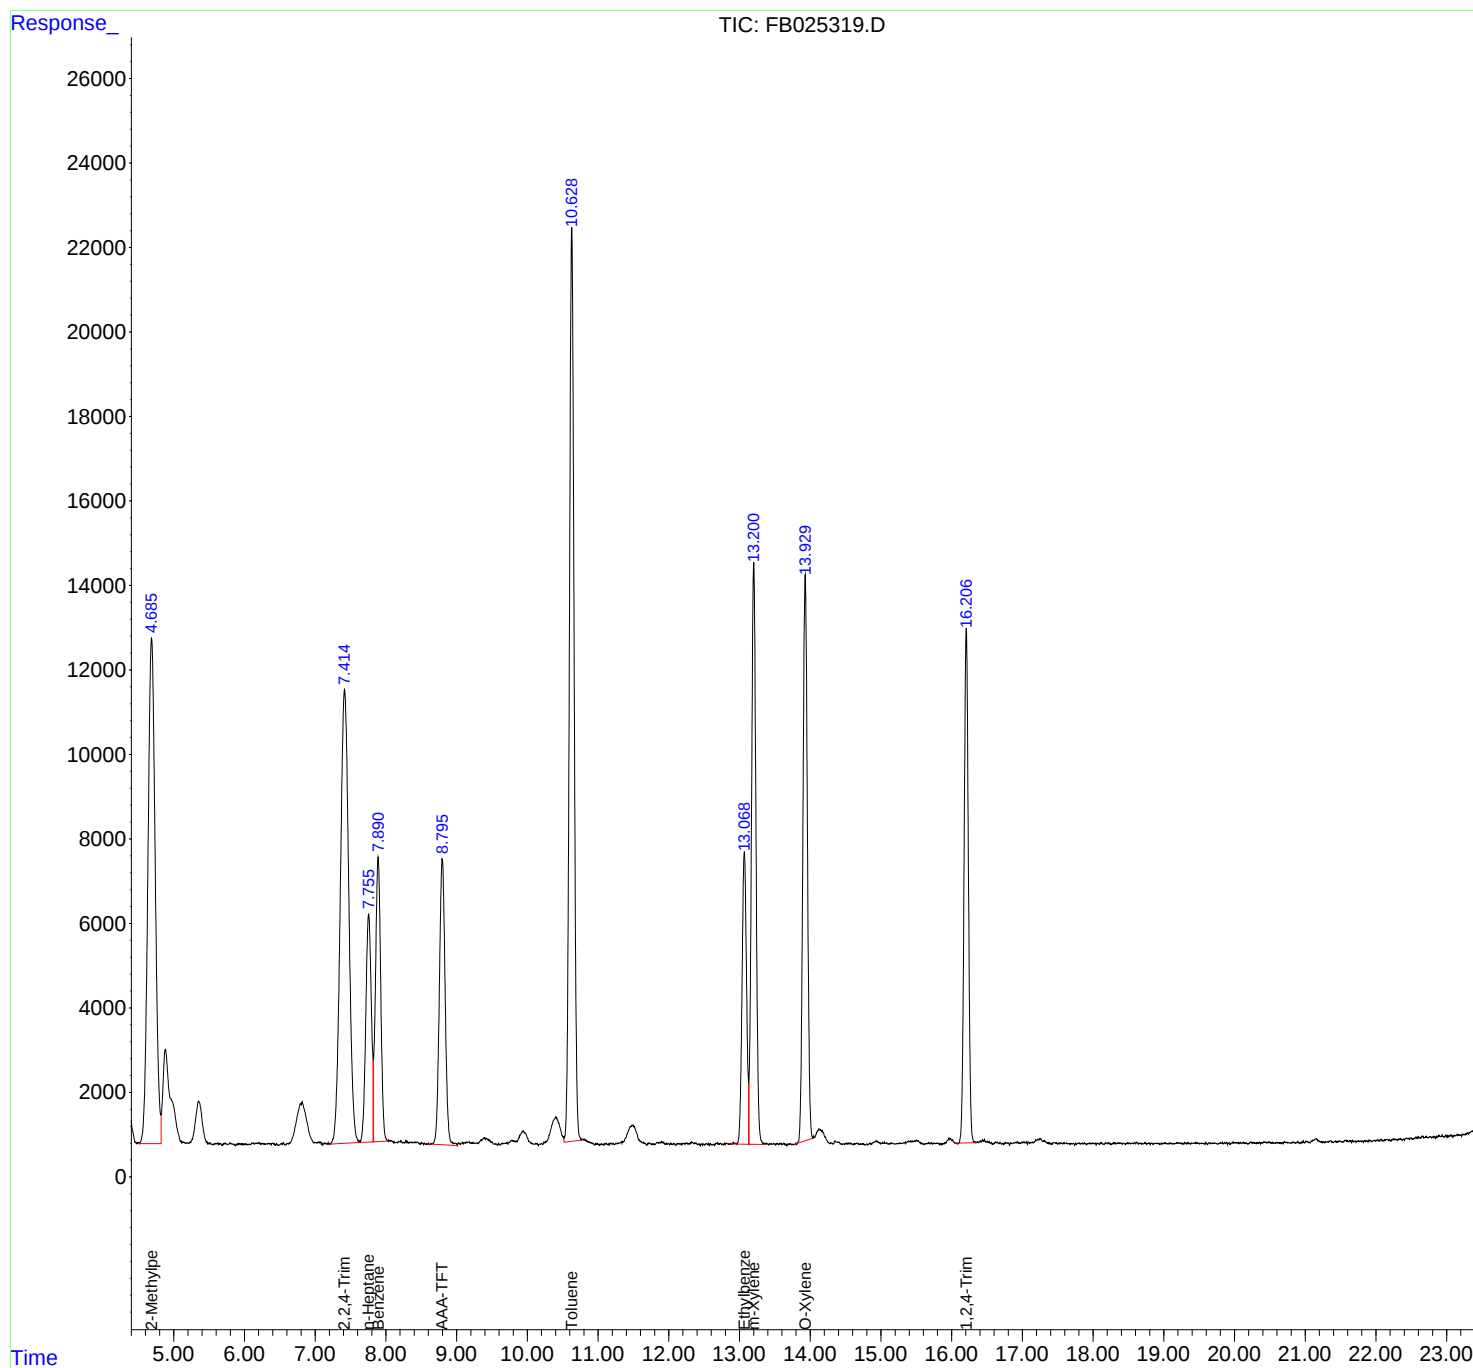


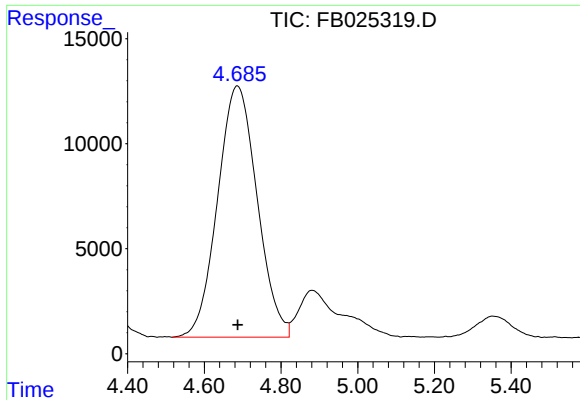

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 857155
Conc: 28.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1210S2

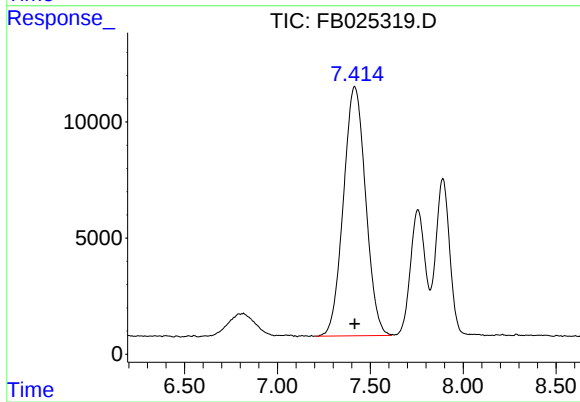


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 891666
Conc: 29.63 ng/ml

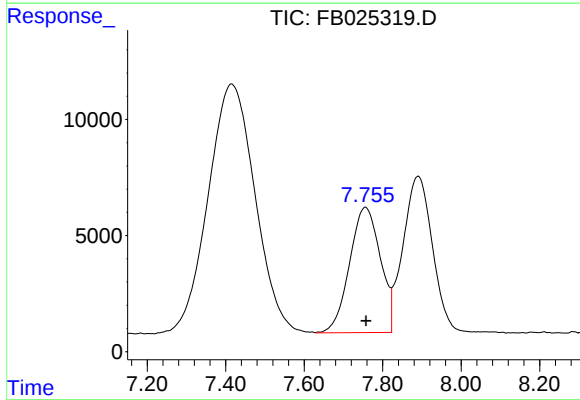


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.001 min
Response: 293624
Conc: 9.92 ng/ml

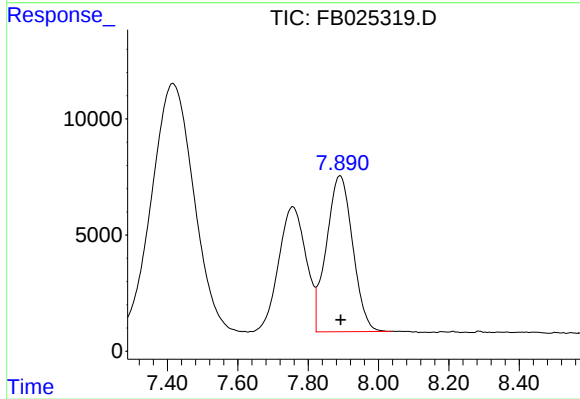

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 348781
Conc: 9.43 ng/ml

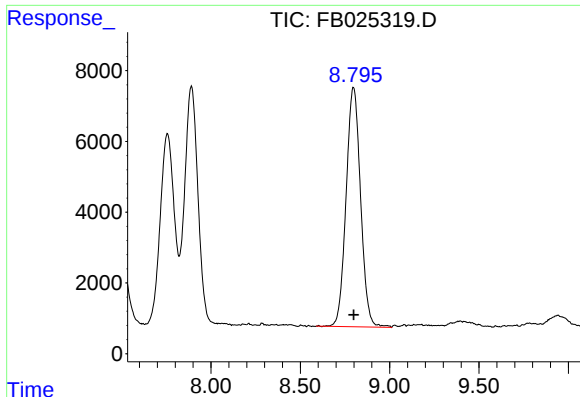

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 380589
Conc: 18.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1210S2

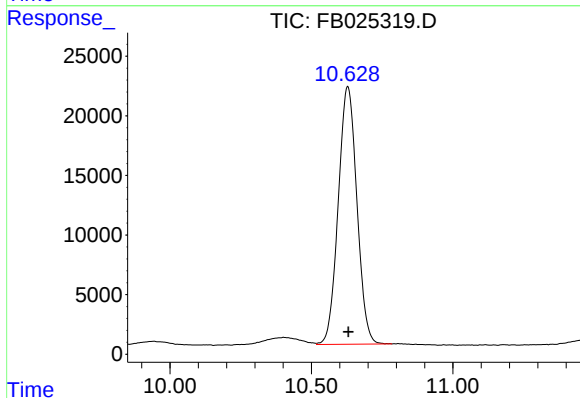


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 990988
Conc: 28.20 ng/ml

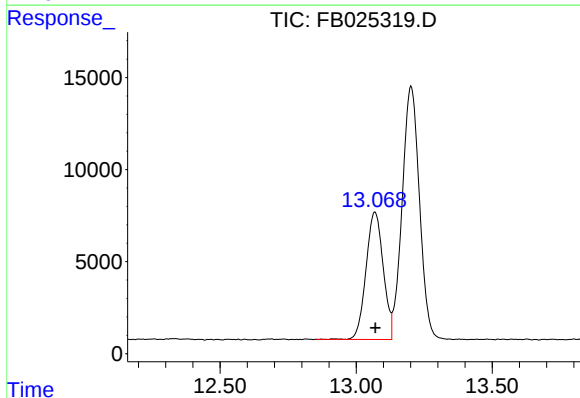


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.001 min
Response: 303680
Conc: 9.30 ng/ml

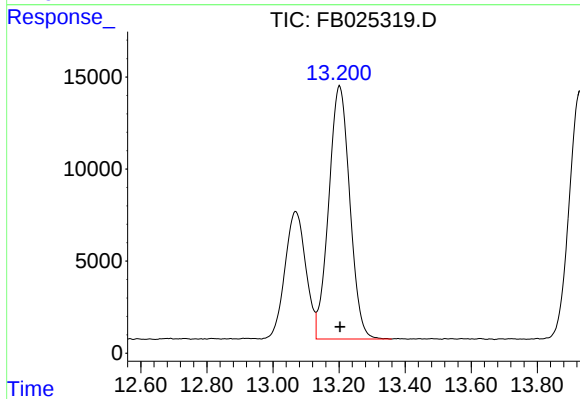

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.002 min
Response: 608383
Conc: 18.80 ng/ml

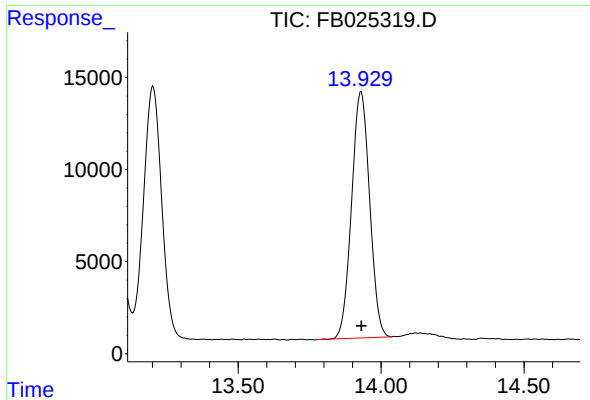

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.002 min
Response: 587492
Conc: 18.58 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1210S2

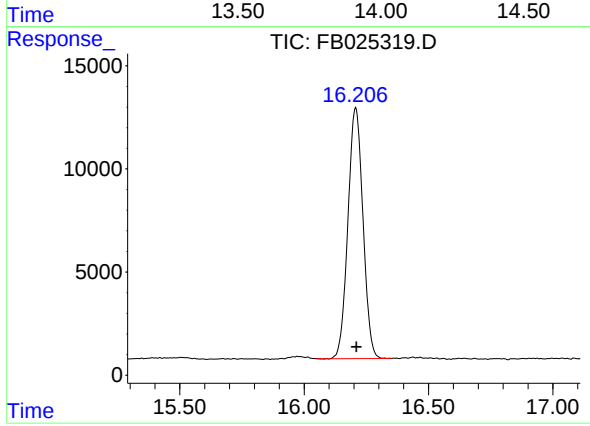

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 510860
Conc: 18.81 ng/ml