

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121020\
 Data File : FB025321.D
 Signal(s) : FID2B.CH
 Acq On : 10 Dec 2020 12:08
 Operator : DD/AJ
 Sample : L4989-02MS
 Misc : 4.99g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-02-120920MS

Integration File: Calibration.e
 Quant Time: Dec 11 00:19:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	358099	17.034 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	701003	23.317 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	671499	22.317 ng/ml
3) t n-Heptane	7.757	217730	7.353 ng/ml
4) t Benzene	7.892	320174	8.656 ng/ml
6) t Toluene	10.630	897245	25.533 ng/ml
7) t Ethylbenzene	13.070	276254	8.457 ng/ml
8) t m-Xylene	13.203	547237	16.907 ng/ml
9) t O-Xylene	13.931	539792	17.075 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	444903	16.384 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121020\
Data File : FB025321.D
Signal(s) : FID2B.CH
Acq On : 10 Dec 2020 12:08
Operator : DD/AJ
Sample : L4989-02MS
Misc : 4.99g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-02-120920MS

Integration File: Calibration.e
Quant Time: Dec 11 00:19:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

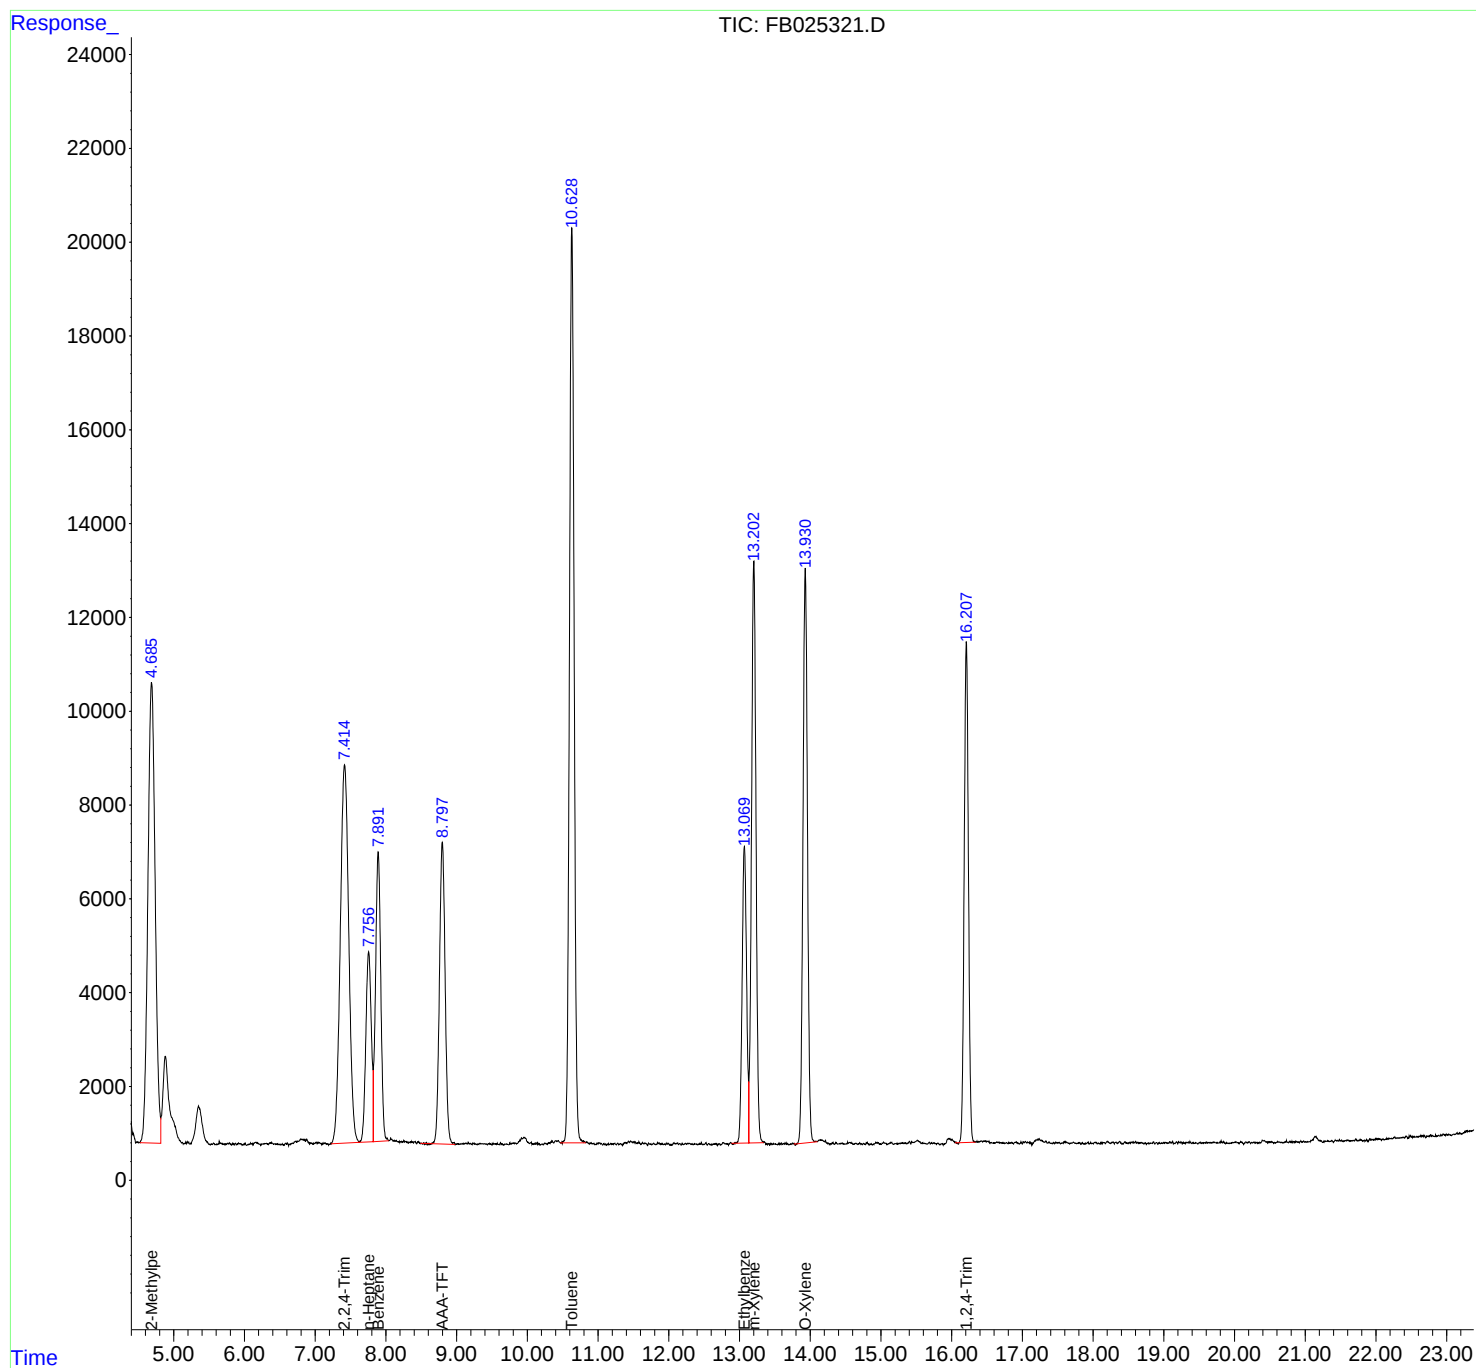


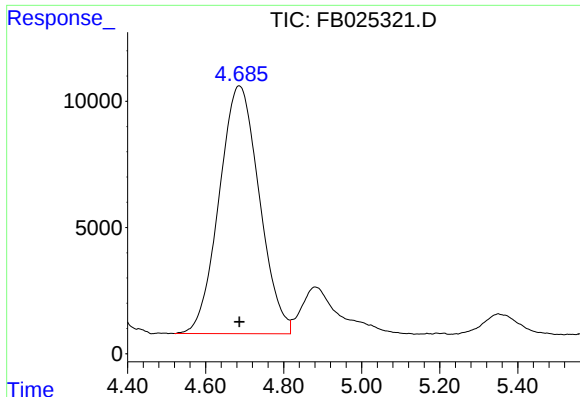

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 701003
Conc: 23.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-02-120920MS

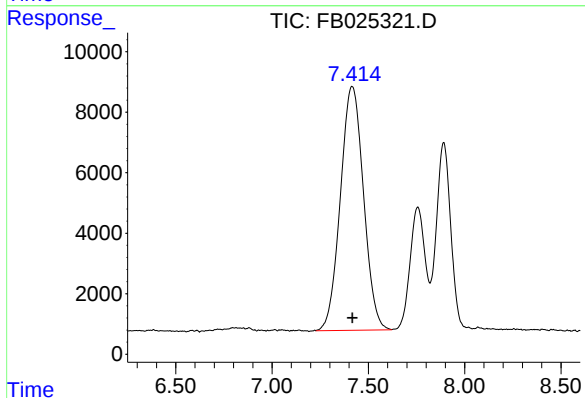


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 671499
Conc: 22.32 ng/ml

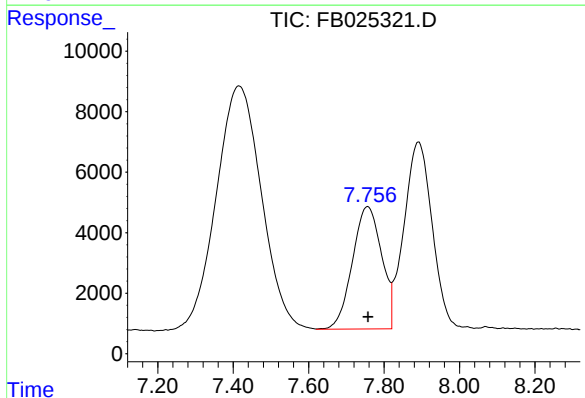


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 217730
Conc: 7.35 ng/ml

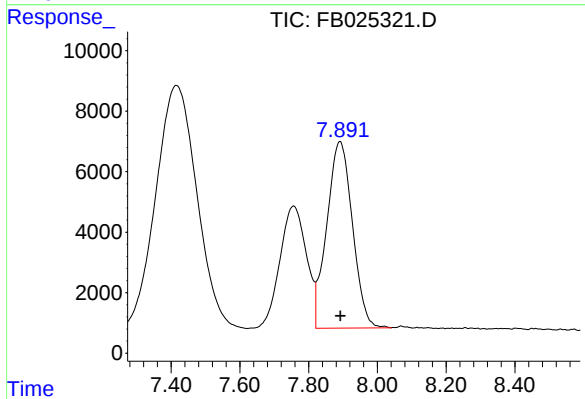

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 320174
Conc: 8.66 ng/ml

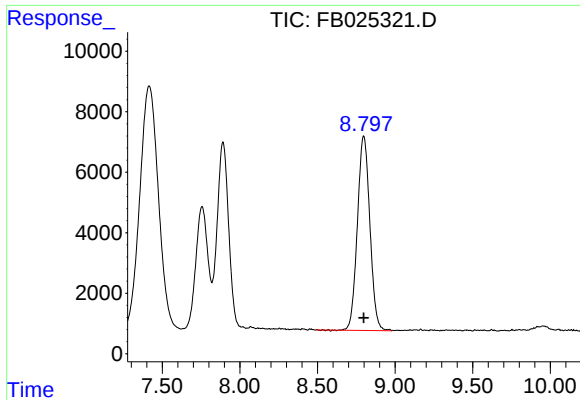

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 358099
Conc: 17.03 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-02-120920MS

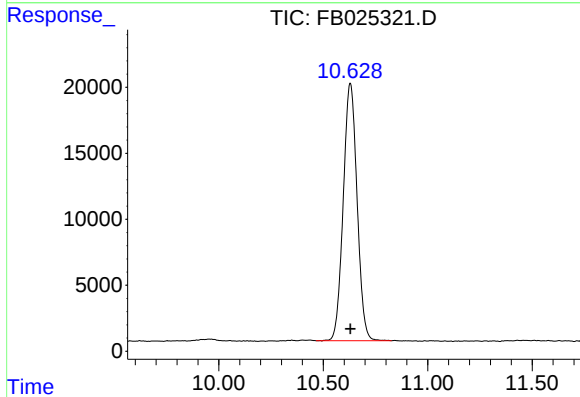


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 897245
Conc: 25.53 ng/ml

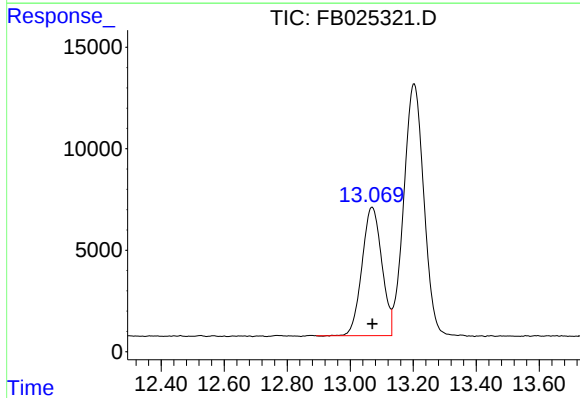


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 276254
Conc: 8.46 ng/ml

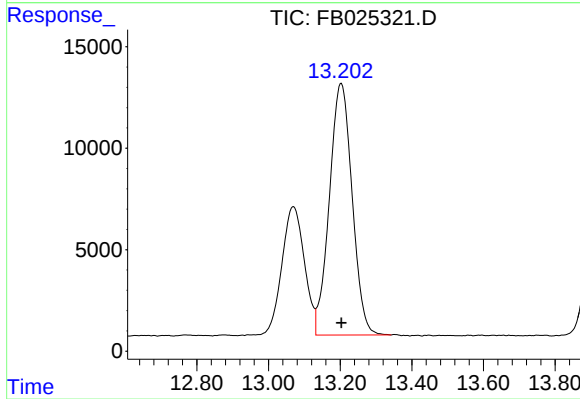

#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 547237
Conc: 16.91 ng/ml

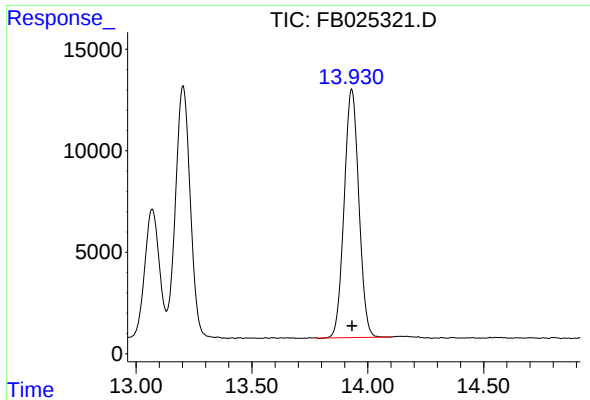

#9 O-Xylene


R.T.: 13.931 min

Delta R.T.: 0.000 min

Response: 539792

Conc: 17.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-02-120920MS

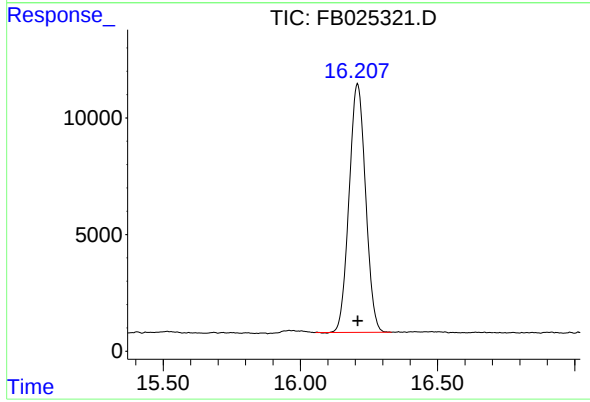

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min

Delta R.T.: 0.000 min

Response: 444903

Conc: 16.38 ng/ml