

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121020\
 Data File : FB025322.D
 Signal(s) : FID2B.CH
 Acq On : 10 Dec 2020 12:38
 Operator : DD/AJ
 Sample : L4989-02MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-02-120920MSD

Integration File: Calibration.e
 Quant Time: Dec 11 00:19:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	419426	19.951 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	749690	24.937 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	648119	21.540 ng/ml
3) t n-Heptane	7.758	211091	7.128 ng/ml
4) t Benzene	7.893	340178	9.197 ng/ml
6) t Toluene	10.631	951657	27.081 ng/ml
7) t Ethylbenzene	13.071	291380	8.920 ng/ml
8) t m-Xylene	13.203	575642	17.785 ng/ml
9) t O-Xylene	13.931	559772	17.707 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	459596	16.925 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121020\
Data File : FB025322.D
Signal(s) : FID2B.CH
Acq On : 10 Dec 2020 12:38
Operator : DD/AJ
Sample : L4989-02MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-02-120920MSD

Integration File: Calibration.e
Quant Time: Dec 11 00:19:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

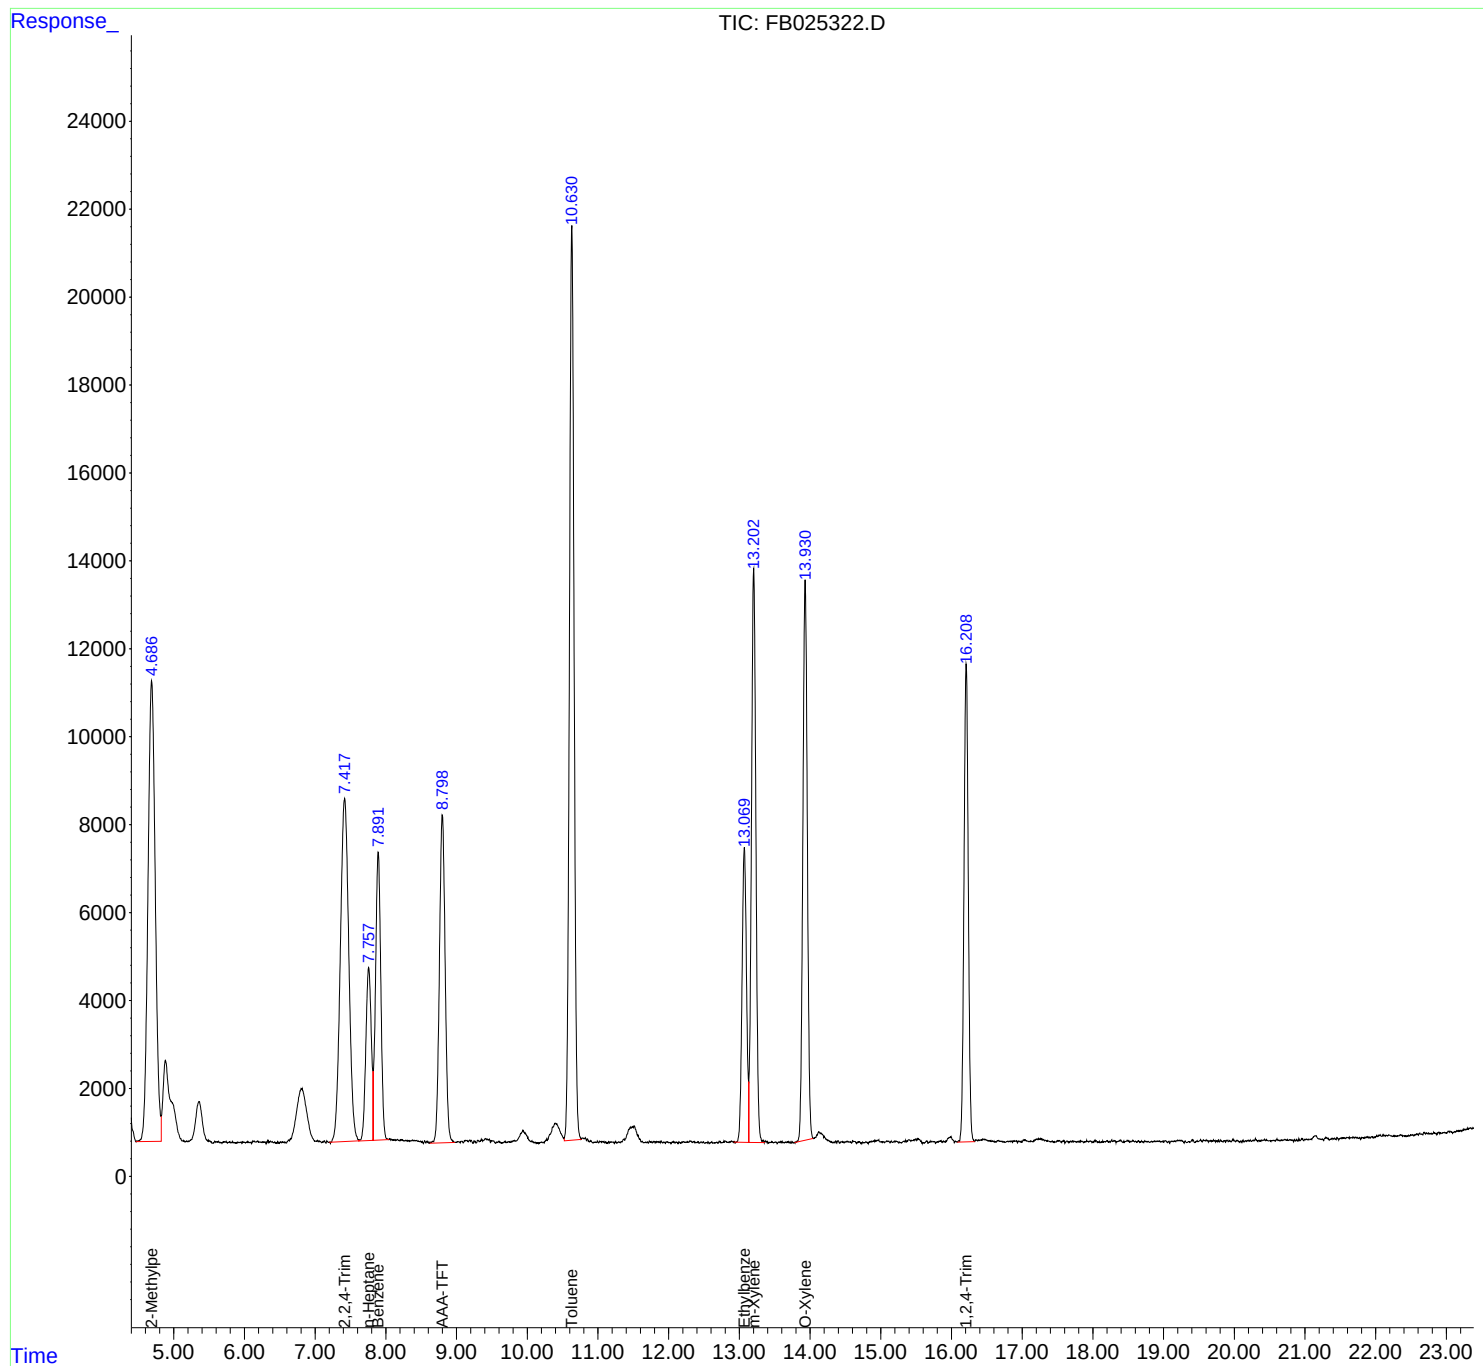


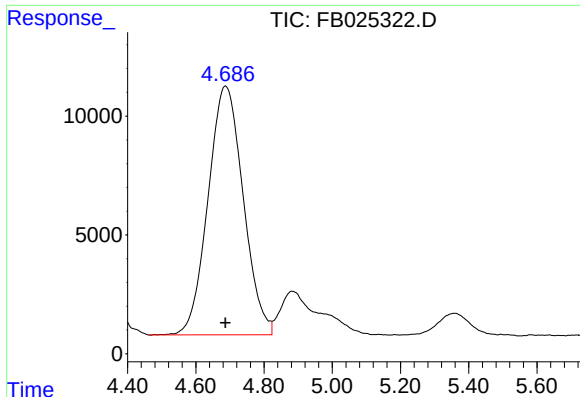

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 749690
Conc: 24.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-02-120920MSD

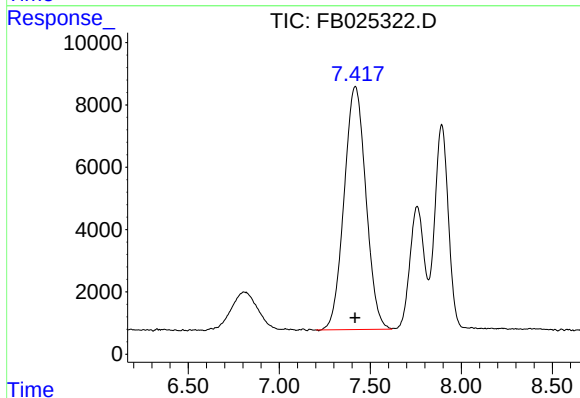


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.002 min
Response: 648119
Conc: 21.54 ng/ml

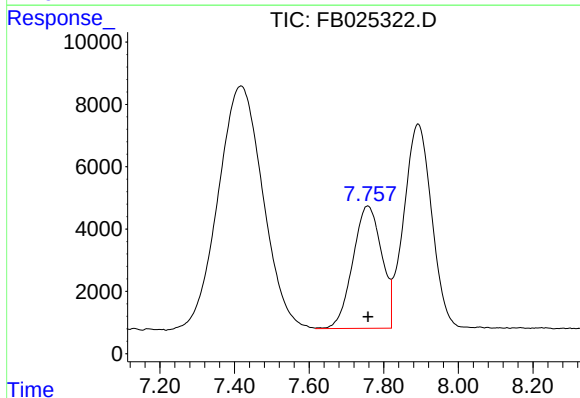


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 211091
Conc: 7.13 ng/ml

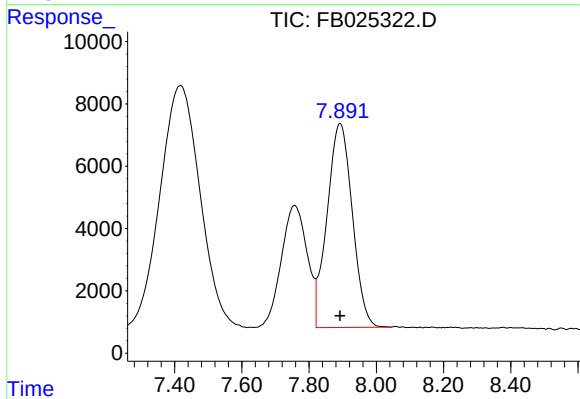

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 340178
Conc: 9.20 ng/ml

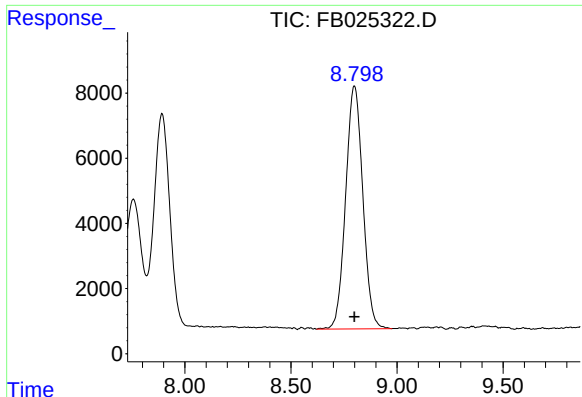

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 419426
Conc: 19.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-02-120920MSD

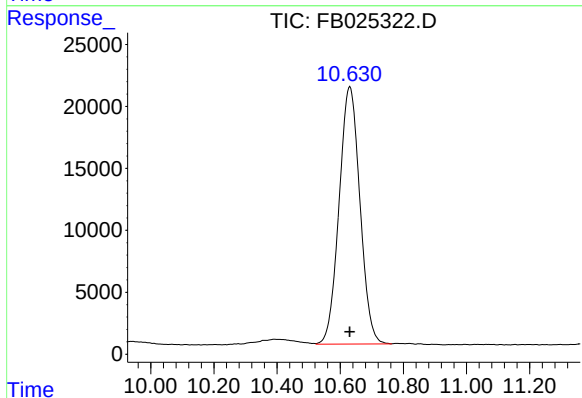


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 951657
Conc: 27.08 ng/ml

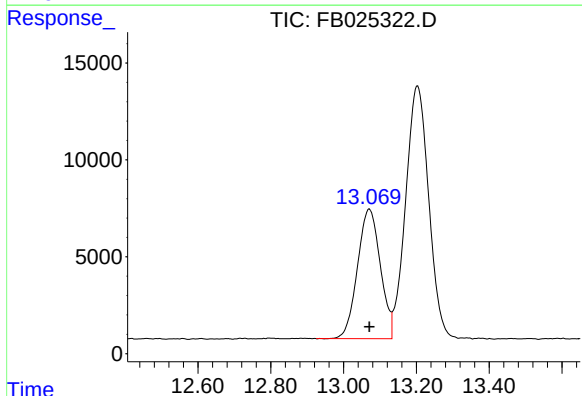


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 291380
Conc: 8.92 ng/ml

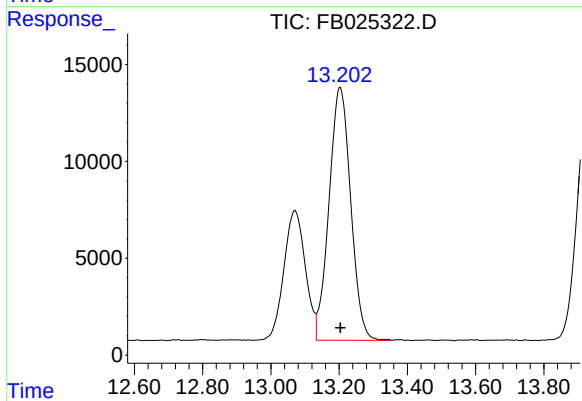

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 575642
Conc: 17.79 ng/ml

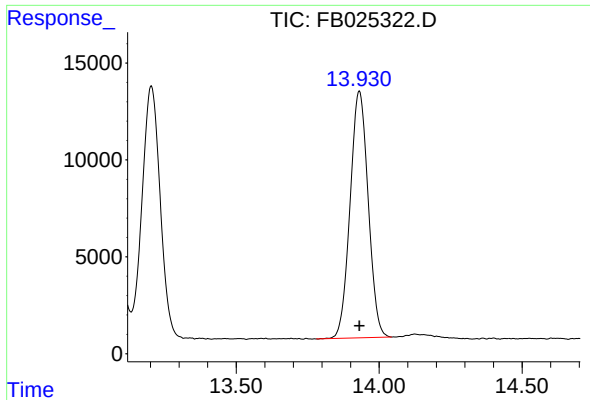

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 559772
Conc: 17.71 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-02-120920MSD

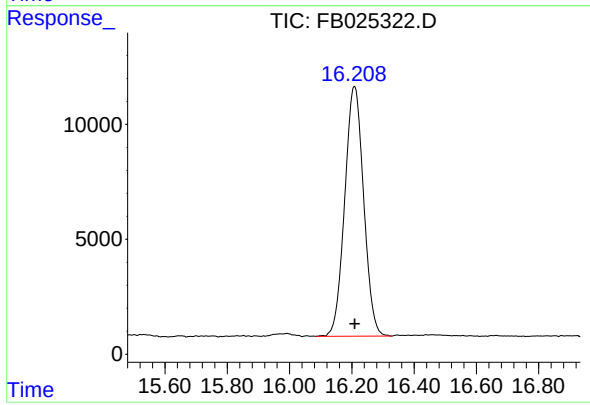

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 459596
Conc: 16.92 ng/ml