

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121119\
 Data File : FB023190.D
 Signal(s) : FID2B.CH
 Acq On : 11 Dec 2019 12:40
 Operator : DD/AJ
 Sample : BSF1211S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 12 00:29:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.795	503953	20.516 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.688	738081	22.586 ng/ml
2) t	2,2,4-Trimethylpentane	7.413	905968	25.981 ng/ml
3) t	n-Heptane	7.753	291555	8.480 ng/ml
4) t	Benzene	7.889	377533	9.061 ng/ml
6) t	Toluene	10.626	1109218	27.535 ng/ml
7) t	Ethylbenzene	13.067	347593	9.008 ng/ml
8) t	m-Xylene	13.200	659651	18.127 ng/ml
9) t	O-Xylene	13.928	634983	18.288 ng/ml
10) t	1,2,4-Trimethylbenzene	16.206	528075	18.831 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121119\
Data File : FB023190.D
Signal(s) : FID2B.CH
Acq On : 11 Dec 2019 12:40
Operator : DD/AJ
Sample : BSF1211S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 12 00:29:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

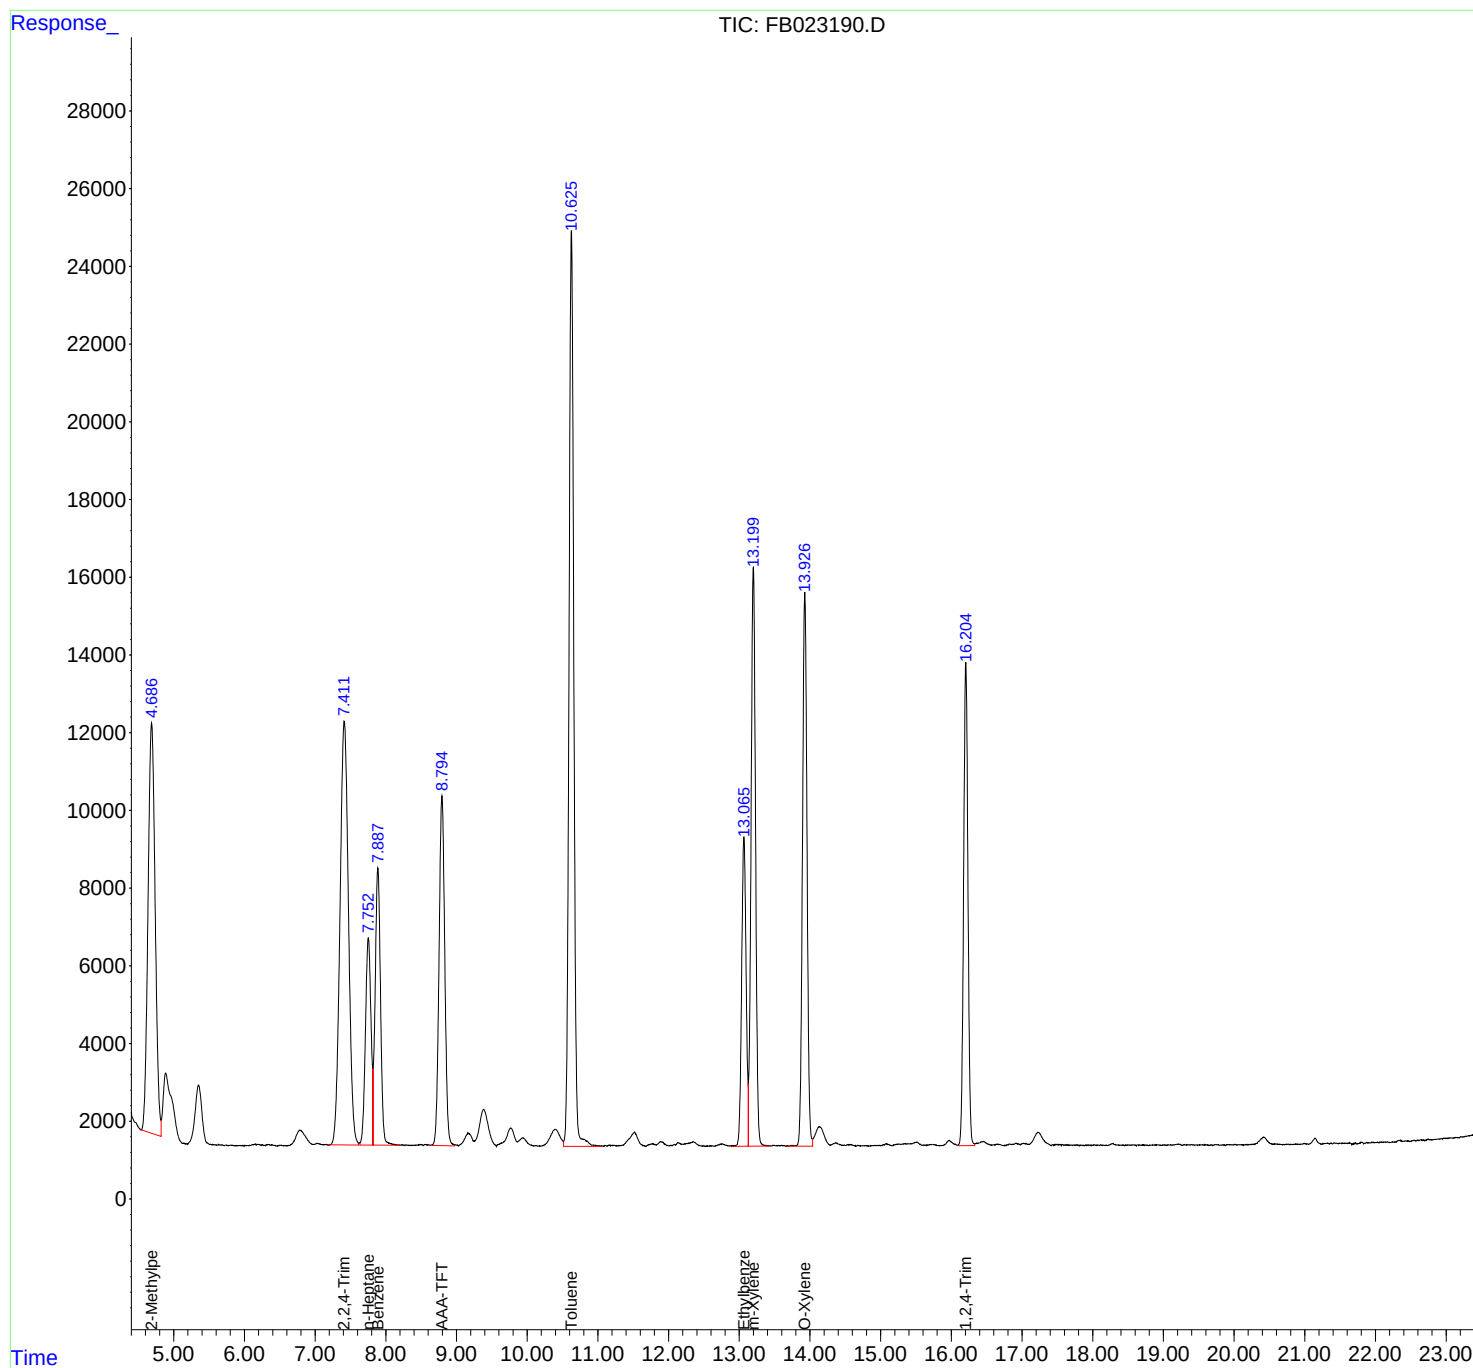

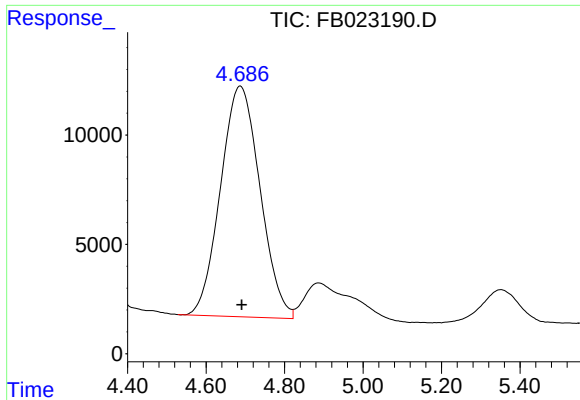


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 738081
Conc: 22.59 ng/ml

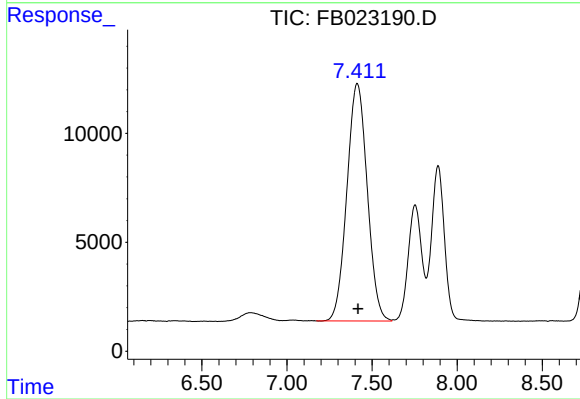


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.005 min
Response: 905968
Conc: 25.98 ng/ml

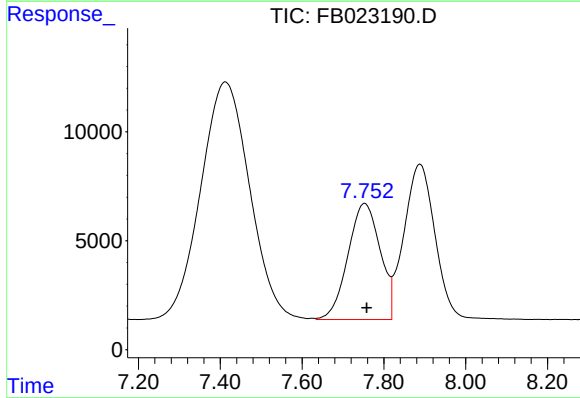


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.004 min
Response: 291555
Conc: 8.48 ng/ml

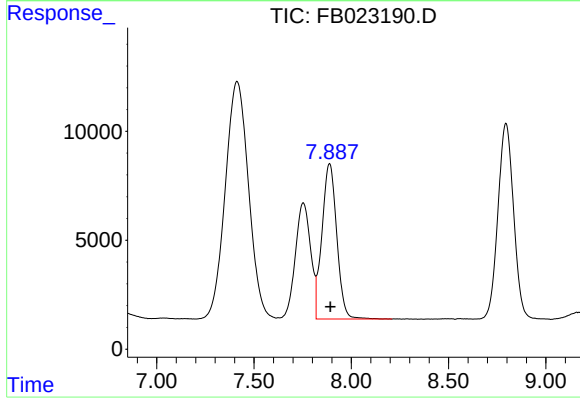


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 377533
Conc: 9.06 ng/ml

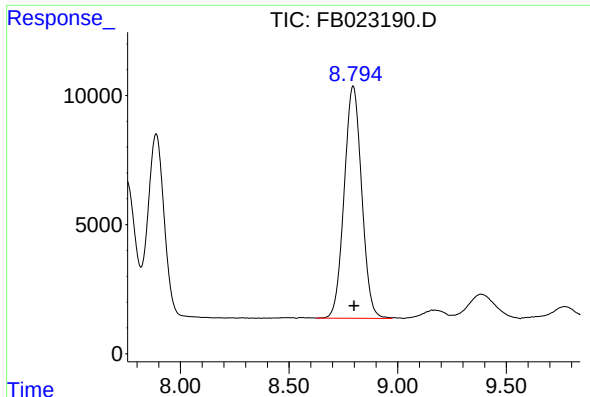


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 503953
Conc: 20.52 ng/ml

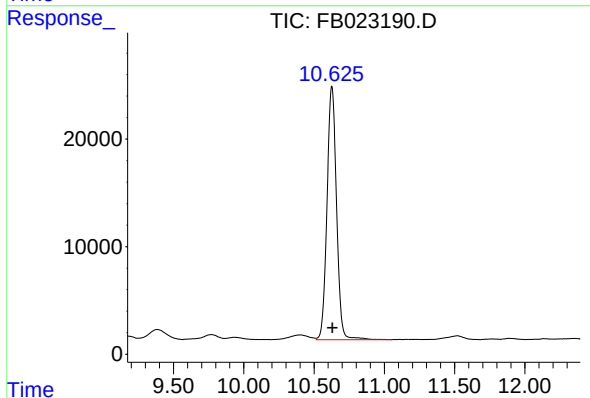


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.004 min
Response: 1109218
Conc: 27.54 ng/ml

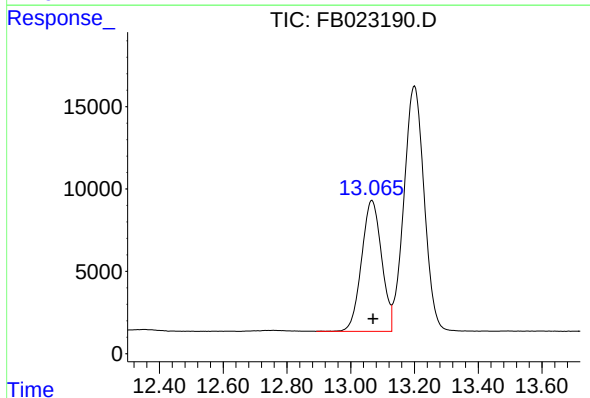


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.004 min
Response: 347593
Conc: 9.01 ng/ml

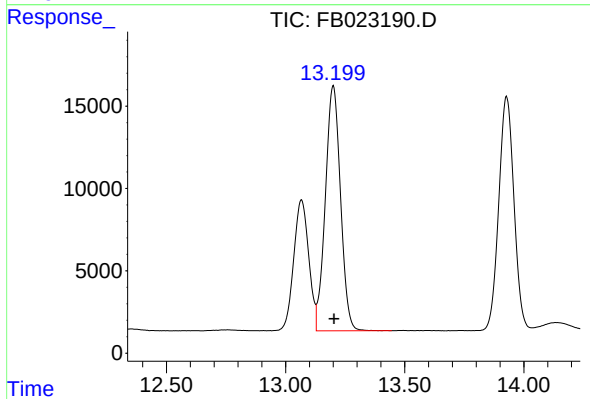


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 659651
Conc: 18.13 ng/ml

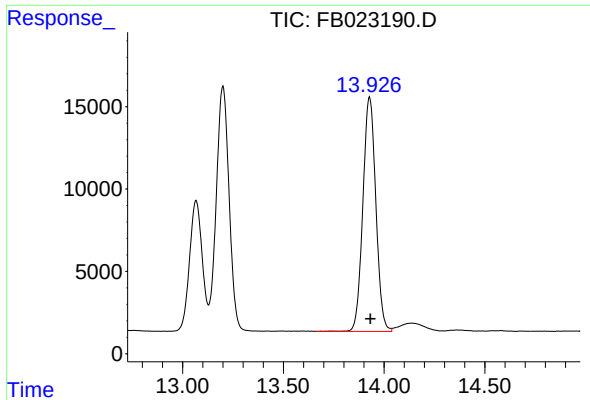

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 634983
Conc: 18.29 ng/ml

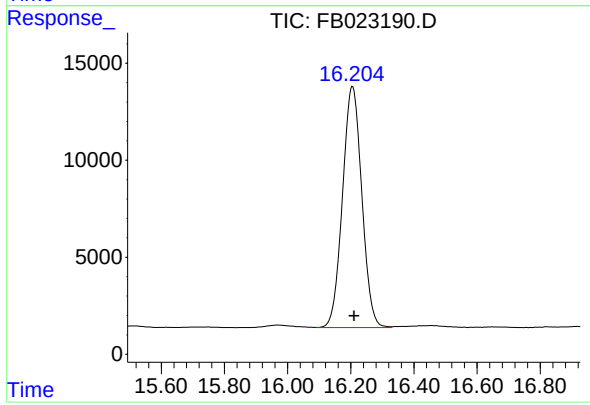

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.005 min
Response: 528075
Conc: 18.83 ng/ml