

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121119\
 Data File : FB023192.D
 Signal(s) : FID2B.CH
 Acq On : 11 Dec 2019 13:59
 Operator : DD/AJ
 Sample : K6242-04MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 12 00:30:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	449351	18.293 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	736579	22.540 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	901882	25.864 ng/ml
3) t n-Heptane	7.754	285823	8.313 ng/ml
4) t Benzene	7.888	369517	8.869 ng/ml
6) t Toluene	10.627	1074478	26.673 ng/ml
7) t Ethylbenzene	13.066	338609	8.775 ng/ml
8) t m-Xylene	13.200	638354	17.542 ng/ml
9) t O-Xylene	13.927	614670	17.703 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	509119	18.155 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121119\
Data File : FB023192.D
Signal(s) : FID2B.CH
Acq On : 11 Dec 2019 13:59
Operator : DD/AJ
Sample : K6242-04MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 12 00:30:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

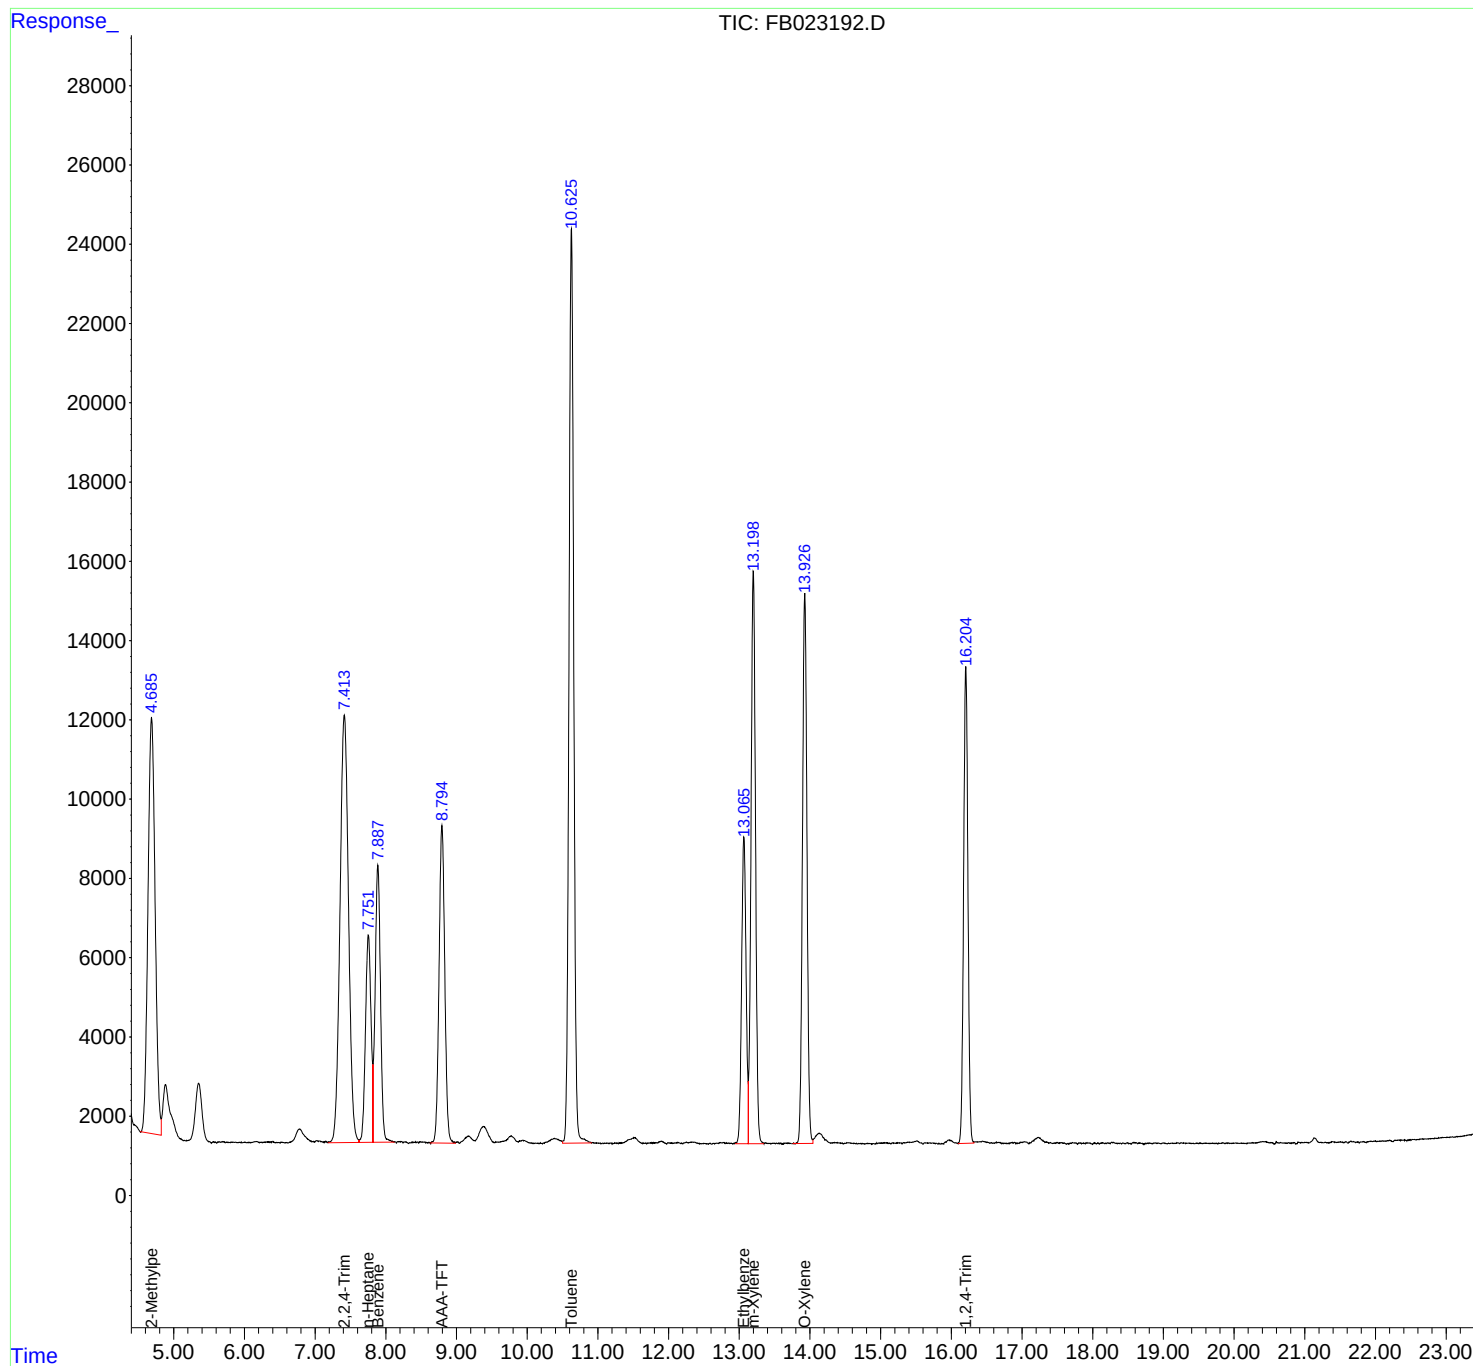

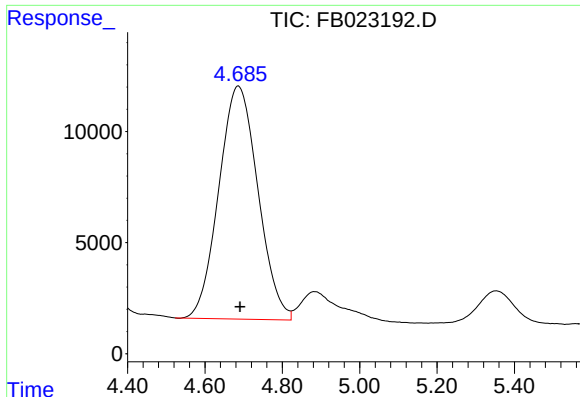


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: -0.004 min
Response: 736579
Conc: 22.54 ng/ml

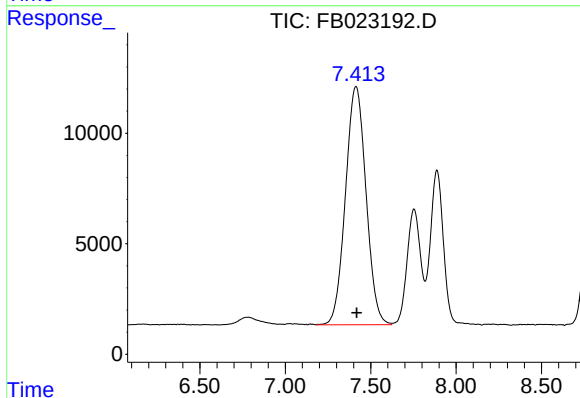


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 901882
Conc: 25.86 ng/ml

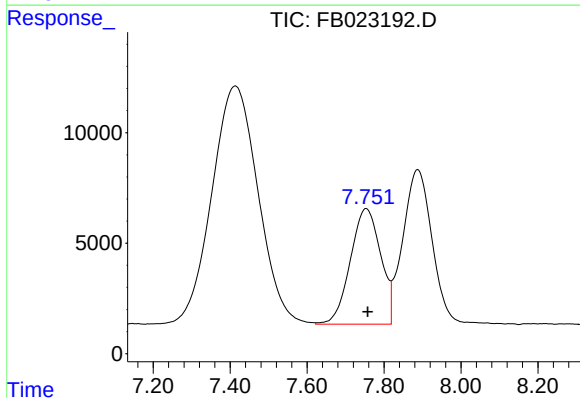


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 285823
Conc: 8.31 ng/ml

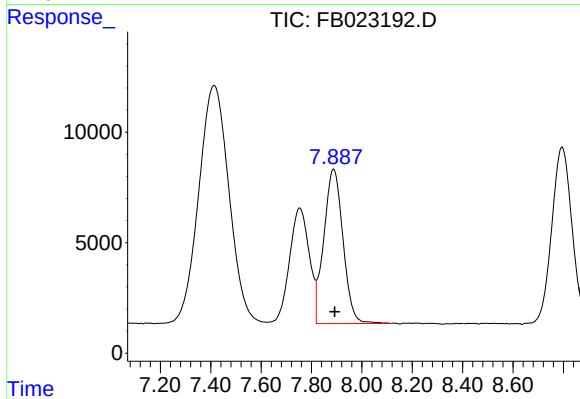


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.004 min
Response: 369517
Conc: 8.87 ng/ml

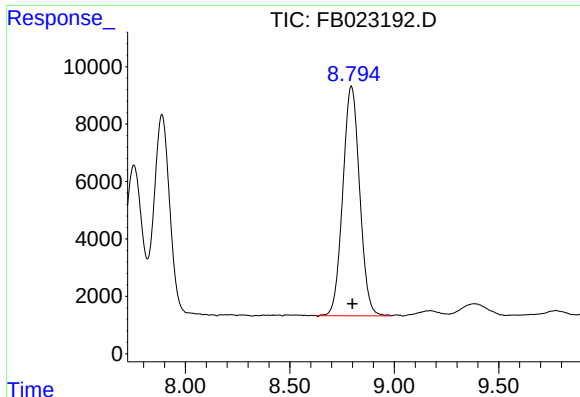


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 449351
Conc: 18.29 ng/ml

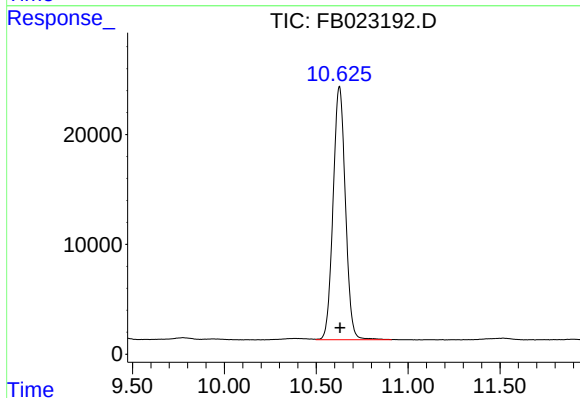


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.004 min
Response: 1074478
Conc: 26.67 ng/ml

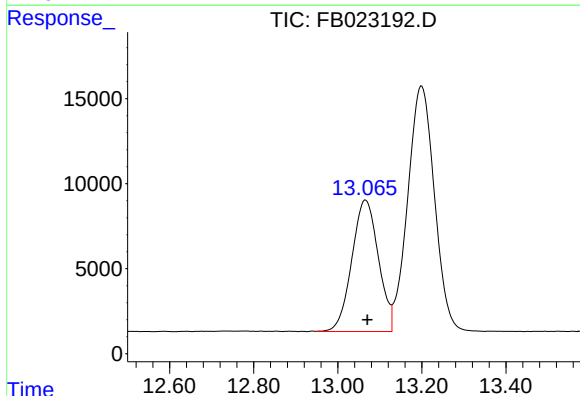


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: -0.004 min
Response: 338609
Conc: 8.77 ng/ml

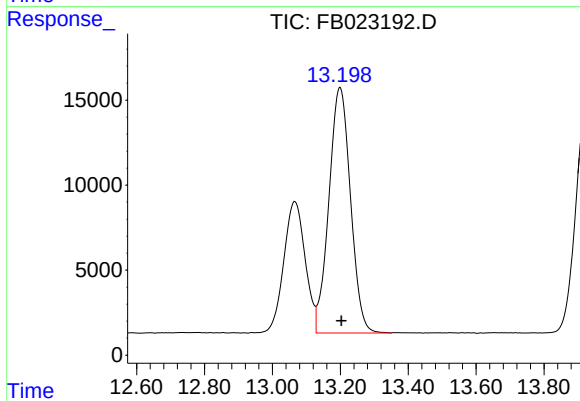


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.004 min
Response: 638354
Conc: 17.54 ng/ml

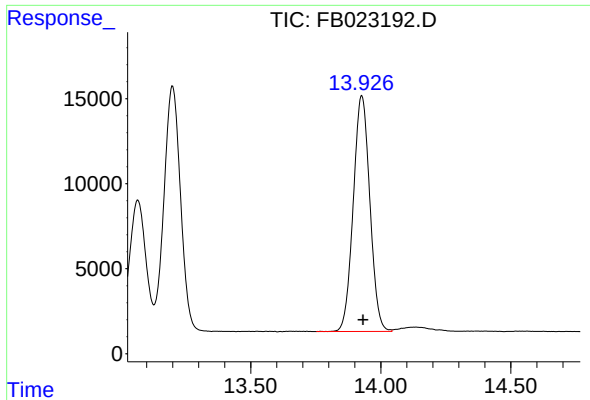

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.004 min
Response: 614670
Conc: 17.70 ng/ml

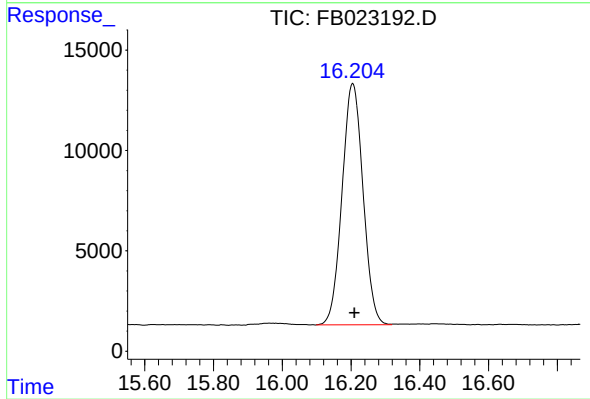

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.005 min
Response: 509119
Conc: 18.15 ng/ml