

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121119\
 Data File : FB023193.D
 Signal(s) : FID2B.CH
 Acq On : 11 Dec 2019 14:29
 Operator : DD/AJ
 Sample : K6242-04MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 12 00:30:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	432324	17.600 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	725164	22.191 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	868200	24.898 ng/ml
3) t n-Heptane	7.755	269192	7.829 ng/ml
4) t Benzene	7.889	365799	8.780 ng/ml
6) t Toluene	10.627	1053512	26.152 ng/ml
7) t Ethylbenzene	13.067	330047	8.553 ng/ml
8) t m-Xylene	13.200	620902	17.063 ng/ml
9) t O-Xylene	13.928	599954	17.279 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	494792	17.644 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121119\
Data File : FB023193.D
Signal(s) : FID2B.CH
Acq On : 11 Dec 2019 14:29
Operator : DD/AJ
Sample : K6242-04MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 12 00:30:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

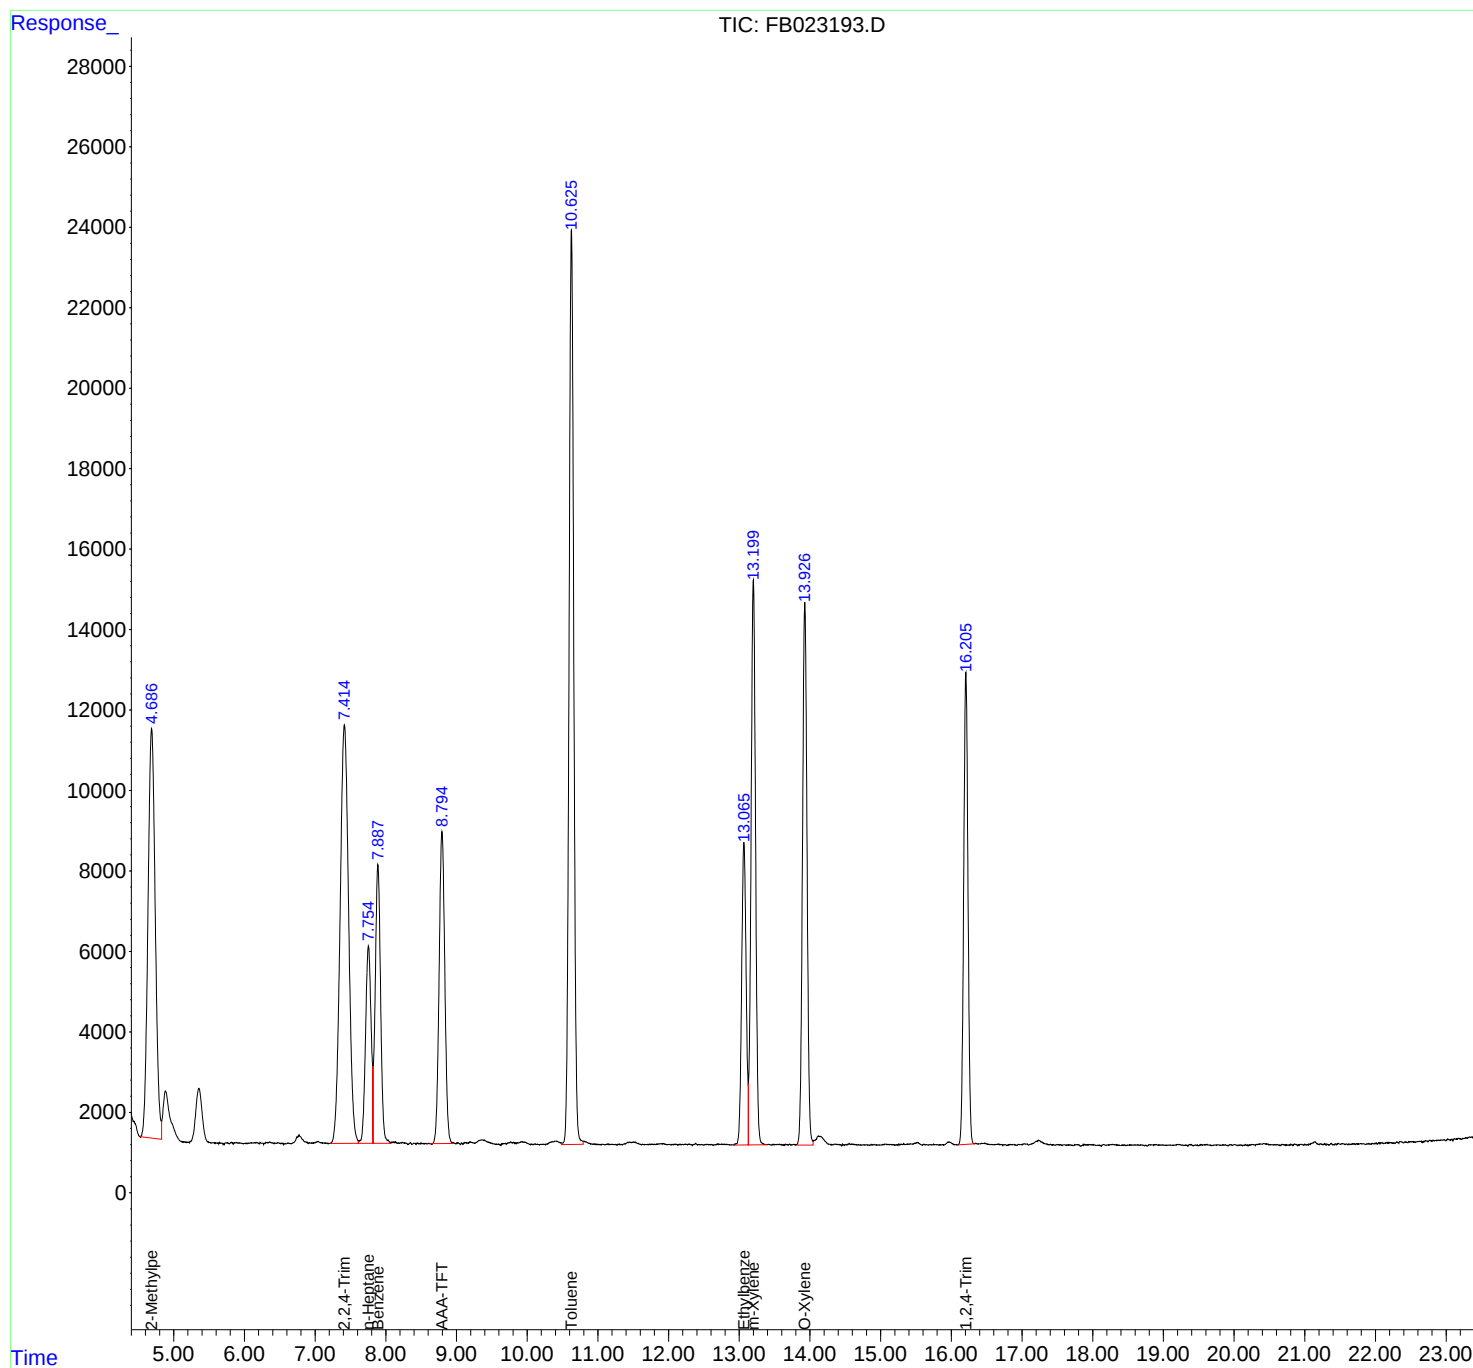

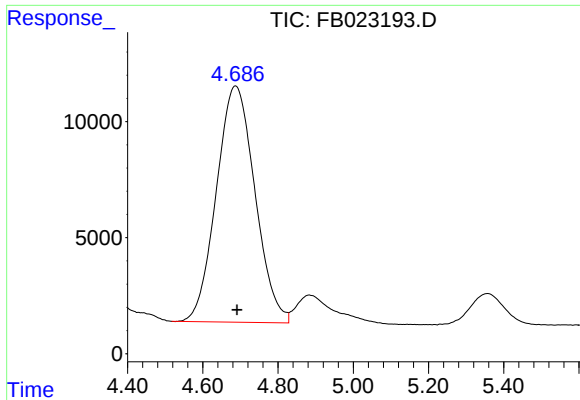


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 725164
Conc: 22.19 ng/ml

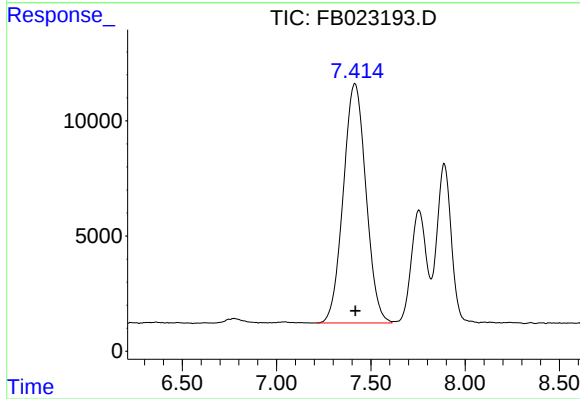


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 868200
Conc: 24.90 ng/ml

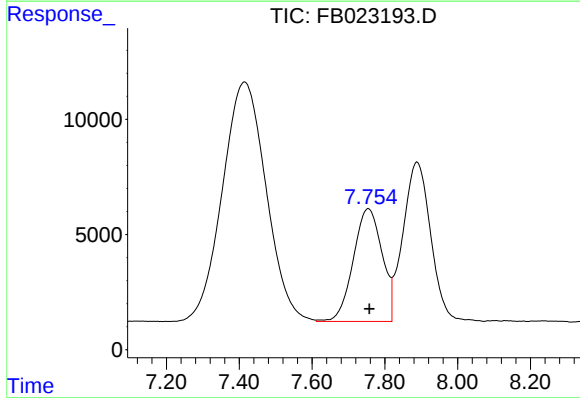


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 269192
Conc: 7.83 ng/ml

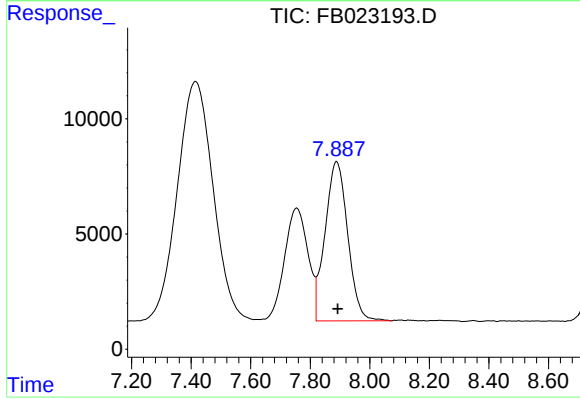


#4 Benzene

R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 365799
Conc: 8.78 ng/ml

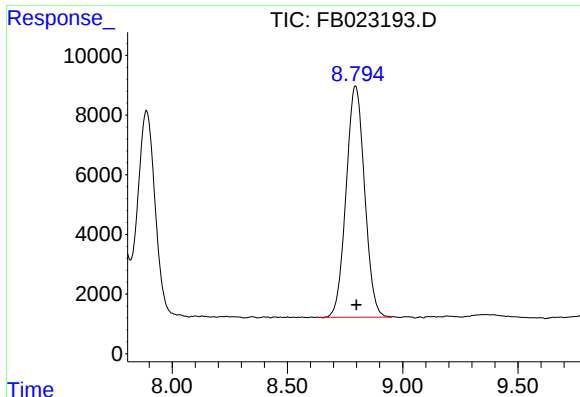


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 432324
Conc: 17.60 ng/ml

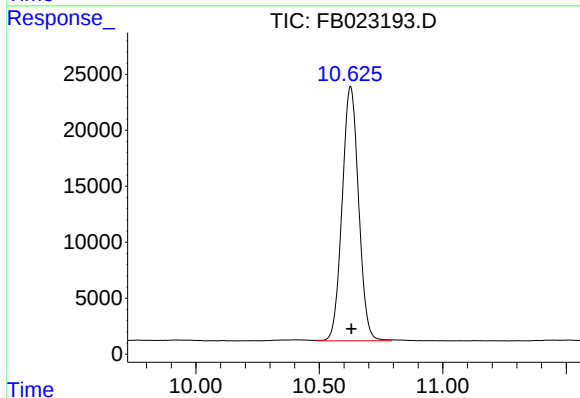


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.004 min
Response: 1053512
Conc: 26.15 ng/ml

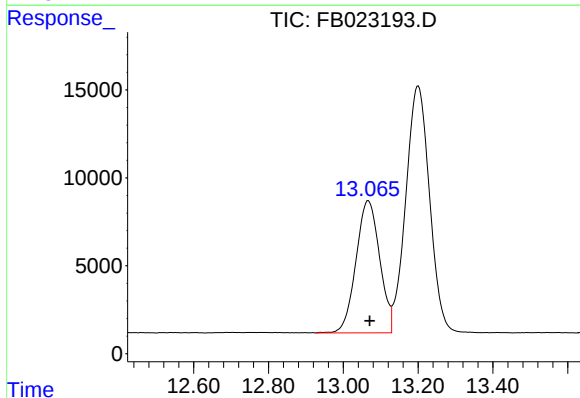


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.004 min
Response: 330047
Conc: 8.55 ng/ml

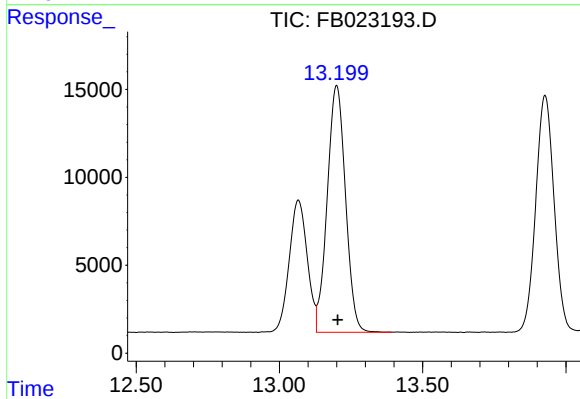

#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.003 min
Response: 620902
Conc: 17.06 ng/ml

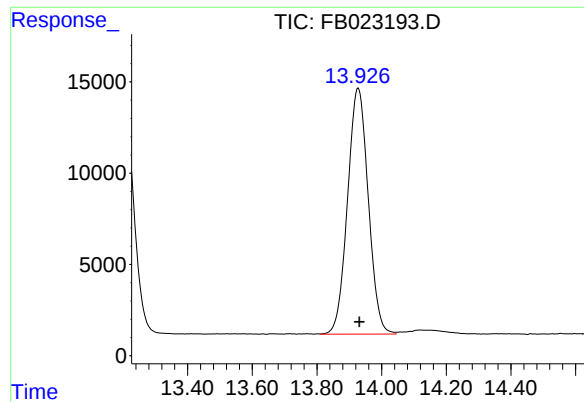


#9 O-Xylene

R.T.: 13.928 min

Delta R.T.: -0.004 min

Response: 599954

Conc: 17.28 ng/ml

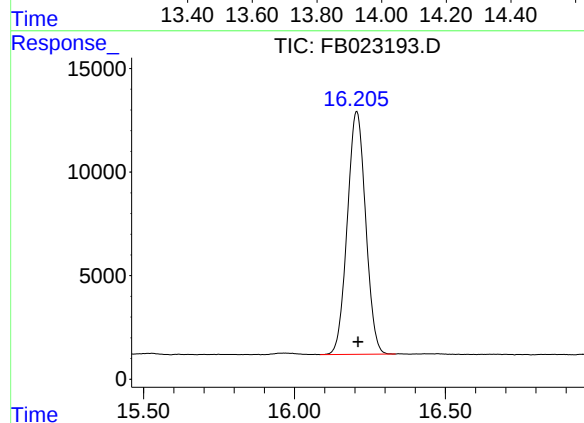

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min

Delta R.T.: -0.004 min

Response: 494792

Conc: 17.64 ng/ml