

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121120\
 Data File : FB025337.D
 Signal(s) : FID2B.CH
 Acq On : 11 Dec 2020 12:44
 Operator : DD/AJ
 Sample : L5042-04MS
 Misc : 4.99g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 KENS-B6-121020-0-6MS

Integration File: SAMPLE.e
 Quant Time: Dec 11 21:58:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	474773	22.583 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	892738	29.695 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	913416	30.357 ng/ml
3) t n-Heptane	7.759	302039	10.200 ng/ml
4) t Benzene	7.893	370153	10.007 ng/ml
6) t Toluene	10.631	1058377	30.118 ng/ml
7) t Ethylbenzene	13.070	326239	9.988 ng/ml
8) t m-Xylene	13.203	648230	20.028 ng/ml
9) t O-Xylene	13.931	628107	19.869 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	550163	20.260 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121120\
Data File : FB025337.D
Signal(s) : FID2B.CH
Acq On : 11 Dec 2020 12:44
Operator : DD/AJ
Sample : L5042-04MS
Misc : 4.99g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-B6-121020-0-6MS

Integration File: SAMPLE.e
Quant Time: Dec 11 21:58:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

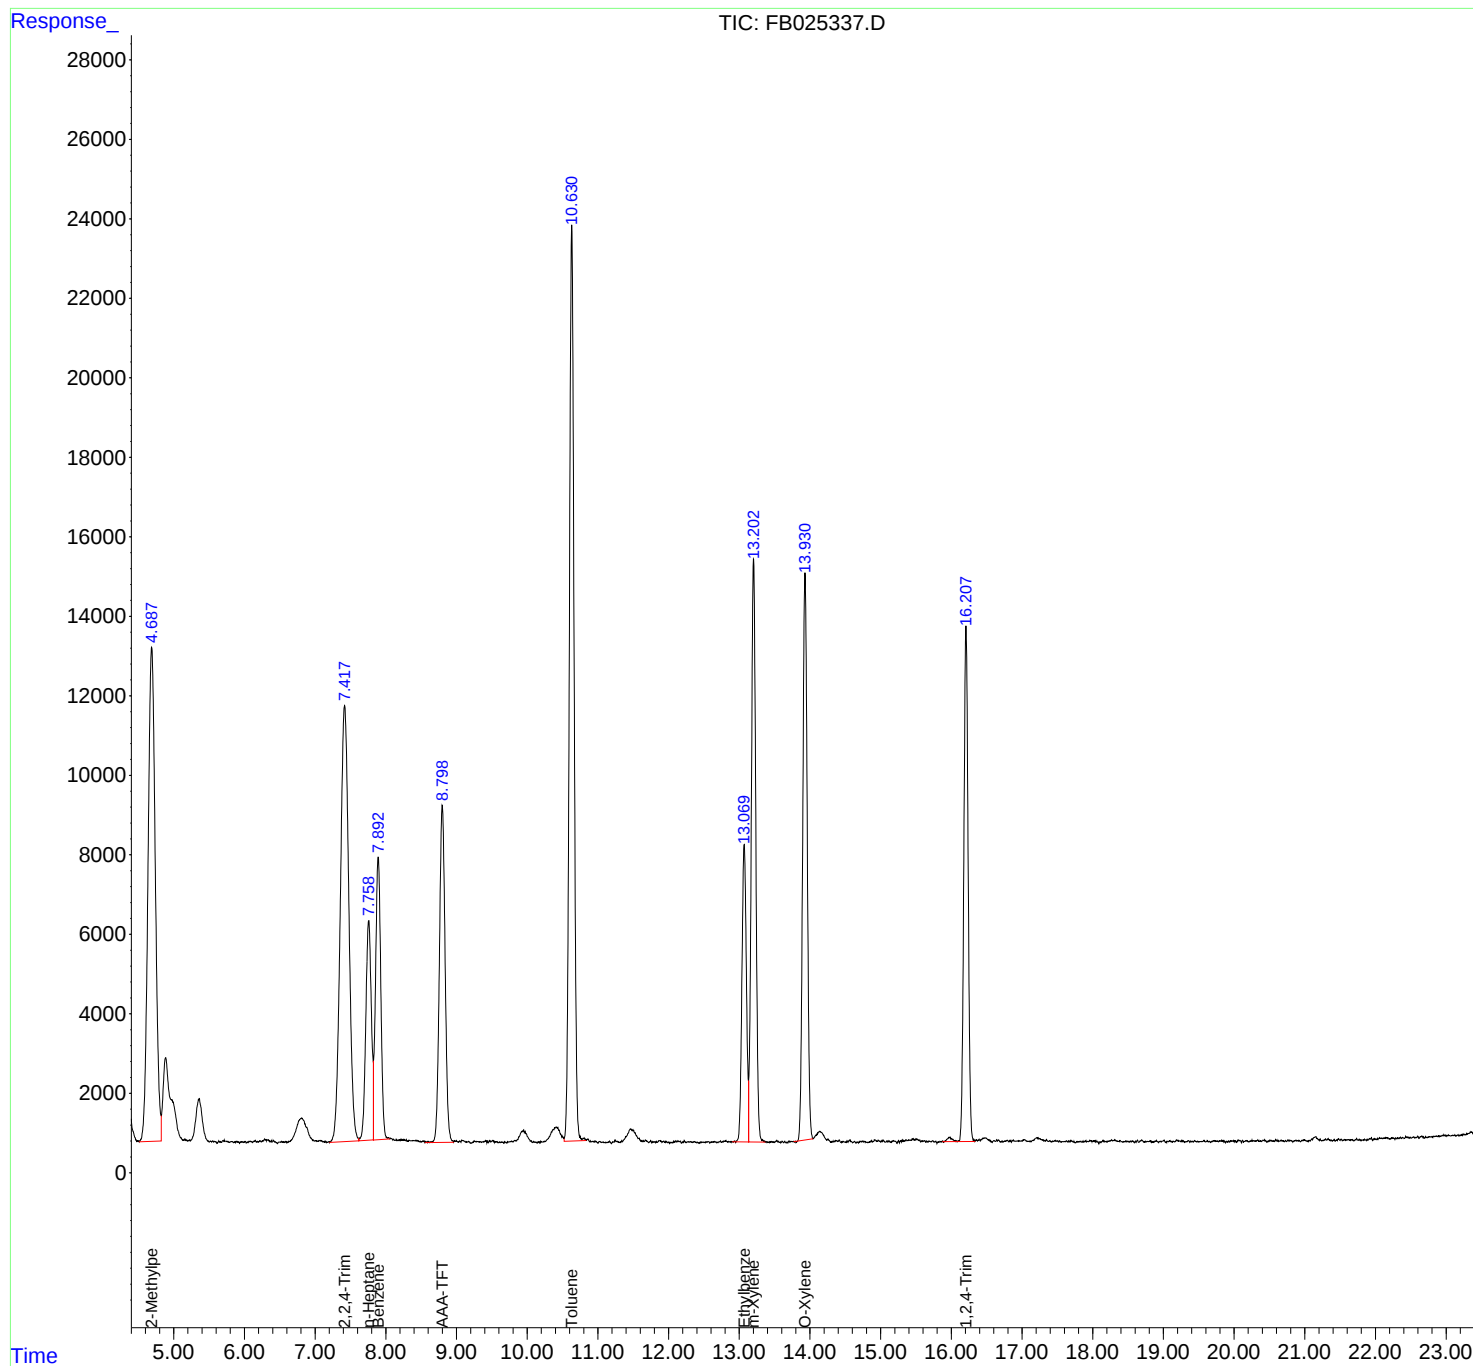


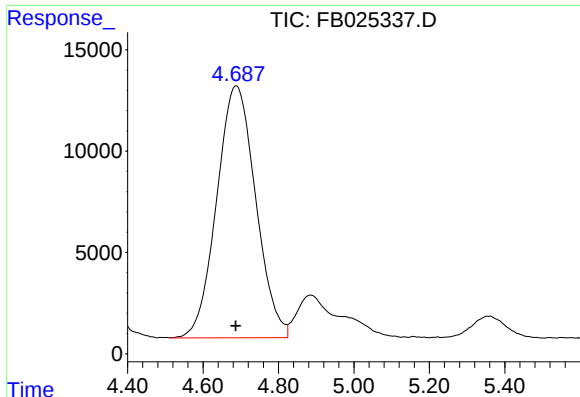

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.001 min
Response: 892738
Conc: 29.69 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B6-121020-0-6MS

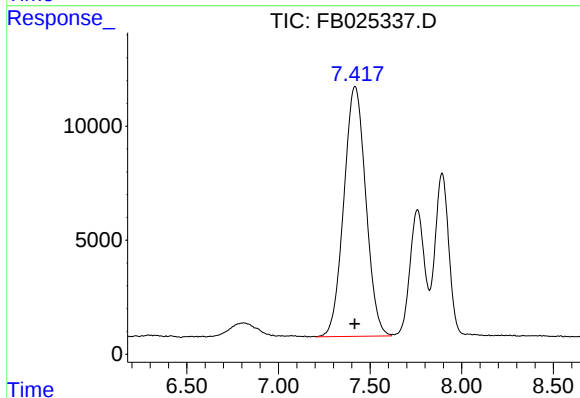


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.002 min
Response: 913416
Conc: 30.36 ng/ml

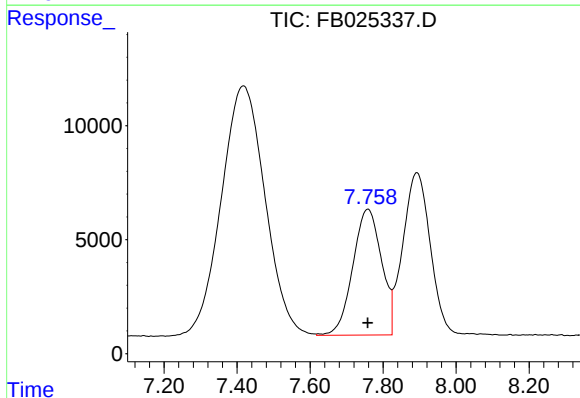


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.001 min
Response: 302039
Conc: 10.20 ng/ml

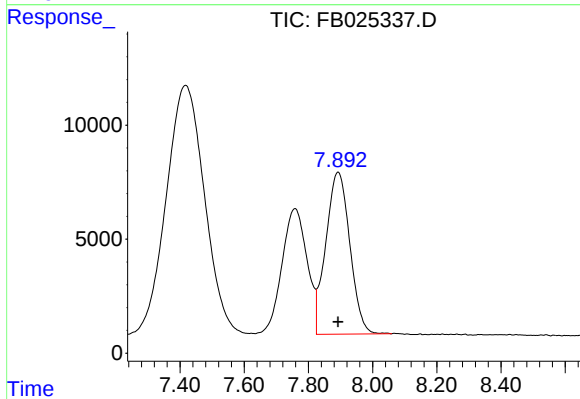

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 370153
Conc: 10.01 ng/ml

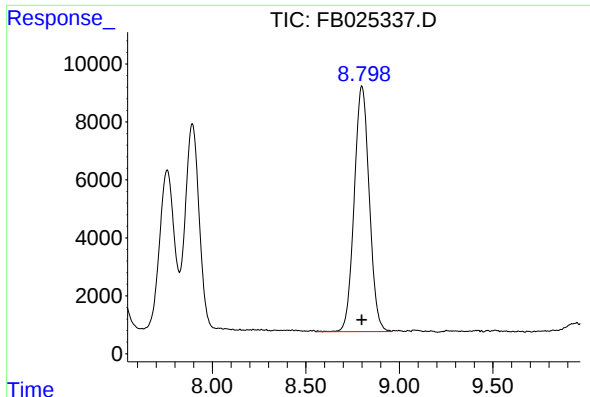

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 474773
Conc: 22.58 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B6-121020-0-6MS

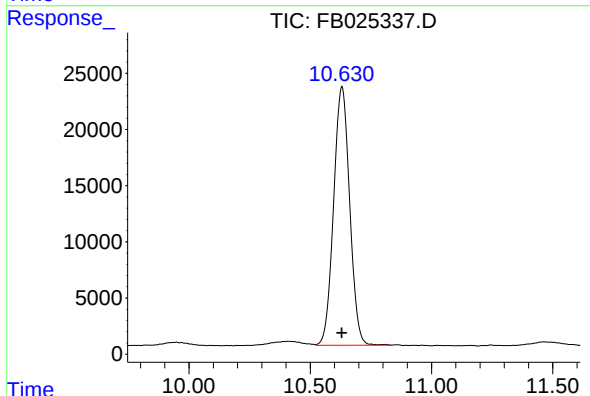


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1058377
Conc: 30.12 ng/ml

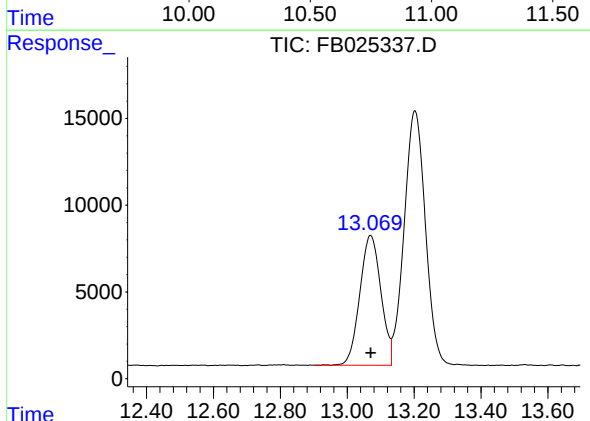


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 326239
Conc: 9.99 ng/ml

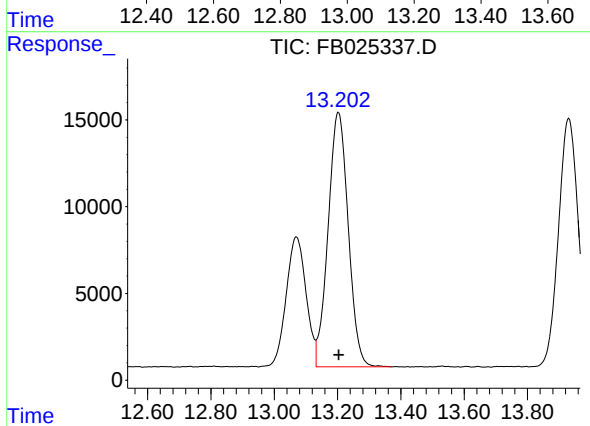

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 648230
Conc: 20.03 ng/ml

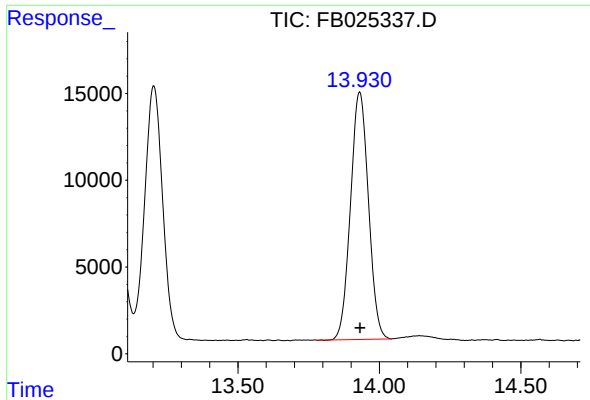

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 628107
Conc: 19.87 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B6-121020-0-6MS

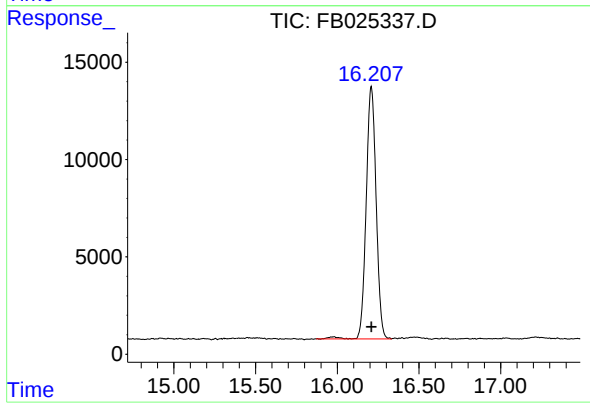

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.001 min
Response: 550163
Conc: 20.26 ng/ml