

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121120\
 Data File : FB025338.D
 Signal(s) : FID2B.CH
 Acq On : 11 Dec 2020 13:15
 Operator : DD/AJ
 Sample : L5042-06MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 KENS-B6-121020-0-6MSD

Integration File: SAMPLE.e
 Quant Time: Dec 11 21:58:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	513476	24.424 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	895068	29.772 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	883195	29.352 ng/ml
3) t n-Heptane	7.756	294988	9.962 ng/ml
4) t Benzene	7.892	377336	10.202 ng/ml
6) t Toluene	10.630	1073673	30.554 ng/ml
7) t Ethylbenzene	13.070	329086	10.075 ng/ml
8) t m-Xylene	13.203	656990	20.298 ng/ml
9) t O-Xylene	13.930	632507	20.008 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	549624	20.240 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121120\
Data File : FB025338.D
Signal(s) : FID2B.CH
Acq On : 11 Dec 2020 13:15
Operator : DD/AJ
Sample : L5042-06MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-B6-121020-0-6MSD

Integration File: SAMPLE.e
Quant Time: Dec 11 21:58:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

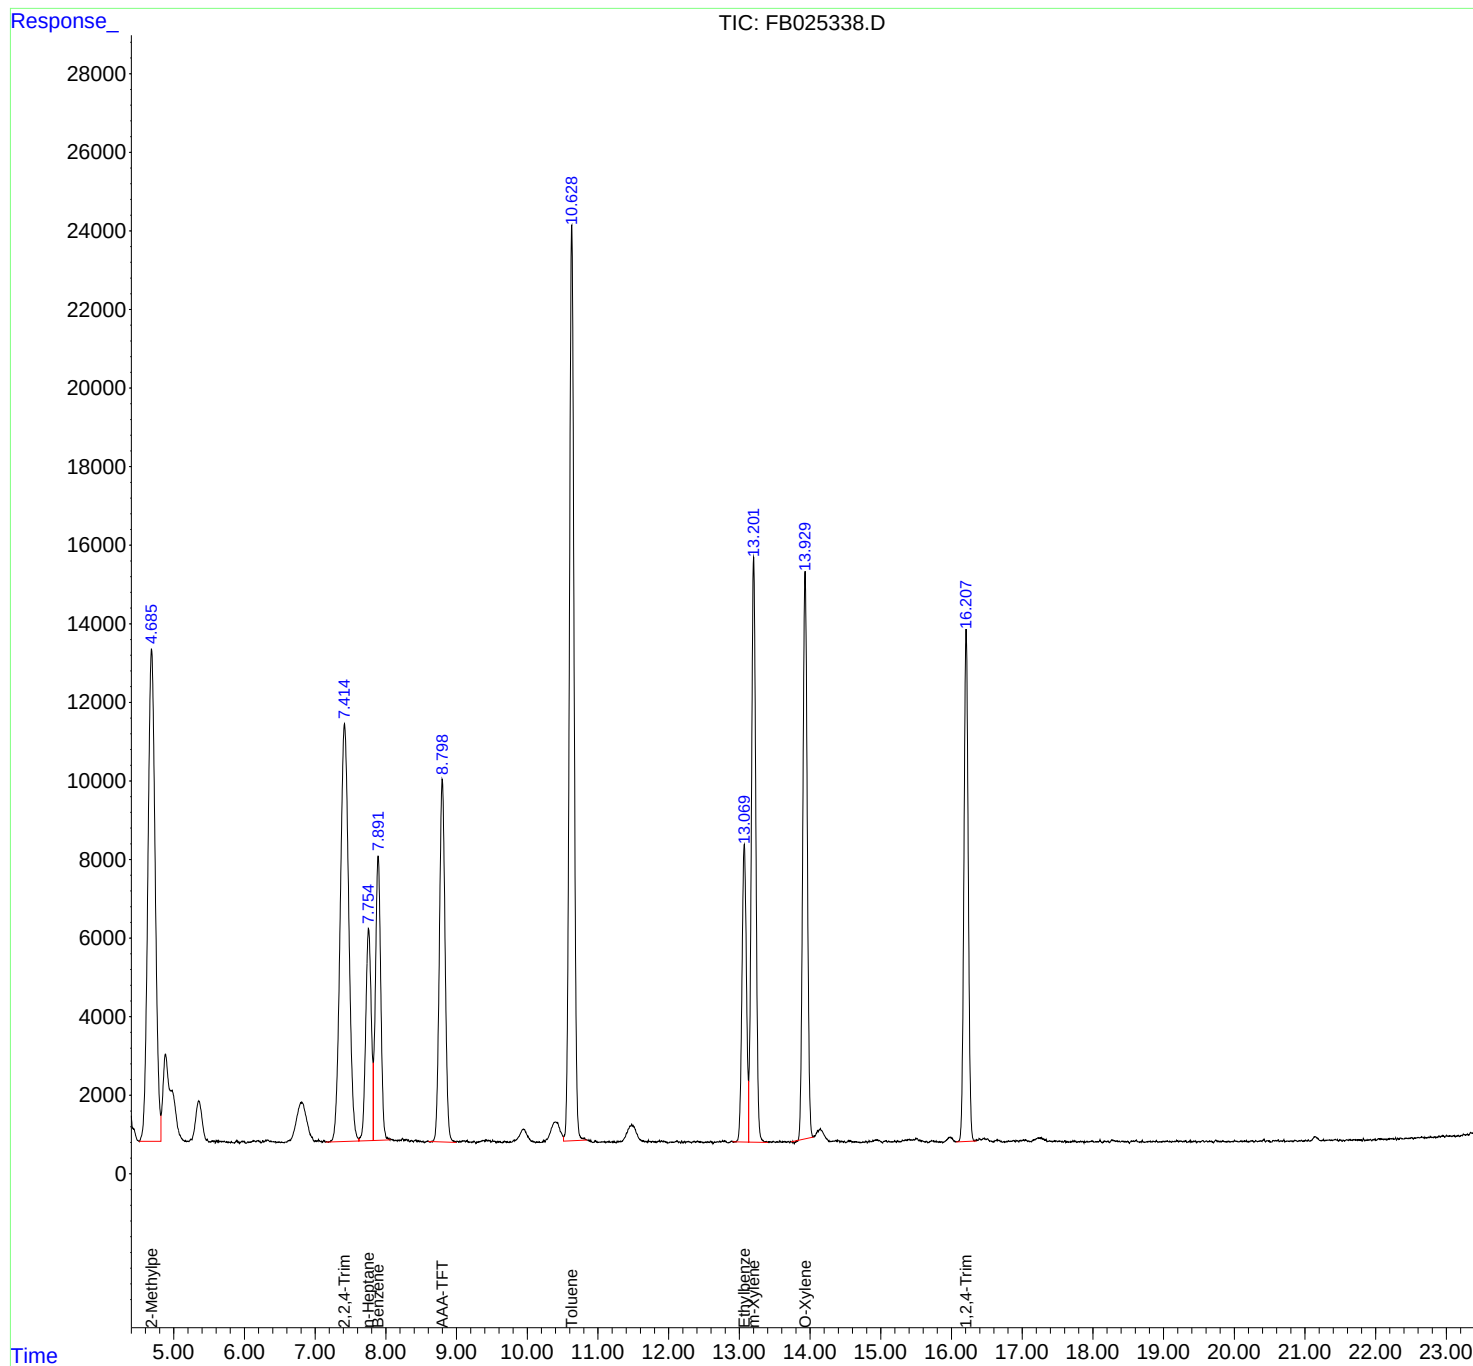


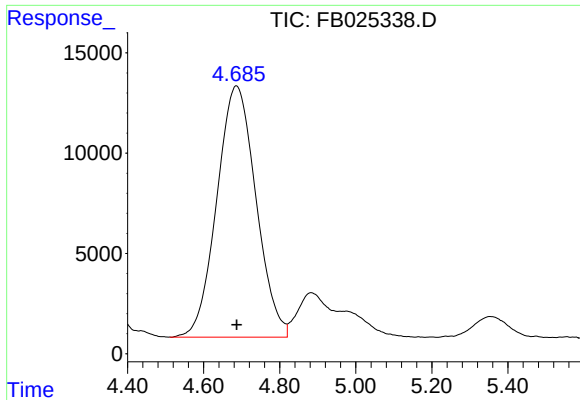

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 895068
Conc: 29.77 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B6-121020-0-6MSD

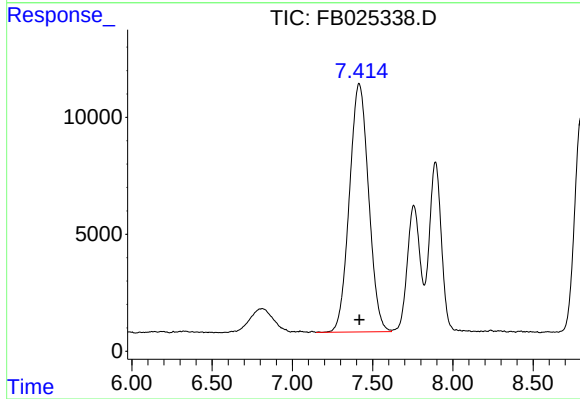


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 883195
Conc: 29.35 ng/ml

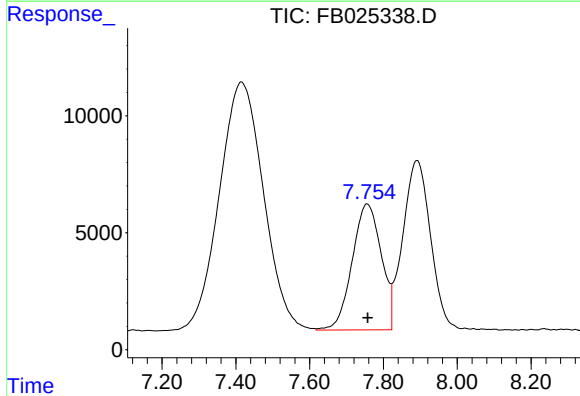


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 294988
Conc: 9.96 ng/ml

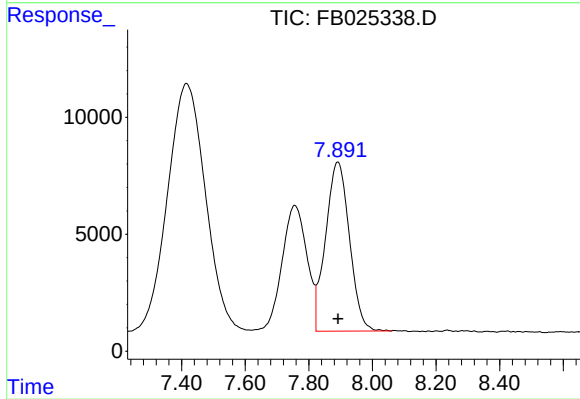

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 377336
Conc: 10.20 ng/ml

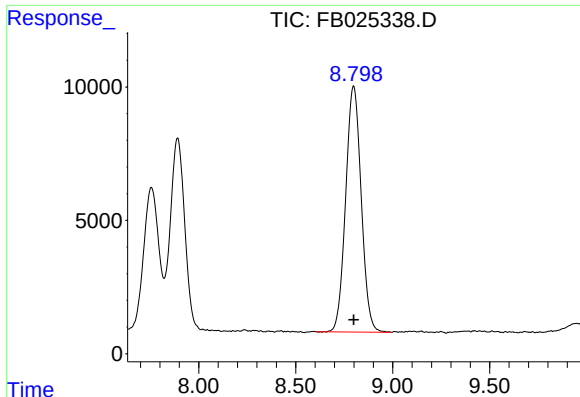

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 513476
Conc: 24.42 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B6-121020-0-6MSD

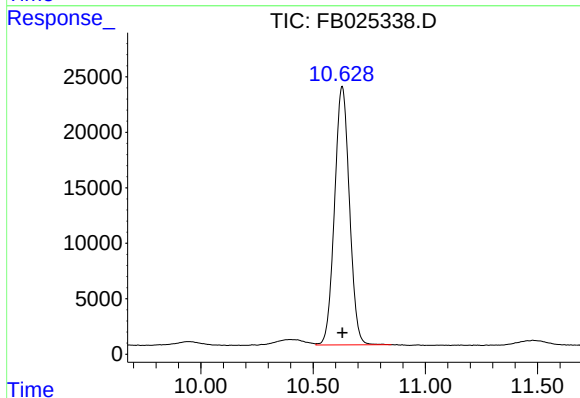


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1073673
Conc: 30.55 ng/ml

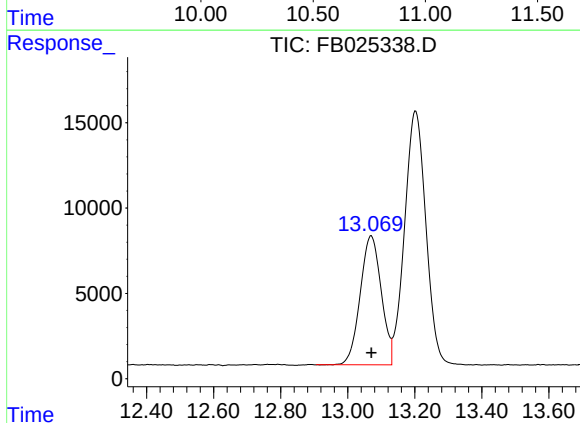


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 329086
Conc: 10.07 ng/ml

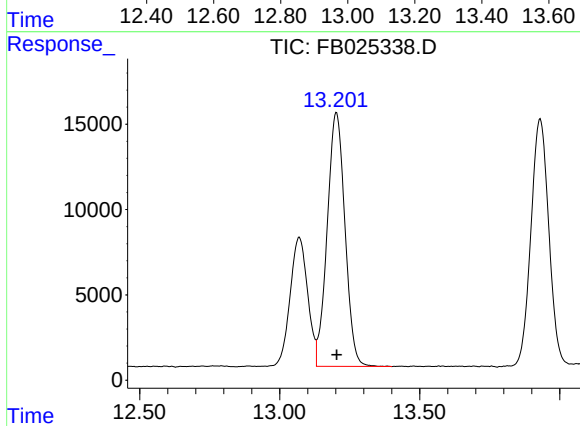

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 656990
Conc: 20.30 ng/ml

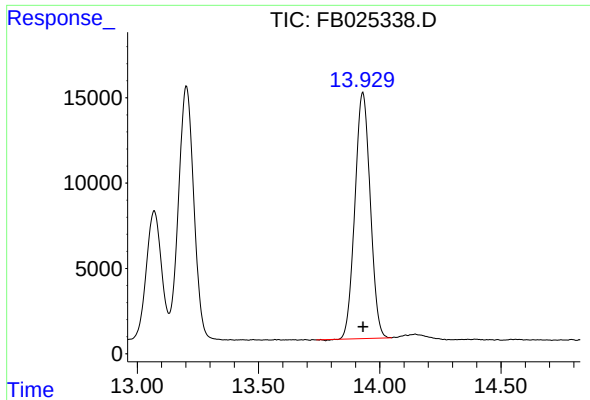

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.001 min
Response: 632507
Conc: 20.01 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B6-121020-0-6MSD

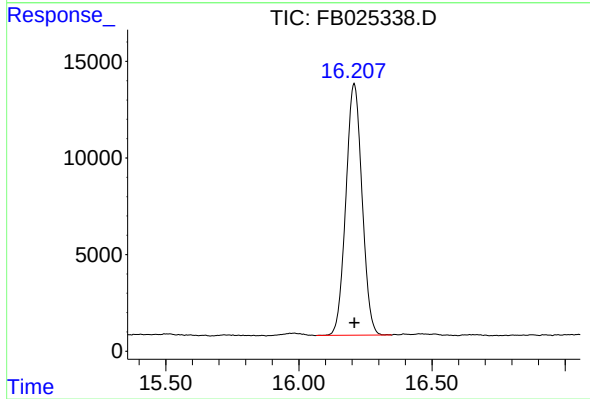

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.001 min
Response: 549624
Conc: 20.24 ng/ml