

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121120\
 Data File : FB025341.D
 Signal(s) : FID2B.CH
 Acq On : 11 Dec 2020 14:46
 Operator : DD/AJ
 Sample : L5043-08MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 KENS-SS2-121020-0-7MSD

Integration File: SAMPLE.e
 Quant Time: Dec 11 21:59:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	526702	25.053 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	874699	29.095 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	831686	27.641 ng/ml
3) t n-Heptane	7.757	273805	9.246 ng/ml
4) t Benzene	7.892	383135	10.358 ng/ml
6) t Toluene	10.630	1081219	30.768 ng/ml
7) t Ethylbenzene	13.071	330435	10.116 ng/ml
8) t m-Xylene	13.204	657772	20.323 ng/ml
9) t O-Xylene	13.931	637370	20.162 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	542472	19.977 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121120\
Data File : FB025341.D
Signal(s) : FID2B.CH
Acq On : 11 Dec 2020 14:46
Operator : DD/AJ
Sample : L5043-08MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-SS2-121020-0-7MSD

Integration File: SAMPLE.e
Quant Time: Dec 11 21:59:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

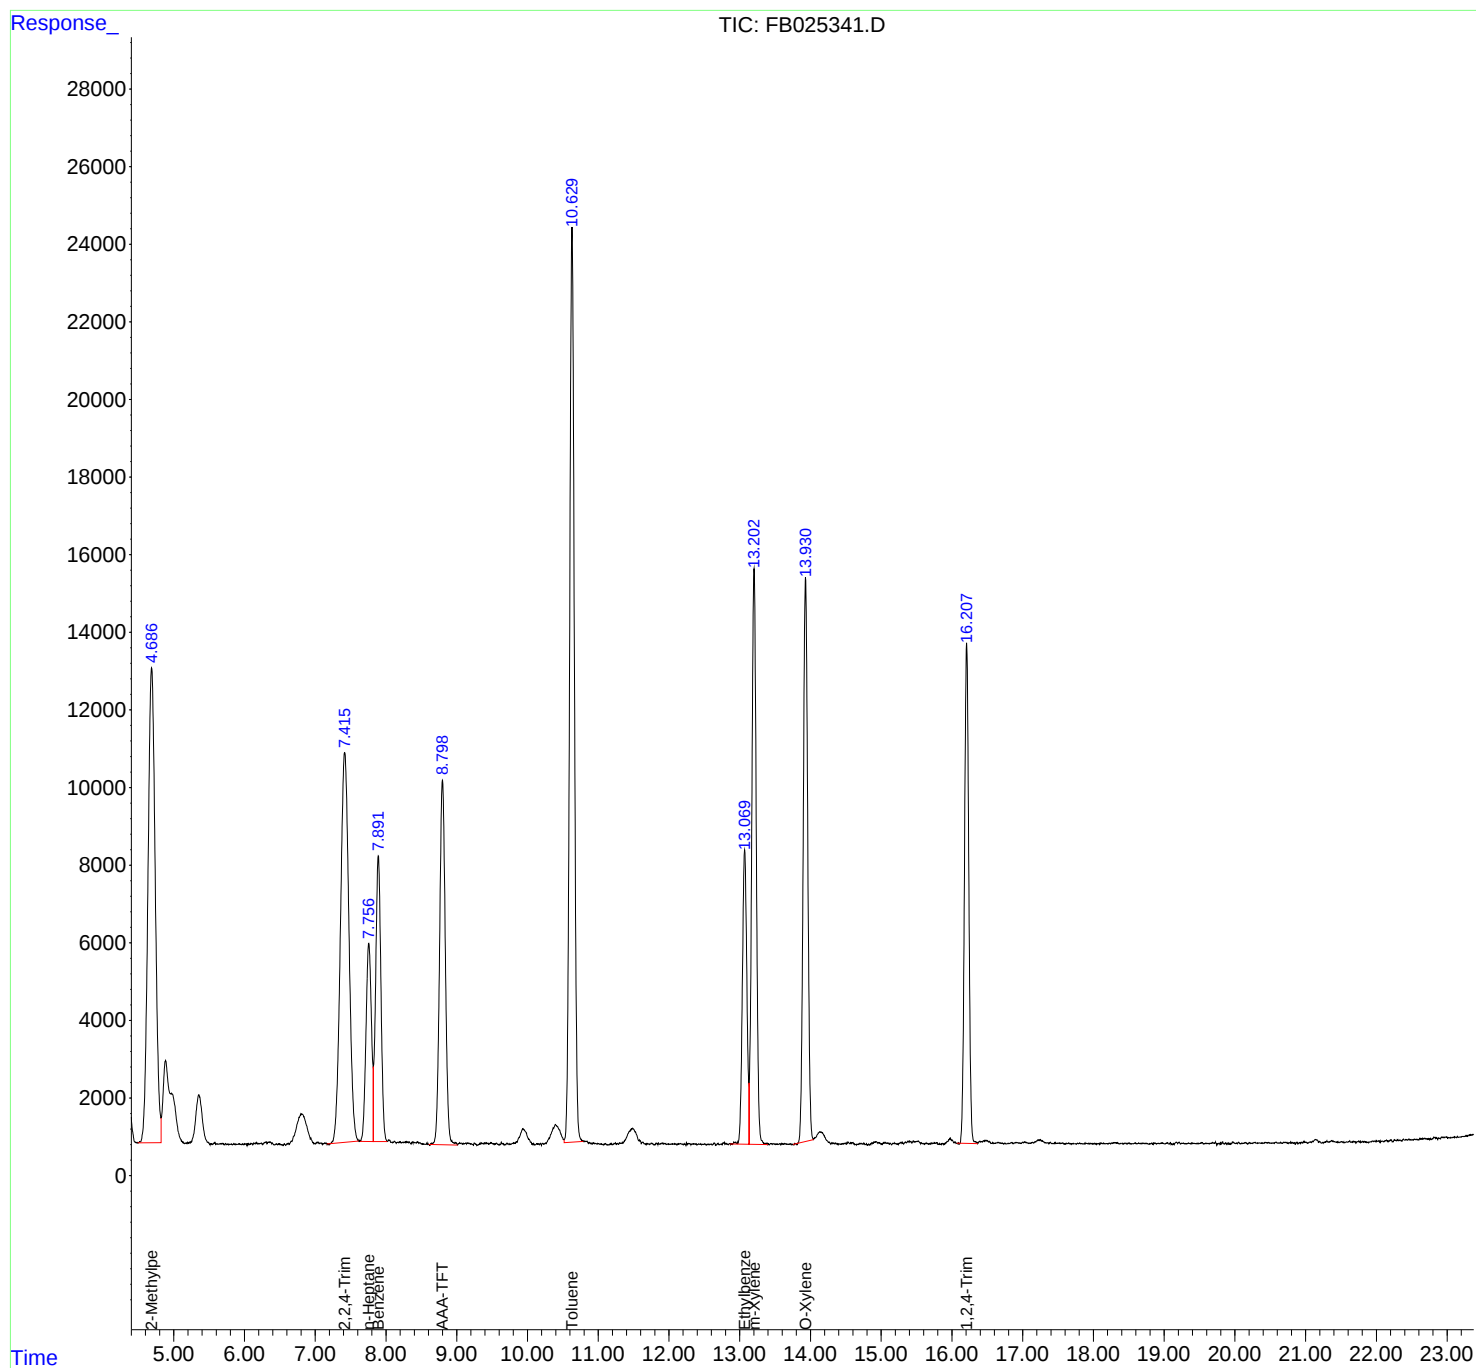


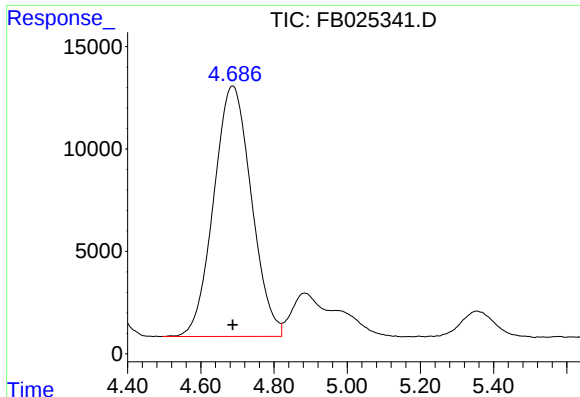

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 874699
Conc: 29.09 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-SS2-121020-0-7MSD

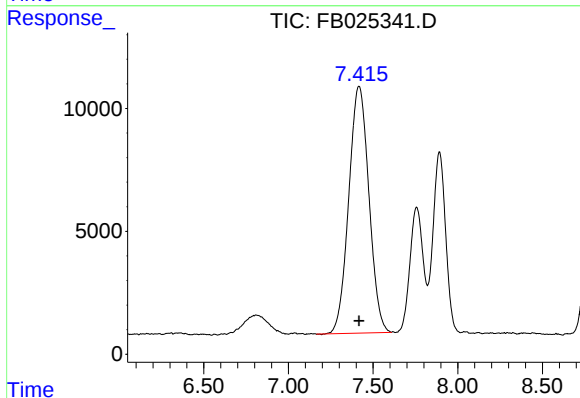


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 831686
Conc: 27.64 ng/ml

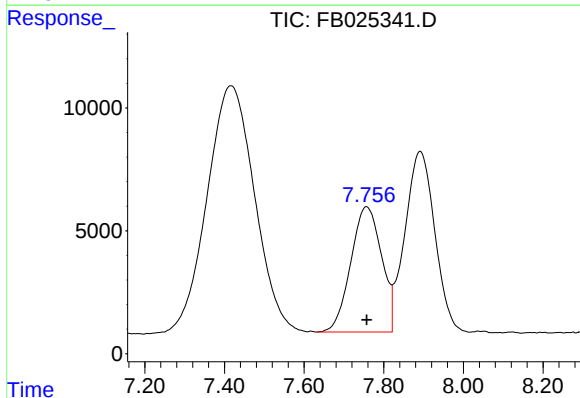


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 273805
Conc: 9.25 ng/ml

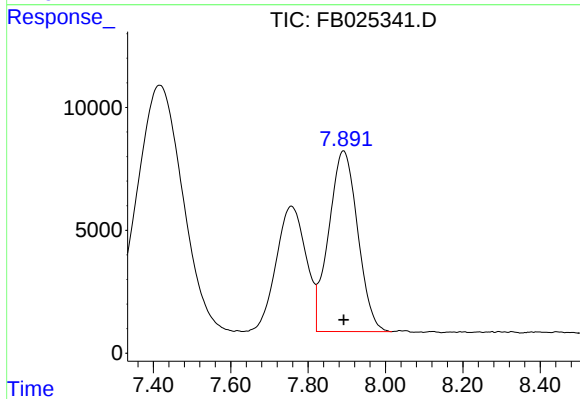

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 383135
Conc: 10.36 ng/ml

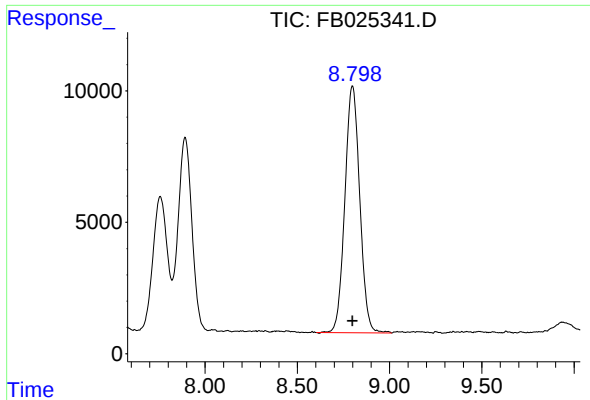

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 526702
Conc: 25.05 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-SS2-121020-0-7MSD

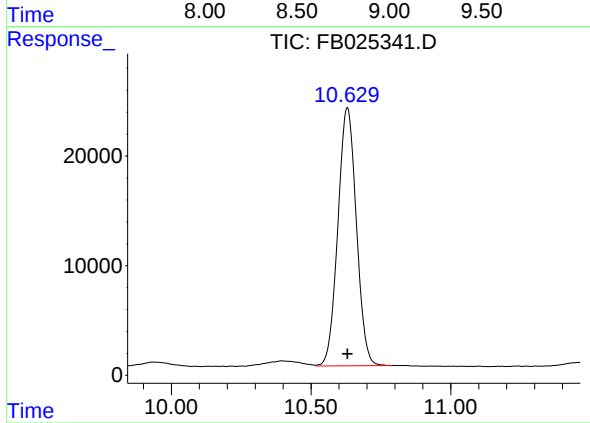


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1081219
Conc: 30.77 ng/ml

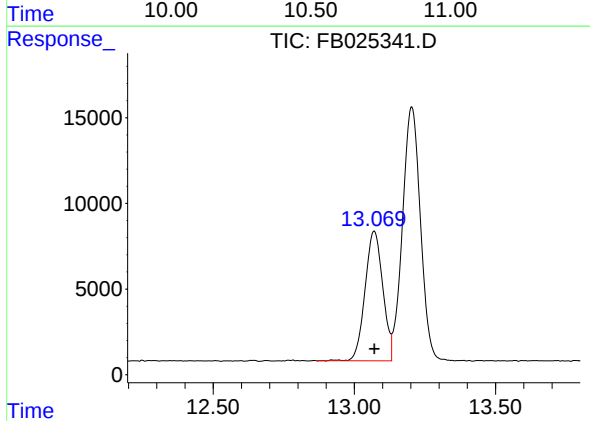


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 330435
Conc: 10.12 ng/ml

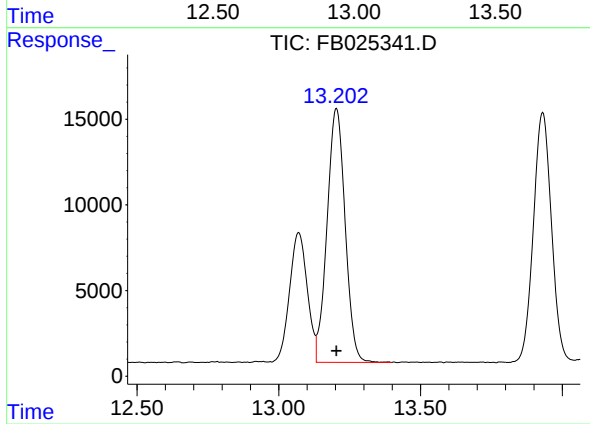

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 657772
Conc: 20.32 ng/ml

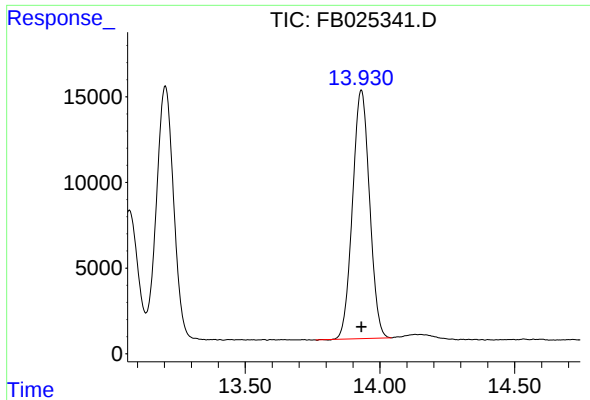

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 637370
Conc: 20.16 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-SS2-121020-0-7MSD

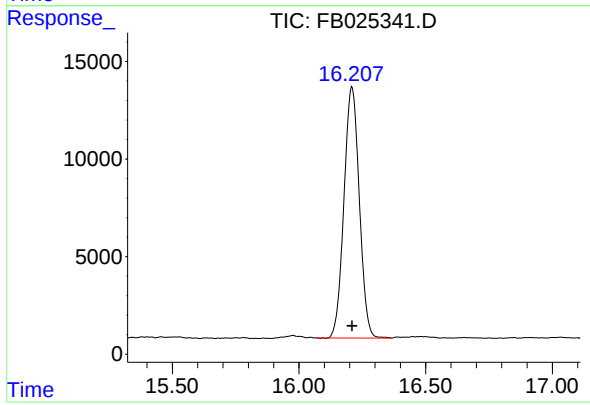

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 542472
Conc: 19.98 ng/ml