

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121120\
Data File : FB025343.D
Signal(s) : FID2B.CH
Acq On : 11 Dec 2020 15:48
Operator : DD/AJ
Sample : L5043-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-SS1-121020-0-7

Integration File: SAMPLE.e
Quant Time: Dec 11 21:59:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	448270	21.323 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121120\
Data File : FB025343.D
Signal(s) : FID2B.CH
Acq On : 11 Dec 2020 15:48
Operator : DD/AJ
Sample : L5043-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-SS1-121020-0-7

Integration File: SAMPLE.e
Quant Time: Dec 11 21:59:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

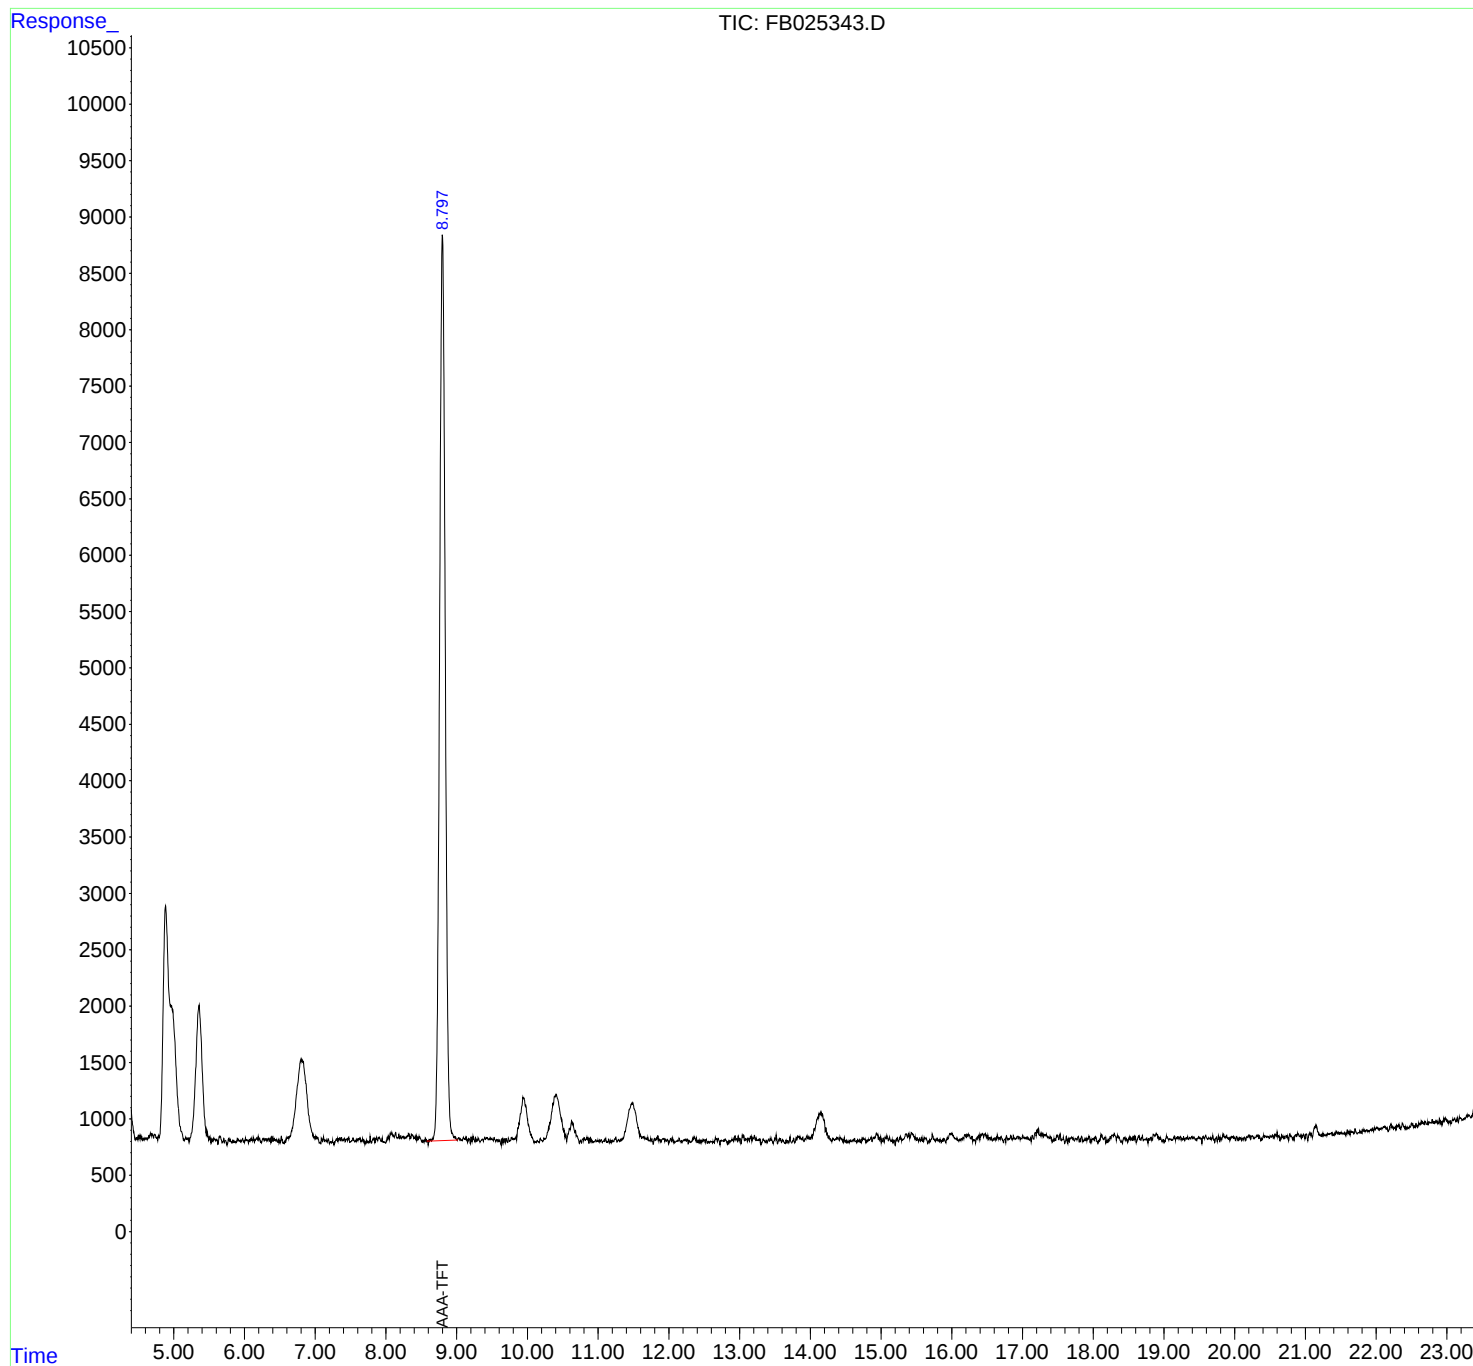

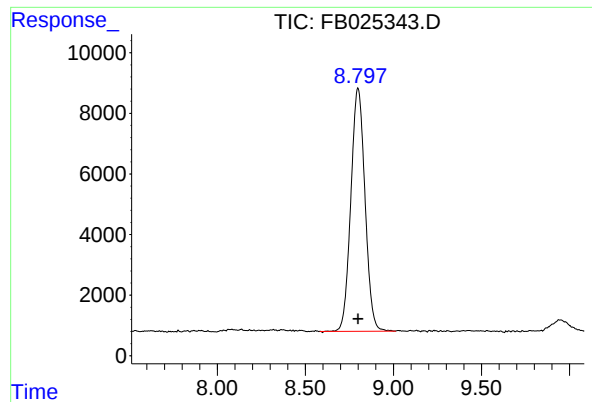

#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 448270
Conc: 21.32 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-SS1-121020-0-7