

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB121218\
Data File : FB019037.D
Signal(s) : FID2B.CH
Acq On : 12 Dec 2018 9:05
Operator : MJ/SJ
Sample : BSF1212S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 12 13:35:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.108	176858	20.234 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.960	453639	29.674 ng/ml
2) t	2,2,4-Trimethylpentane	7.724	470339	30.530 ng/ml
3) t	n-Heptane	8.063	149276	10.043 ng/ml
4) t	Benzene	8.202	189092	10.498 ng/ml
6) t	Toluene	10.957	467749	30.815 ng/ml
7) t	Ethylbenzene	13.407	158744	10.218 ng/ml
8) t	m-Xylene	13.539	336907	20.680 ng/ml
9) t	O-Xylene	14.271	349801	20.688 ng/ml
10) t	1,2,4-Trimethylbenzene	16.554	417748	20.642 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB121218\
Data File : FB019037.D
Signal(s) : FID2B.CH
Acq On : 12 Dec 2018 9:05
Operator : MJ/SJ
Sample : BSF1212S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 12 13:35:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

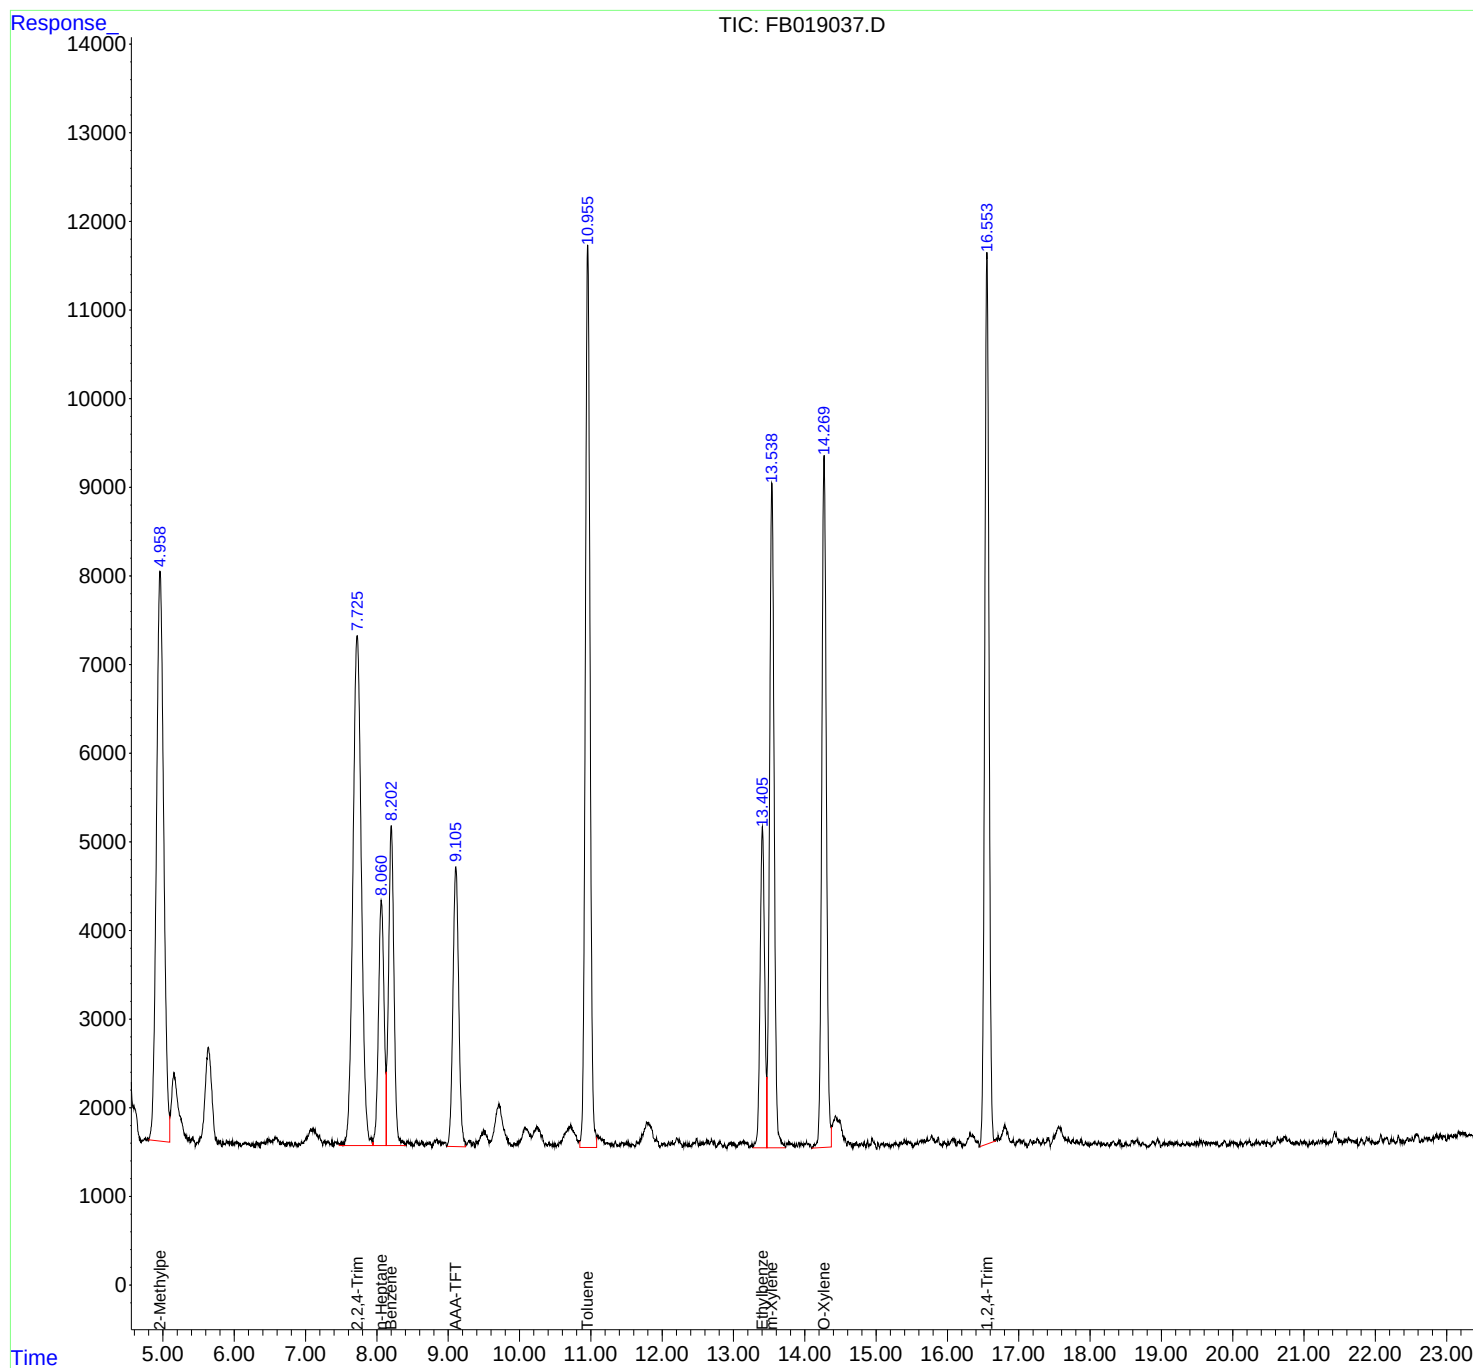

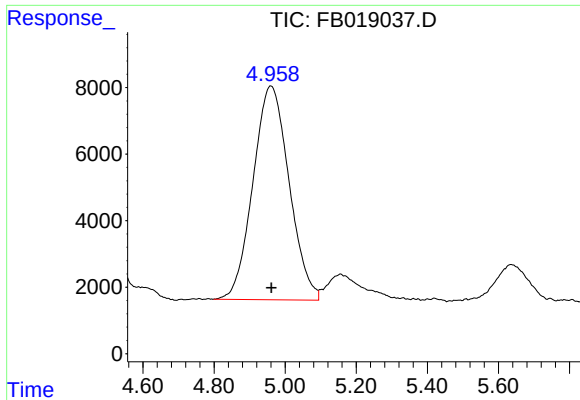


#1 2-Methylpentane

R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 453639
Conc: 29.67 ng/ml

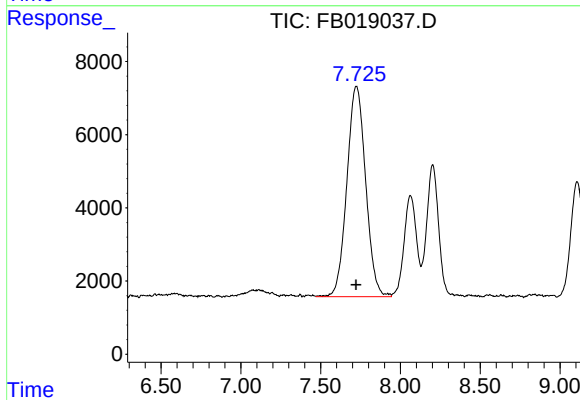


#2 2,2,4-Trimethylpentane

R.T.: 7.724 min
Delta R.T.: 0.000 min
Response: 470339
Conc: 30.53 ng/ml

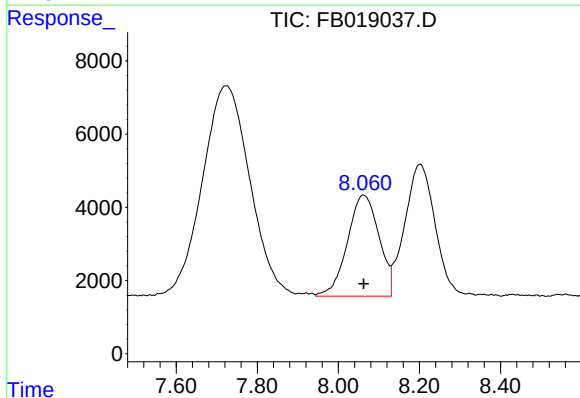


#3 n-Heptane

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 149276
Conc: 10.04 ng/ml

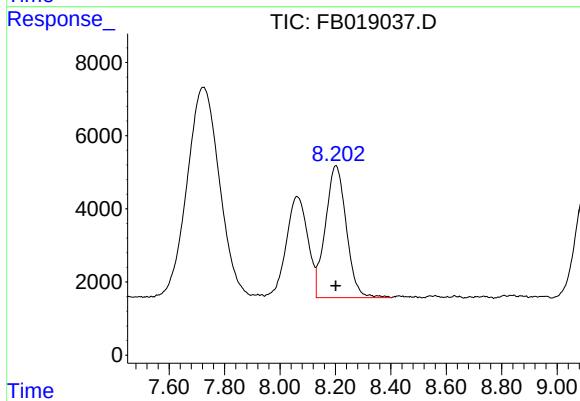


#4 Benzene

R.T.: 8.202 min
Delta R.T.: 0.001 min
Response: 189092
Conc: 10.50 ng/ml

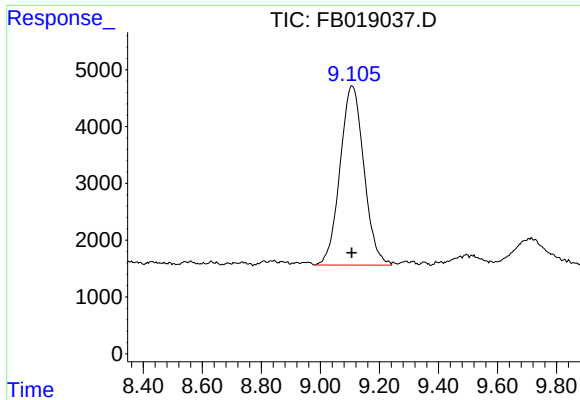


#5 AAA-TFT

R.T.: 9.108 min
 Delta R.T.: 0.001 min
 Response: 176858
 Conc: 20.23 ng/ml

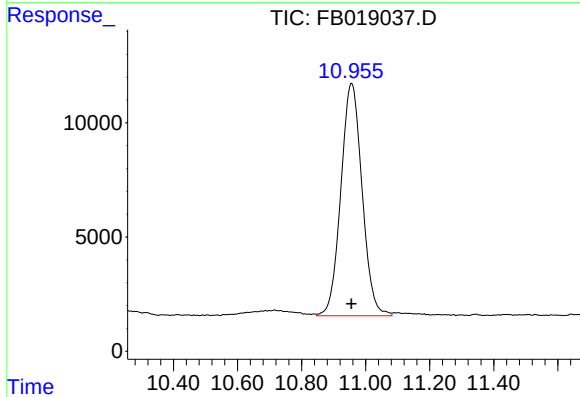


#6 Toluene

R.T.: 10.957 min
 Delta R.T.: 0.000 min
 Response: 467749
 Conc: 30.82 ng/ml

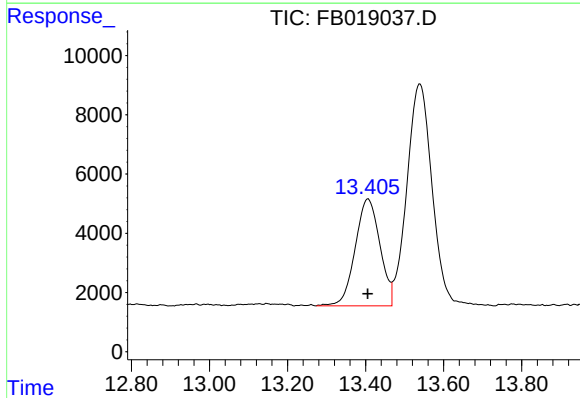


#7 Ethylbenzene

R.T.: 13.407 min
 Delta R.T.: 0.001 min
 Response: 158744
 Conc: 10.22 ng/ml

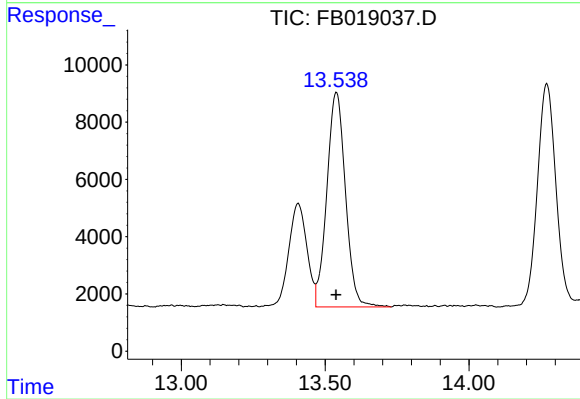


#8 m-Xylene

R.T.: 13.539 min
 Delta R.T.: 0.002 min
 Response: 336907
 Conc: 20.68 ng/ml

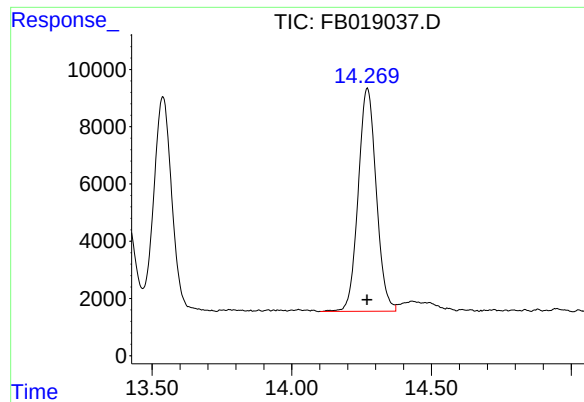

#9 O-Xylene

R.T.: 14.271 min
Delta R.T.: 0.001 min
Response: 349801
Conc: 20.69 ng/ml

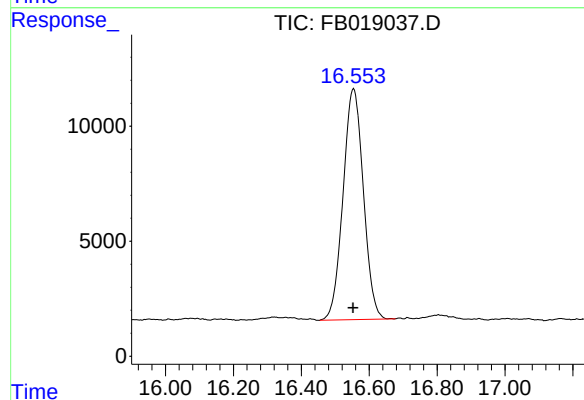

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: 0.001 min
Response: 417748
Conc: 20.64 ng/ml