

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB1121219\
 Data File : FB023205.D
 Signal(s) : FID2B.CH
 Acq On : 12 Dec 2019 12:37
 Operator : DD/AJ
 Sample : BSF1212S1
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 13 00:21:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	498687	20.302 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	1069794	32.737 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	1182882	33.922 ng/ml
3) t n-Heptane	7.750	387958	11.283 ng/ml
4) t Benzene	7.884	460573	11.054 ng/ml
6) t Toluene	10.622	1360617	33.776 ng/ml
7) t Ethylbenzene	13.063	428395	11.102 ng/ml
8) t m-Xylene	13.196	821936	22.587 ng/ml
9) t O-Xylene	13.924	785178	22.614 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	654595	23.342 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121219\
Data File : FB023205.D
Signal(s) : FID2B.CH
Acq On : 12 Dec 2019 12:37
Operator : DD/AJ
Sample : BSF1212S1
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 13 00:21:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

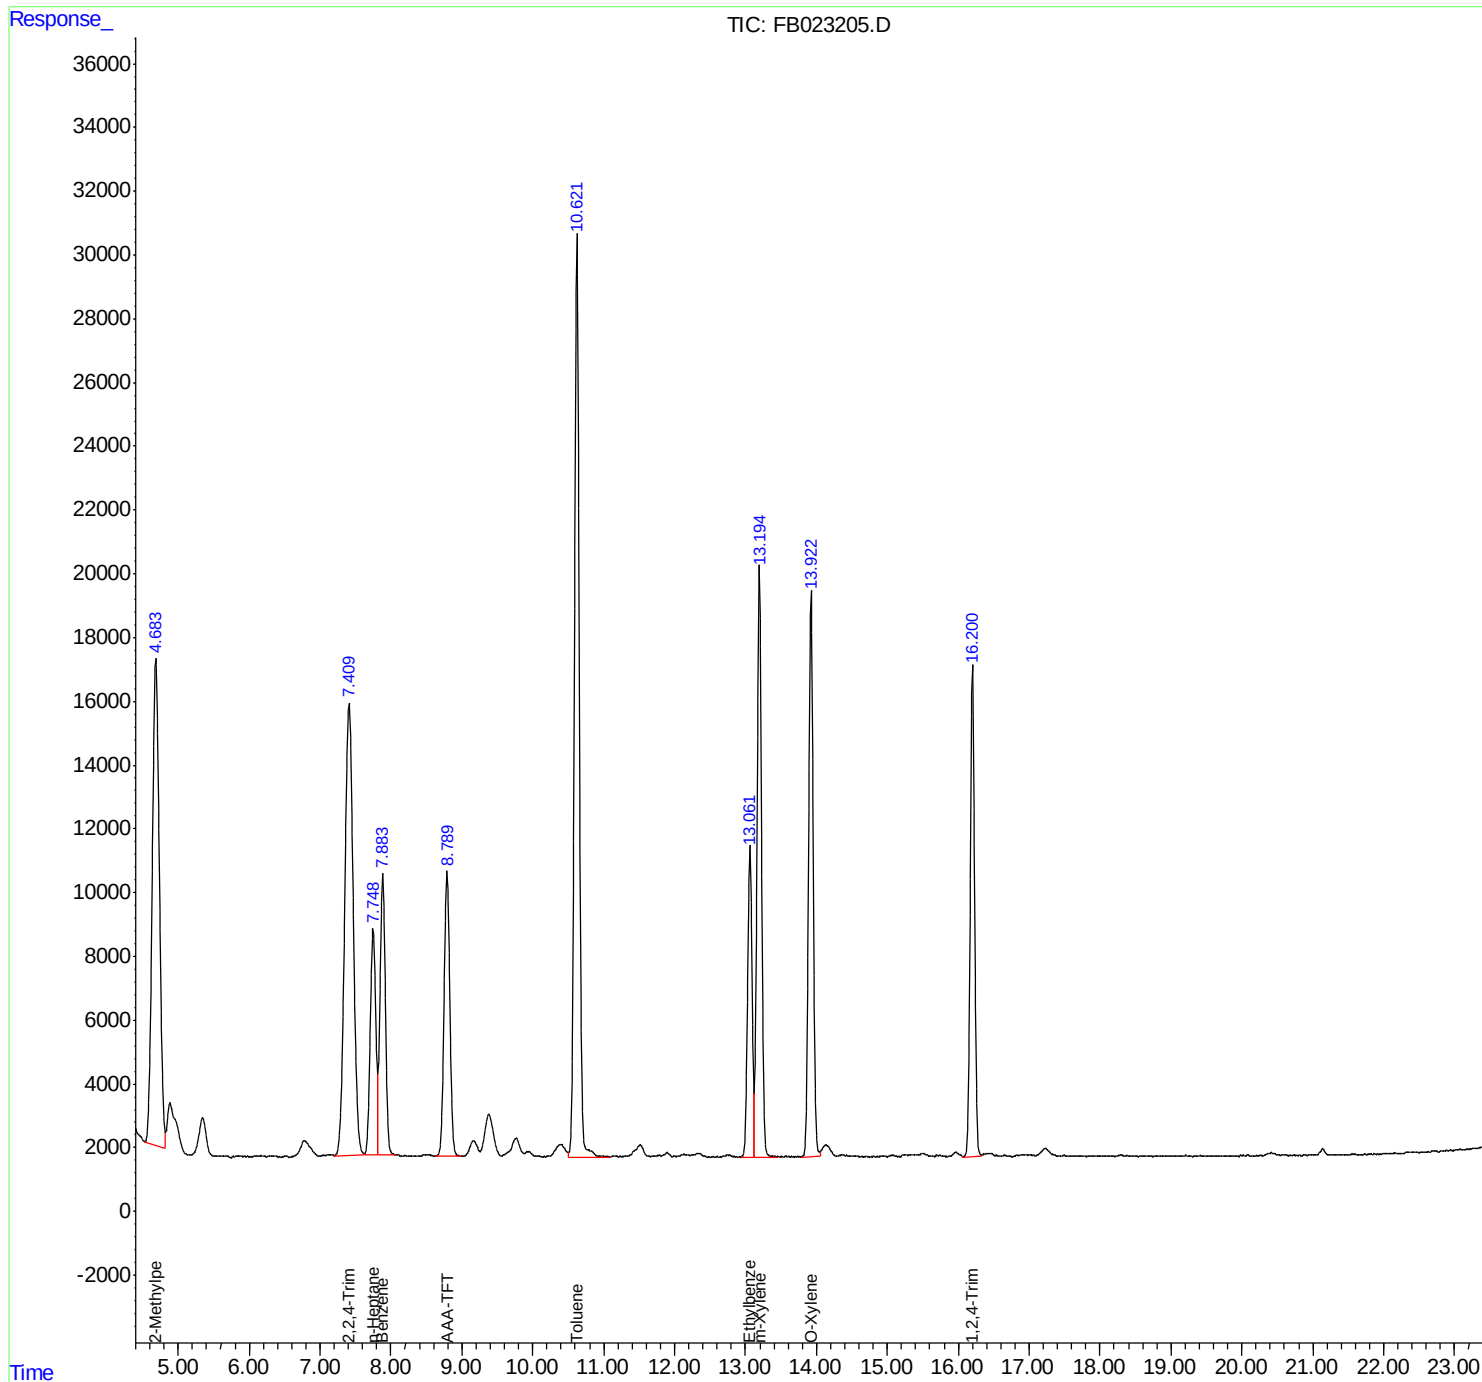

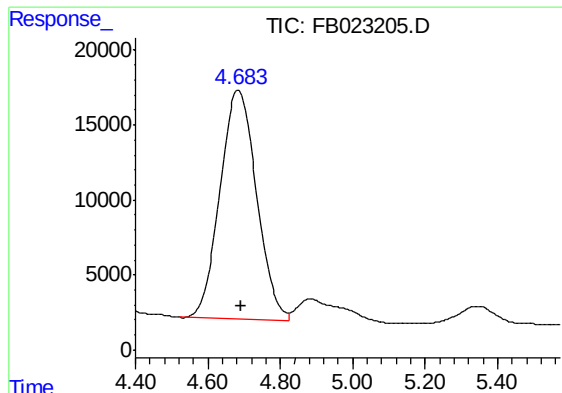


#1 2-Methylpentane

R.T.: 4.684 min
Delta R.T.: -0.007 min
Response: 1069794
Conc: 32.74 ng/ml

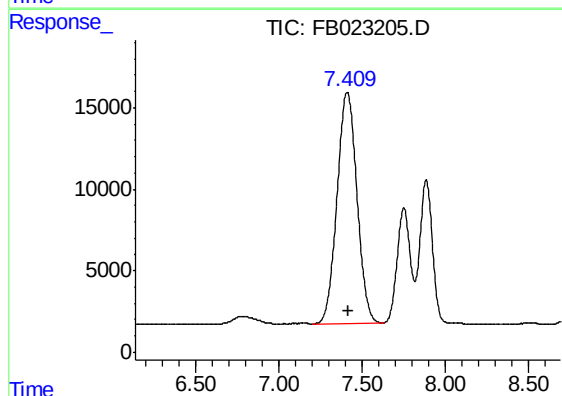


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.008 min
Response: 1182882
Conc: 33.92 ng/ml

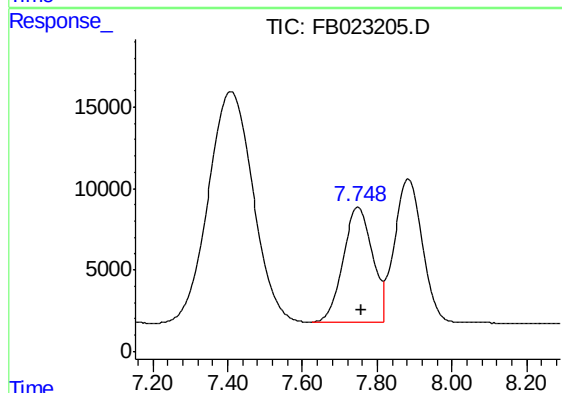


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.008 min
Response: 387958
Conc: 11.28 ng/ml

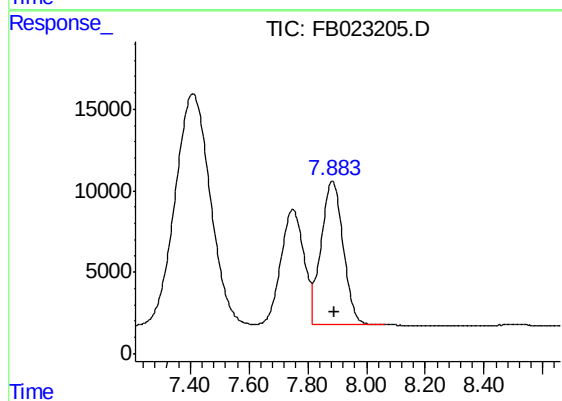


#4 Benzene

R.T.: 7.884 min
Delta R.T.: -0.008 min
Response: 460573
Conc: 11.05 ng/ml

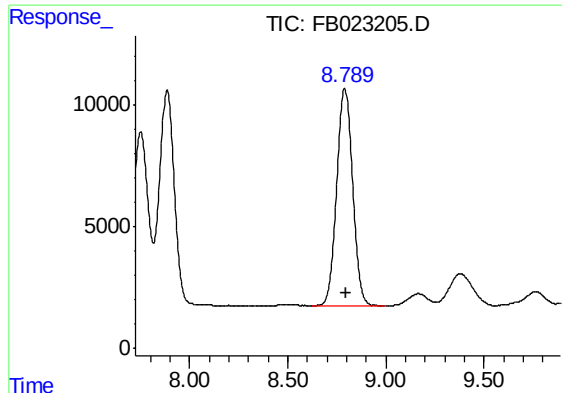


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.008 min
Response: 498687
Conc: 20.30 ng/ml

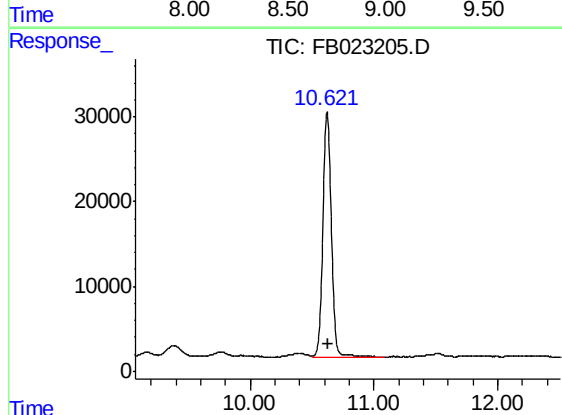


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.008 min
Response: 1360617
Conc: 33.78 ng/ml

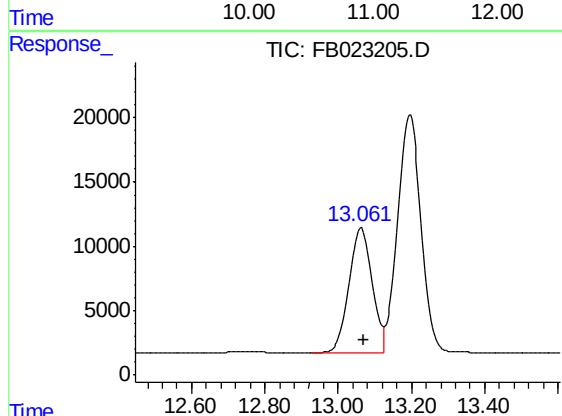


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.008 min
Response: 428395
Conc: 11.10 ng/ml

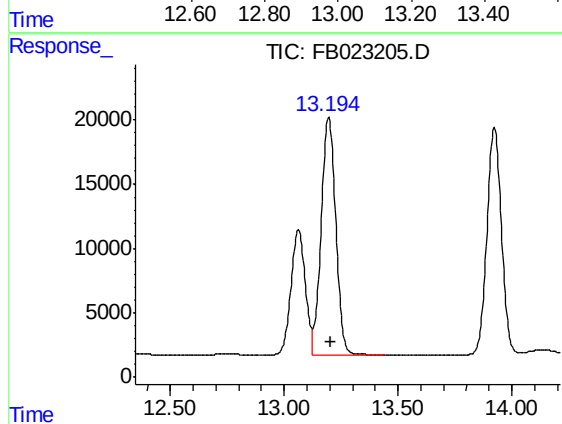


#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: -0.008 min
Response: 821936
Conc: 22.59 ng/ml

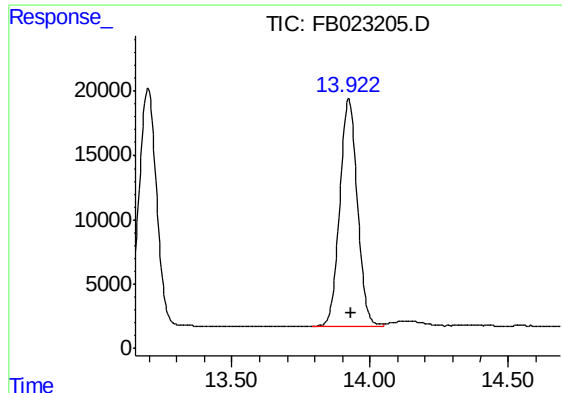

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.008 min
Response: 785178
Conc: 22.61 ng/ml

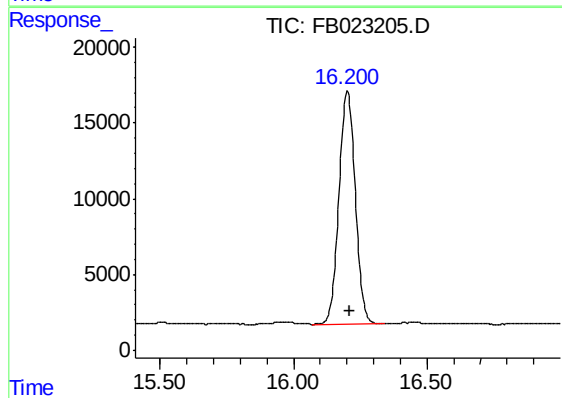

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.009 min
Response: 654595
Conc: 23.34 ng/ml