

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
 Data File : FB023207.D
 Signal(s) : FID2B.CH
 Acq On : 12 Dec 2019 16:59
 Operator : DD/AJ
 Sample : K6247-05MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 13 00:21:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	534423	21.756 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	1028789	31.482 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	1150023	32.980 ng/ml
3) t n-Heptane	7.750	377279	10.973 ng/ml
4) t Benzene	7.885	451229	10.830 ng/ml
6) t Toluene	10.623	1302139	32.324 ng/ml
7) t Ethylbenzene	13.062	414462	10.741 ng/ml
8) t m-Xylene	13.196	793664	21.810 ng/ml
9) t O-Xylene	13.924	753701	21.707 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	621291	22.155 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121219\
Data File : FB023207.D
Signal(s) : FID2B.CH
Acq On : 12 Dec 2019 16:59
Operator : DD/AJ
Sample : K6247-05MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 13 00:21:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

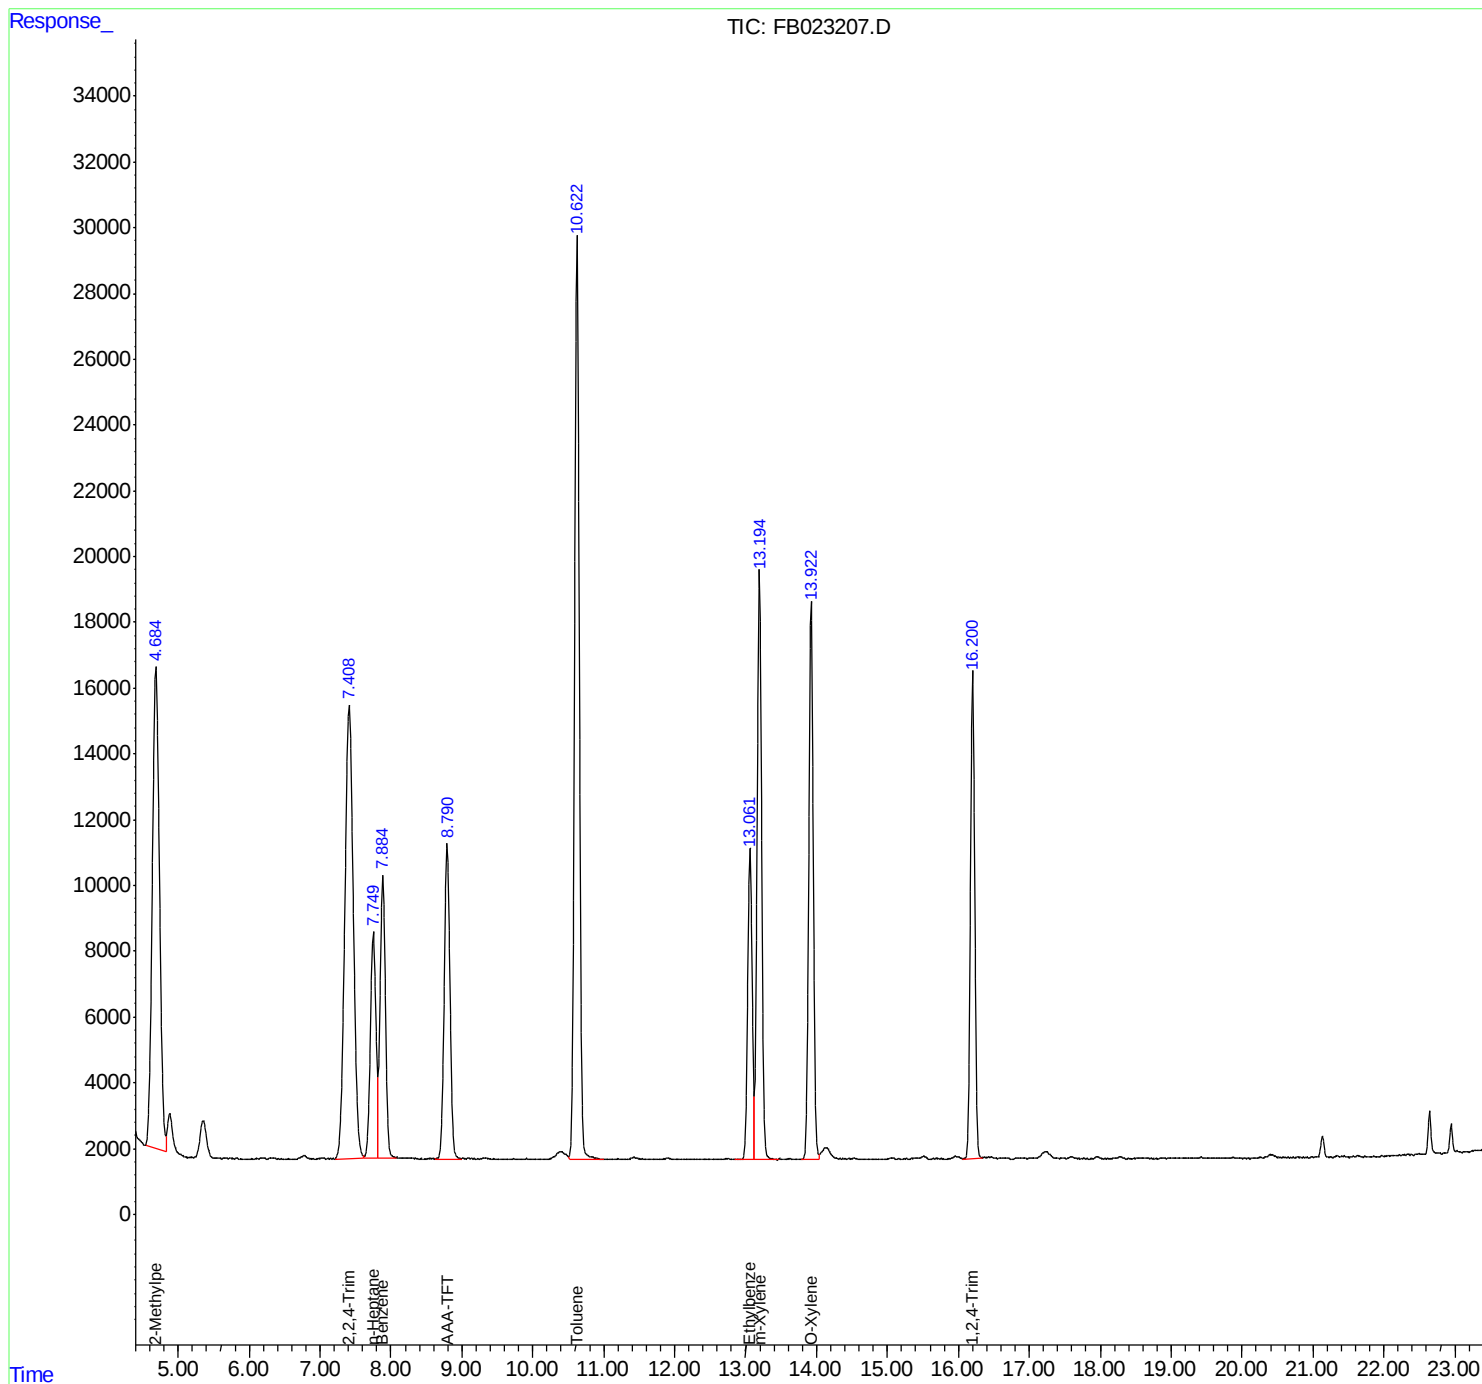

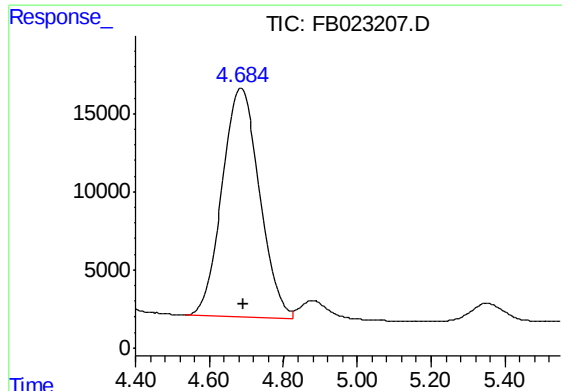


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.006 min
Response: 1028789
Conc: 31.48 ng/ml

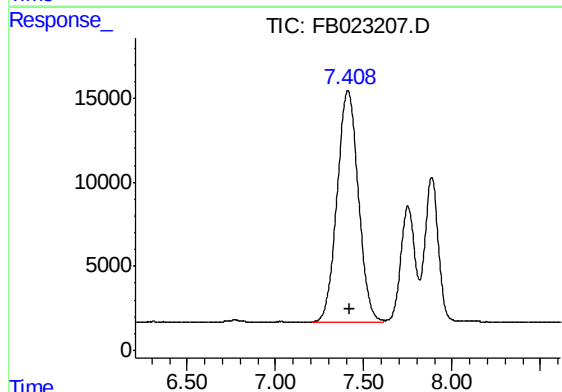


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.008 min
Response: 1150023
Conc: 32.98 ng/ml

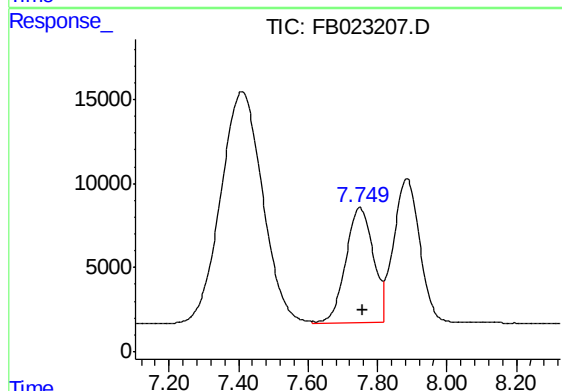


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.008 min
Response: 377279
Conc: 10.97 ng/ml

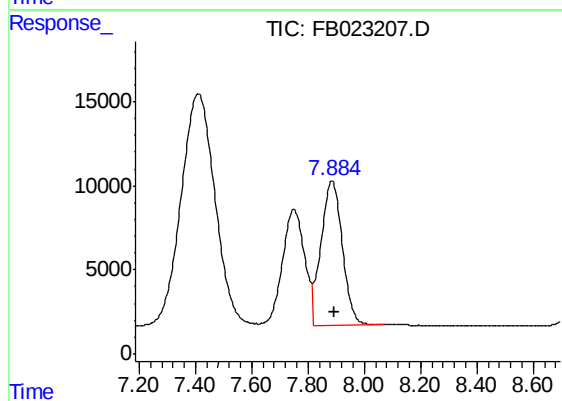


#4 Benzene

R.T.: 7.885 min
Delta R.T.: -0.008 min
Response: 451229
Conc: 10.83 ng/ml

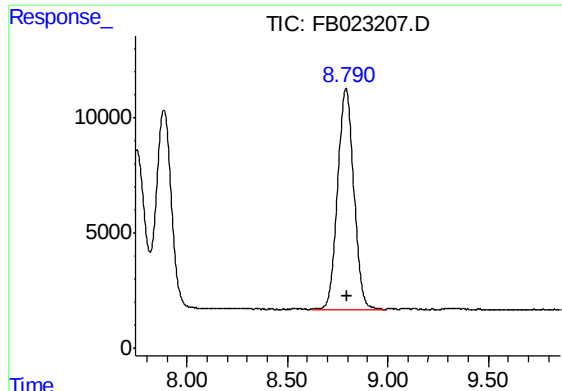


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.008 min
Response: 534423
Conc: 21.76 ng/ml

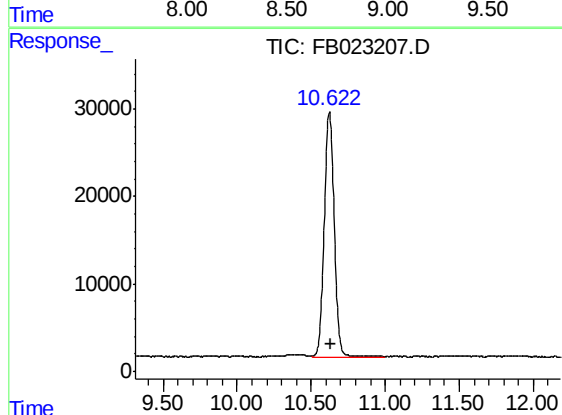


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.007 min
Response: 1302139
Conc: 32.32 ng/ml

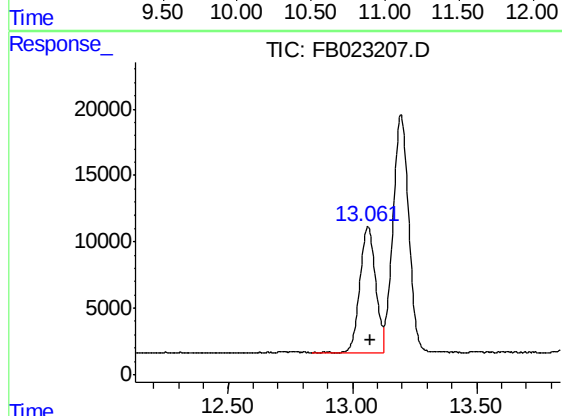


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.008 min
Response: 414462
Conc: 10.74 ng/ml

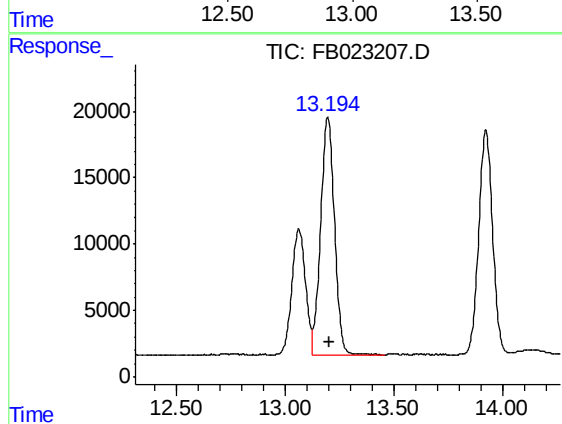


#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: -0.008 min
Response: 793664
Conc: 21.81 ng/ml

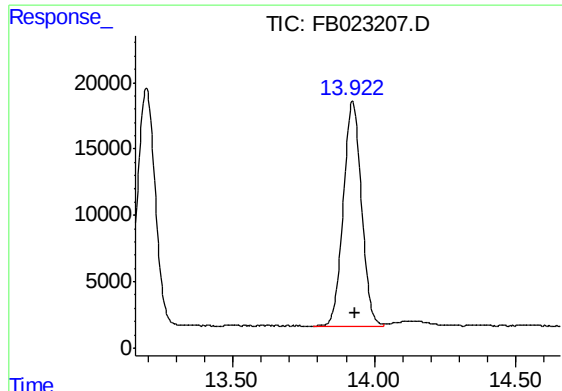

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.008 min
Response: 753701
Conc: 21.71 ng/ml

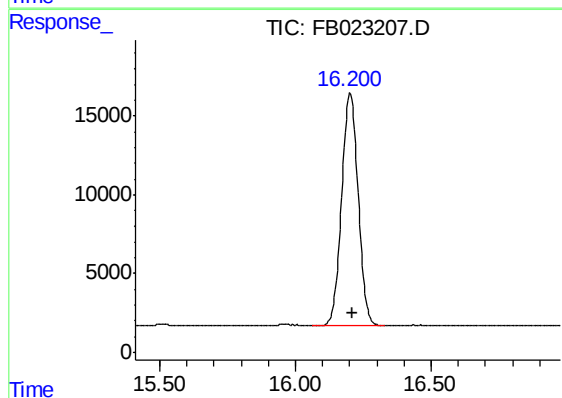

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.009 min
Response: 621291
Conc: 22.15 ng/ml