

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB112219\
 Data File : FB023208.D
 Signal(s) : FID2B.CH
 Acq On : 12 Dec 2019 17:30
 Operator : DD/AJ
 Sample : K6247-05MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 13 00:21:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	431370	17.561 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	857179	26.231 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	945128	27.104 ng/ml
3) t n-Heptane	7.752	309801	9.010 ng/ml
4) t Benzene	7.886	368976	8.856 ng/ml
6) t Toluene	10.624	1056678	26.231 ng/ml
7) t Ethylbenzene	13.064	326042	8.449 ng/ml
8) t m-Xylene	13.197	616991	16.955 ng/ml
9) t O-Xylene	13.925	598883	17.249 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	514125	18.333 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121219\
Data File : FB023208.D
Signal(s) : FID2B.CH
Acq On : 12 Dec 2019 17:30
Operator : DD/AJ
Sample : K6247-05MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 13 00:21:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

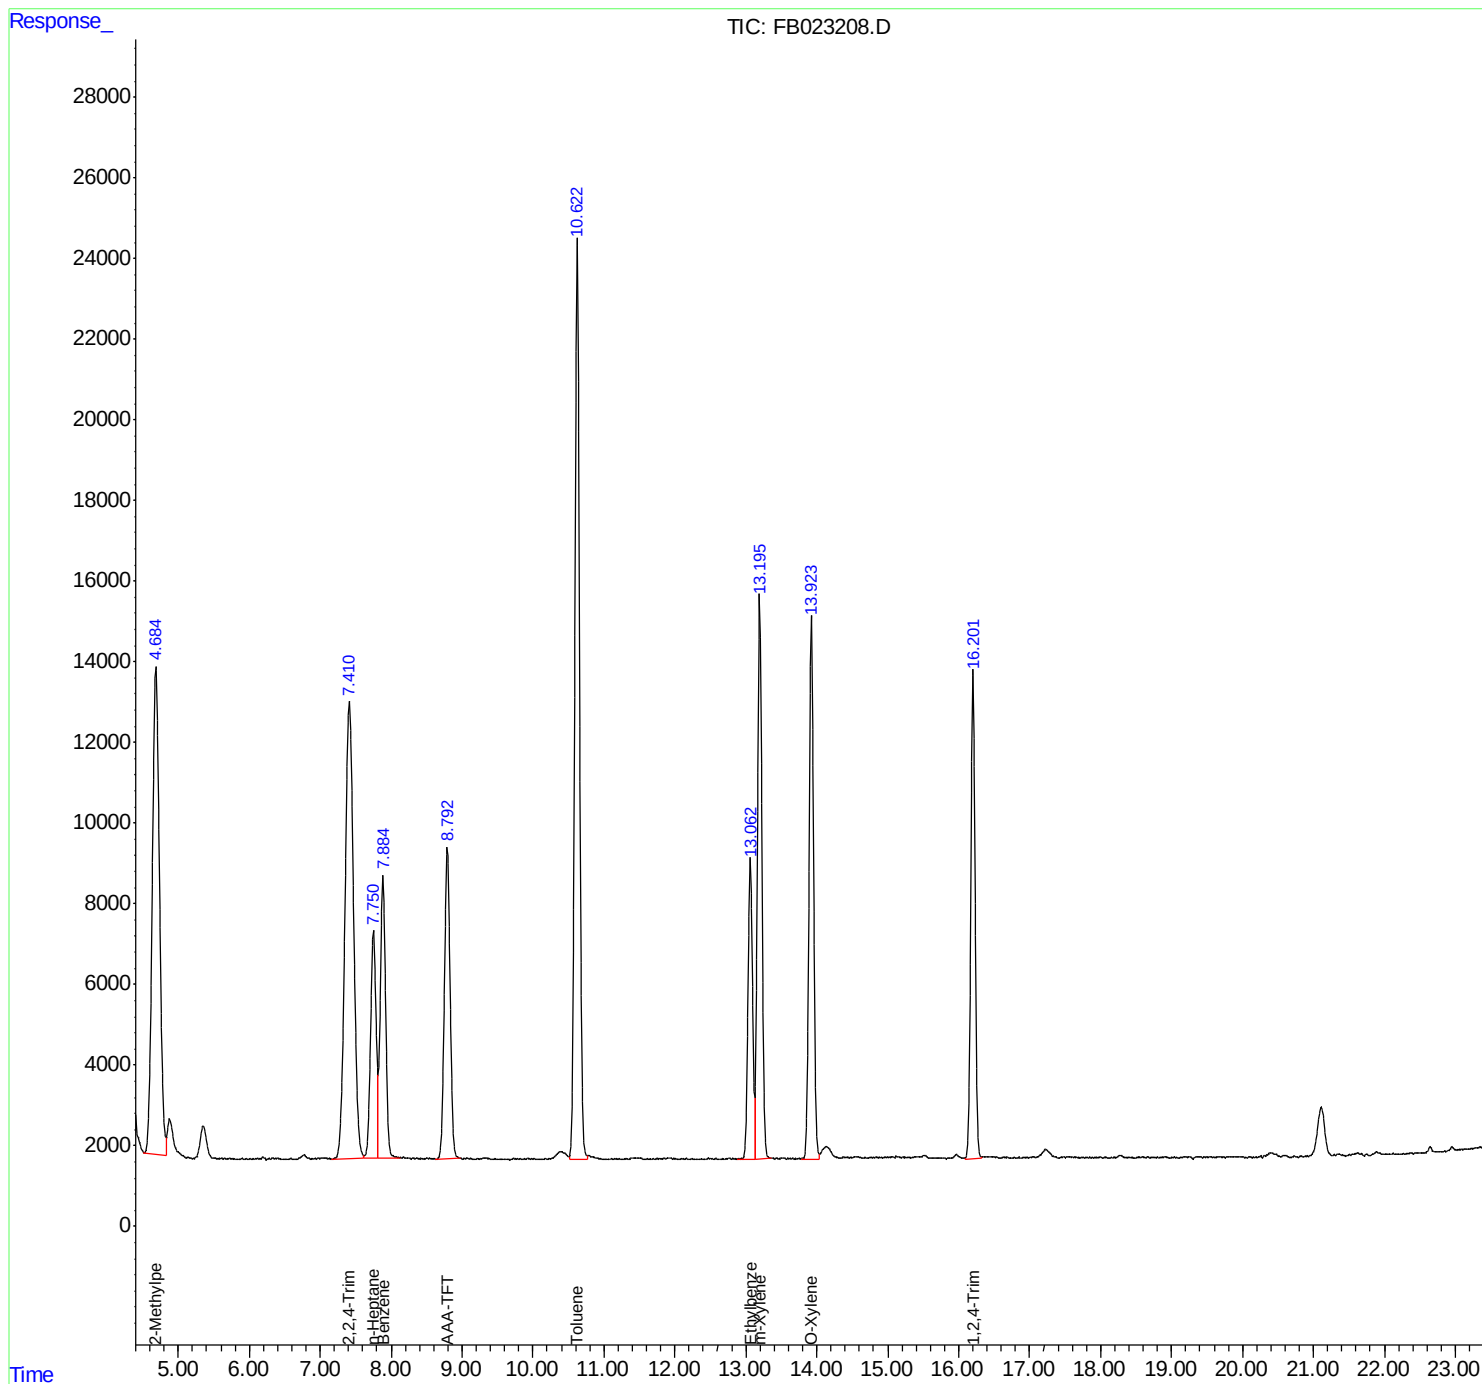

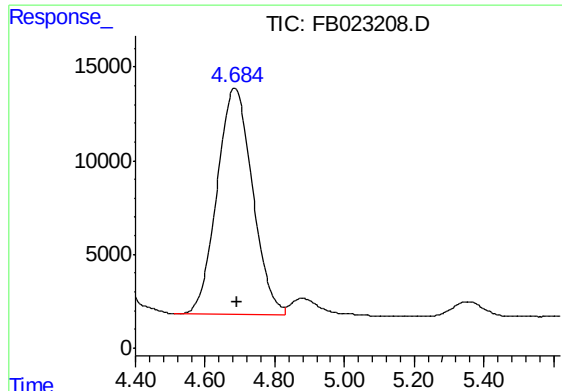


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.006 min
Response: 857179
Conc: 26.23 ng/ml

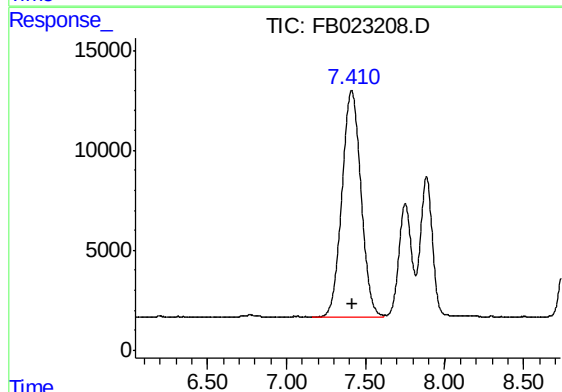


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.007 min
Response: 945128
Conc: 27.10 ng/ml

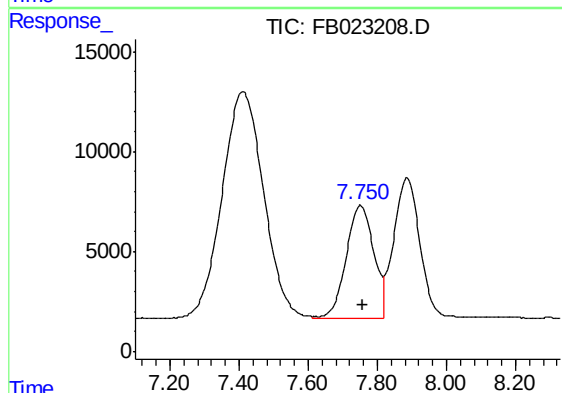


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: -0.006 min
Response: 309801
Conc: 9.01 ng/ml

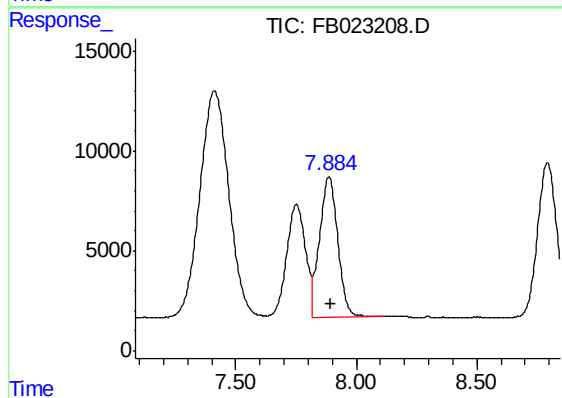


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.007 min
Response: 368976
Conc: 8.86 ng/ml

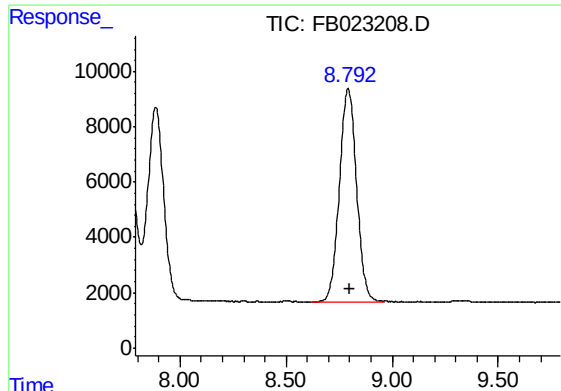


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.006 min
Response: 431370
Conc: 17.56 ng/ml

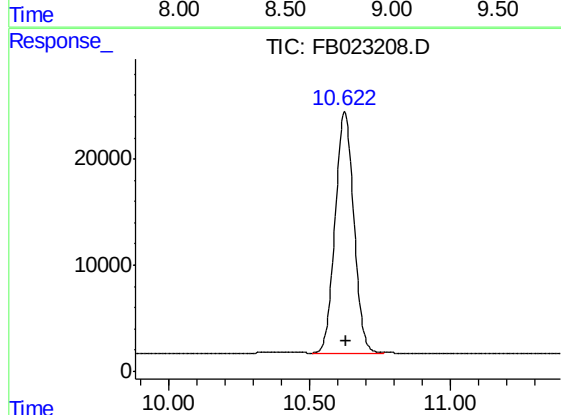


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.007 min
Response: 1056678
Conc: 26.23 ng/ml

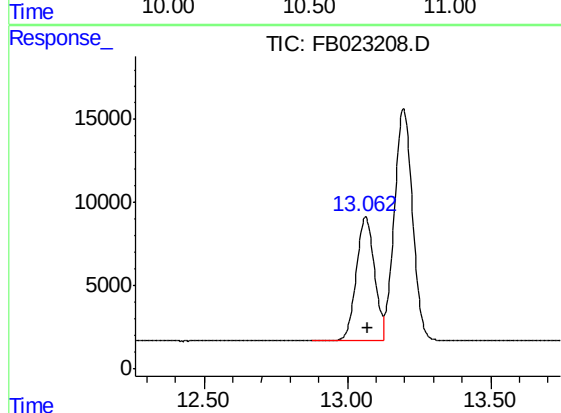


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: -0.007 min
Response: 326042
Conc: 8.45 ng/ml

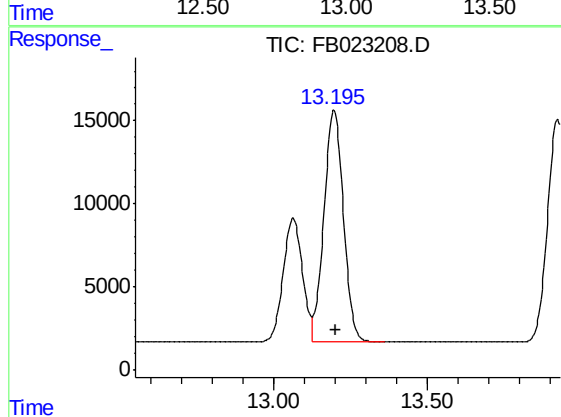


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: -0.007 min
Response: 616991
Conc: 16.96 ng/ml

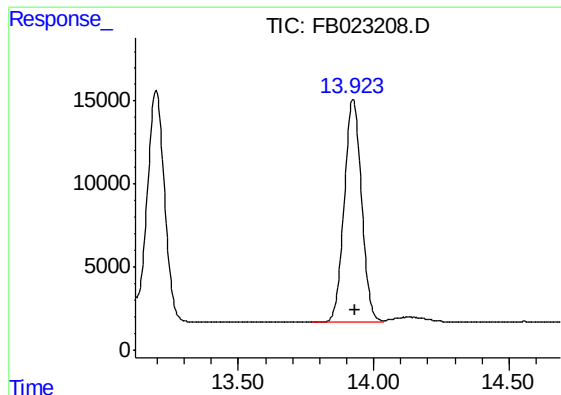

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: -0.007 min
Response: 598883
Conc: 17.25 ng/ml

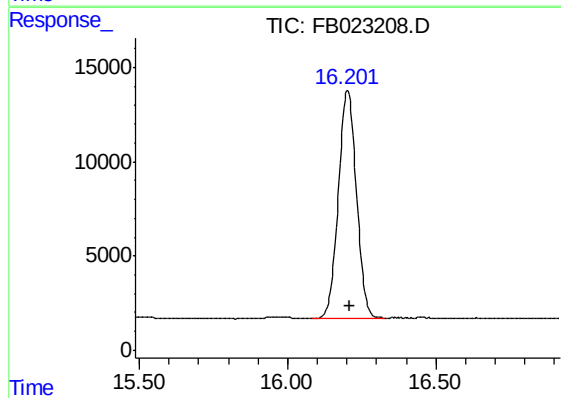

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: -0.008 min
Response: 514125
Conc: 18.33 ng/ml