

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121225\
Data File : FB032424.D
Signal(s) : FID2B.CH
Acq On : 12 Dec 2025 9:33
Operator : YP/AJ
Sample : VBF121225S1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 12 22:08:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	485684	21.558 ng/ml
Target Compounds			
6) t Toluene	10.609	241	0.005 ng/ml
8) t m-Xylene	13.185	6706	0.156 ng/ml
9) t O-Xylene	13.922	6828	0.165 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	21514	0.611 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121225\
Data File : FB032424.D
Signal(s) : FID2B.CH
Acq On : 12 Dec 2025 9:33
Operator : YP/AJ
Sample : VBF121225S1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 12 22:08:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120525.M
Quant Title :
QLast Update : Fri Dec 05 17:59:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

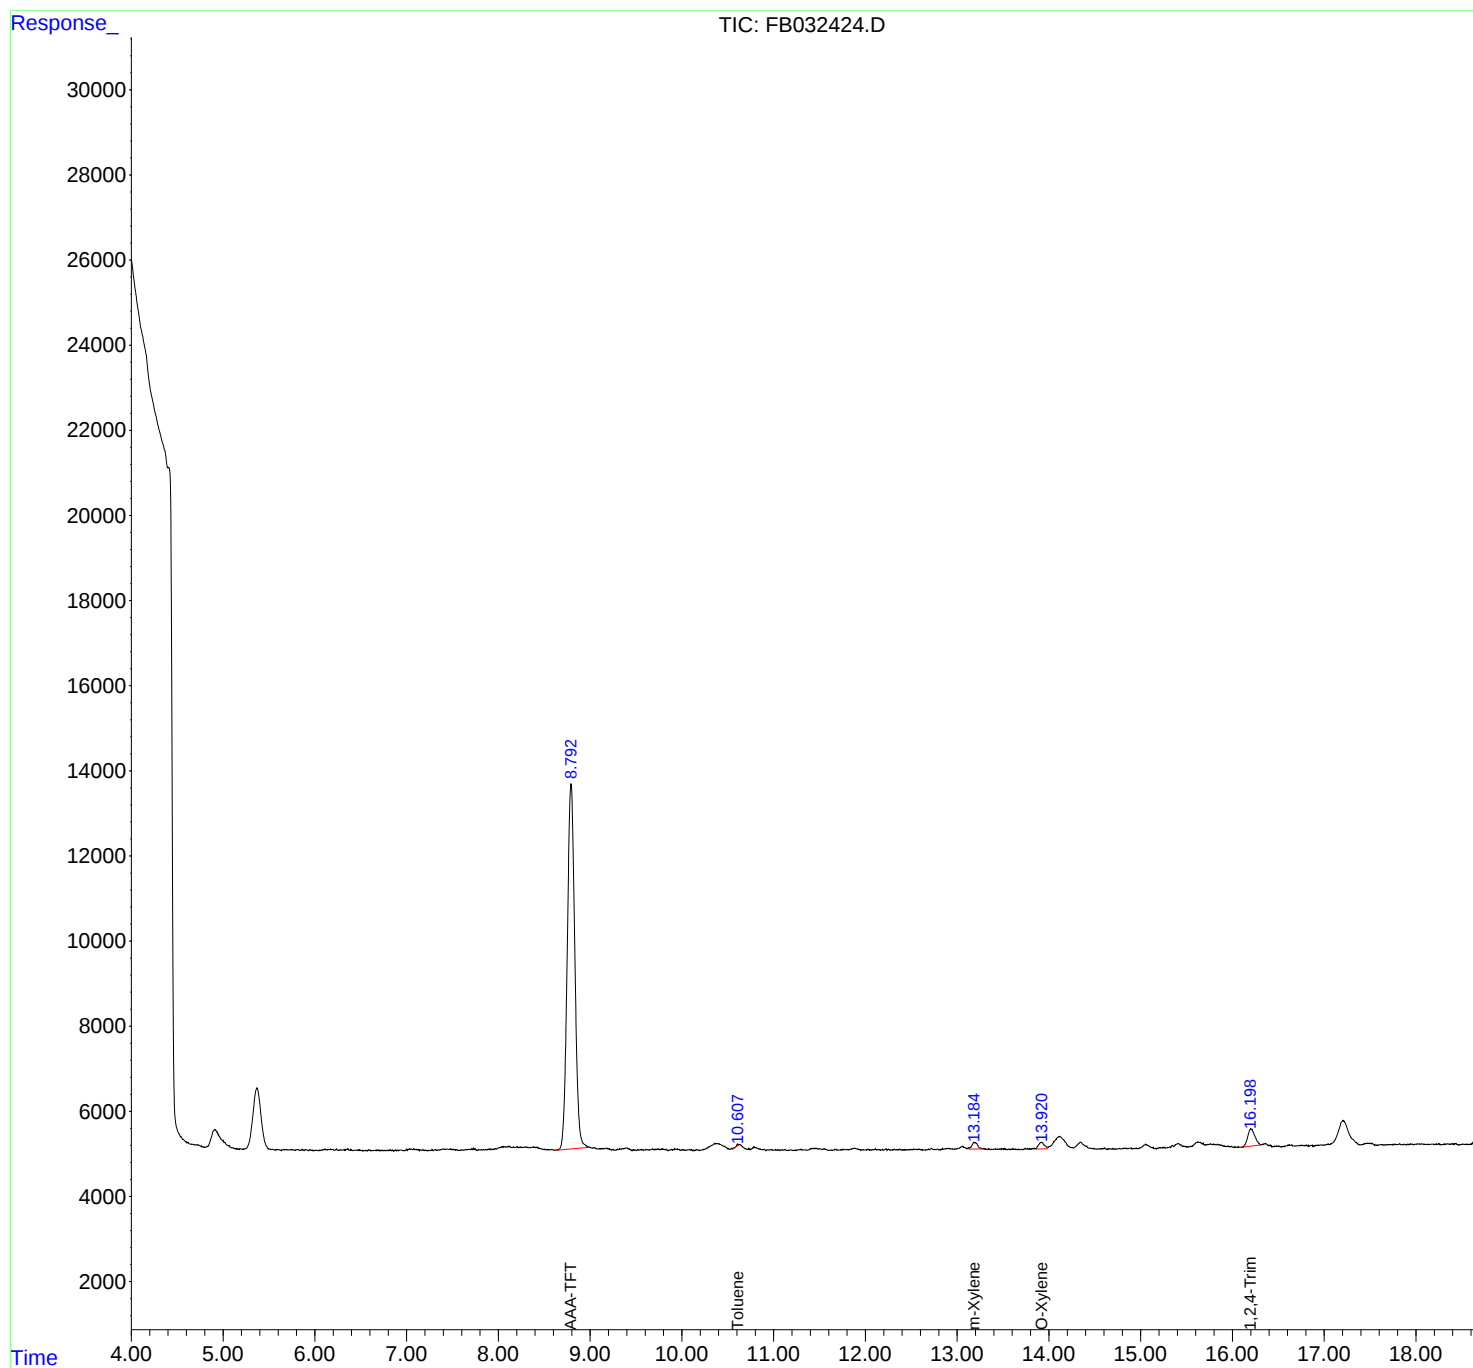


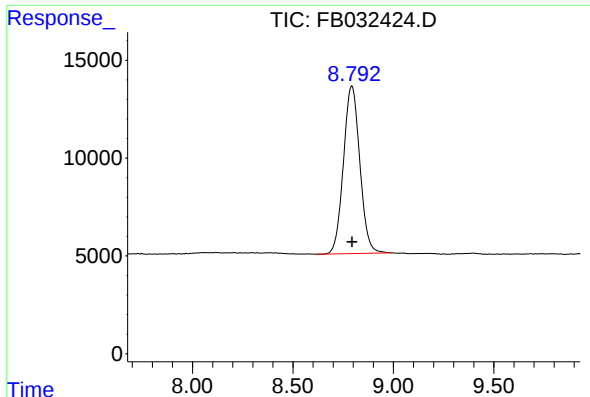

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: -0.001 min
Response: 485684
Conc: 21.56 ng/ml

Instrument :
FID_B
ClientSampleId :

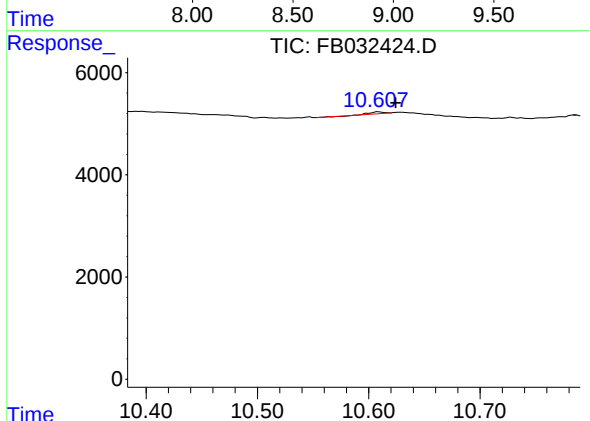


#6 Toluene

R.T.: 10.609 min
Delta R.T.: -0.015 min
Response: 241
Conc: 0.01 ng/ml

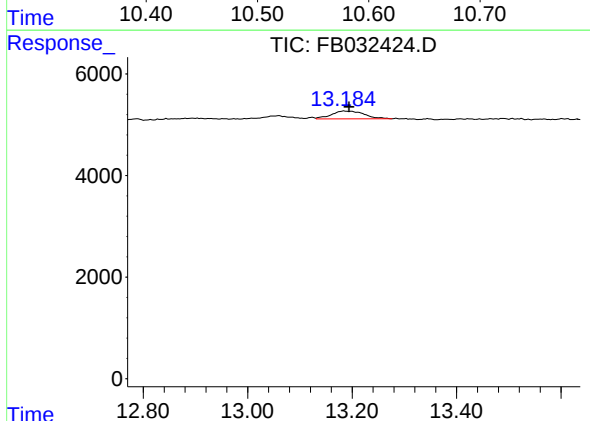


#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: -0.009 min
Response: 6706
Conc: 0.16 ng/ml

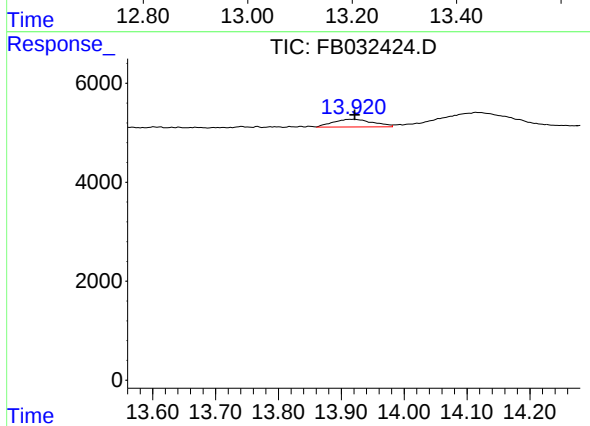

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.000 min
Response: 6828
Conc: 0.16 ng/ml

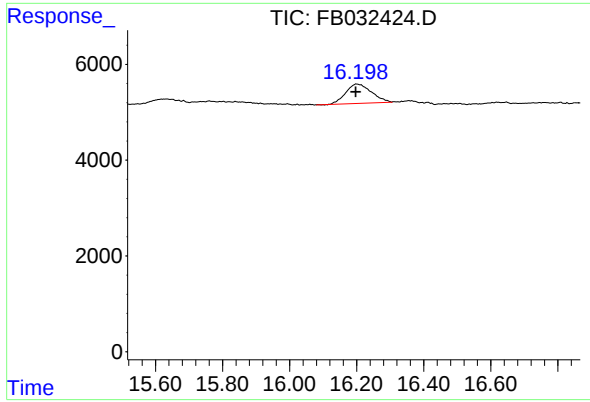

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.002 min
Response: 21514
Conc: 0.61 ng/ml

Instrument :
FID_B
ClientSampleId :