

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121318\
 Data File : FB019063.D
 Signal(s) : FID2B.CH
 Acq On : 13 Dec 2018 10:25
 Operator : MJ/SJ
 Sample : BSF1213S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 14 05:46:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.105	199417	22.815 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.957	441279	28.865 ng/ml
2) t 2,2,4-Trimethylpentane	7.722	473947	30.764 ng/ml
3) t n-Heptane	8.062	154752	10.412 ng/ml
4) t Benzene	8.201	189802	10.537 ng/ml
6) t Toluene	10.955	451163	29.723 ng/ml
7) t Ethylbenzene	13.405	154508	9.945 ng/ml
8) t m-Xylene	13.538	324869	19.941 ng/ml
9) t O-Xylene	14.269	338237	20.004 ng/ml
10) t 1,2,4-Trimethylbenzene	16.552	405345	20.029 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121318\
Data File : FB019063.D
Signal(s) : FID2B.CH
Acq On : 13 Dec 2018 10:25
Operator : MJ/SJ
Sample : BSF1213S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 14 05:46:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

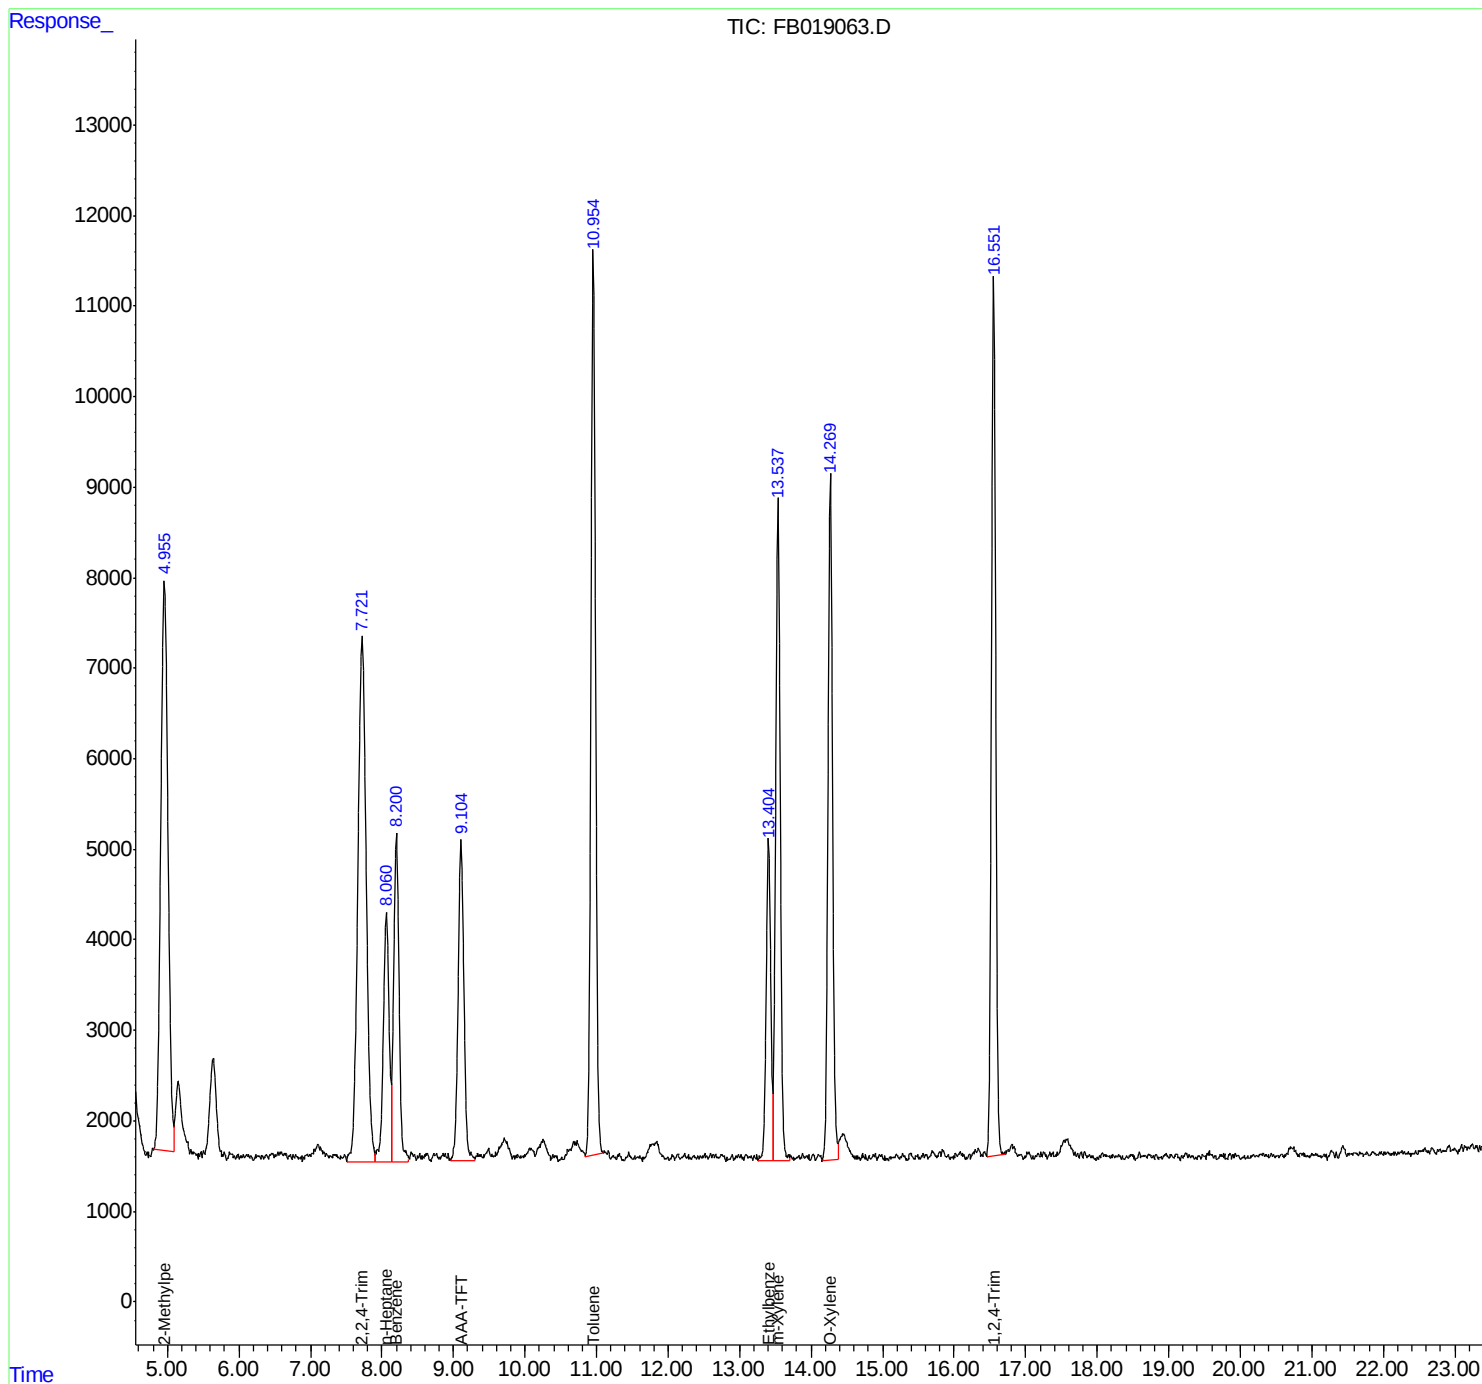

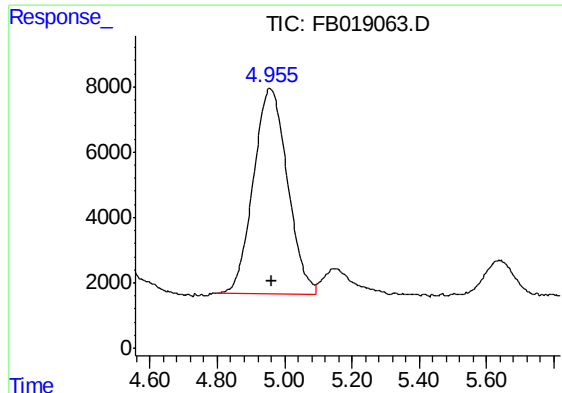


#1 2-Methylpentane

R.T.: 4.957 min
Delta R.T.: -0.004 min
Response: 441279
Conc: 28.87 ng/ml

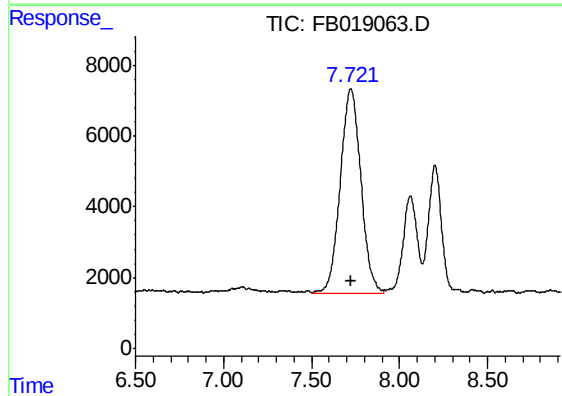


#2 2,2,4-Trimethylpentane

R.T.: 7.722 min
Delta R.T.: 0.000 min
Response: 473947
Conc: 30.76 ng/ml

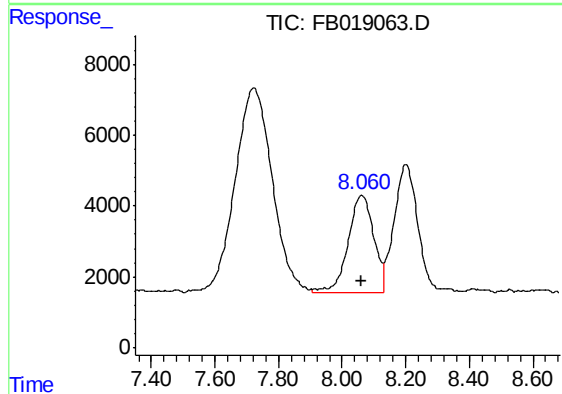


#3 n-Heptane

R.T.: 8.062 min
Delta R.T.: 0.000 min
Response: 154752
Conc: 10.41 ng/ml

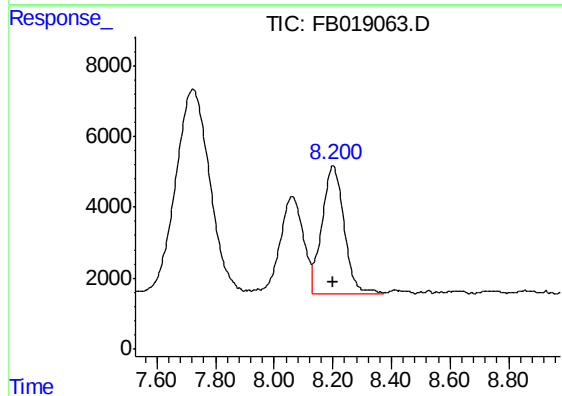


#4 Benzene

R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 189802
Conc: 10.54 ng/ml

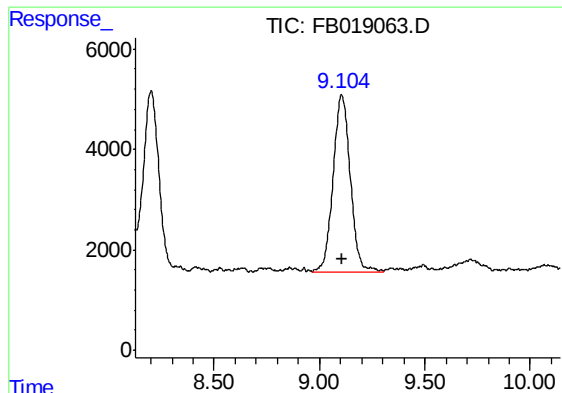


#5 AAA-TFT

R.T.: 9.105 min
Delta R.T.: -0.001 min
Response: 199417
Conc: 22.81 ng/ml

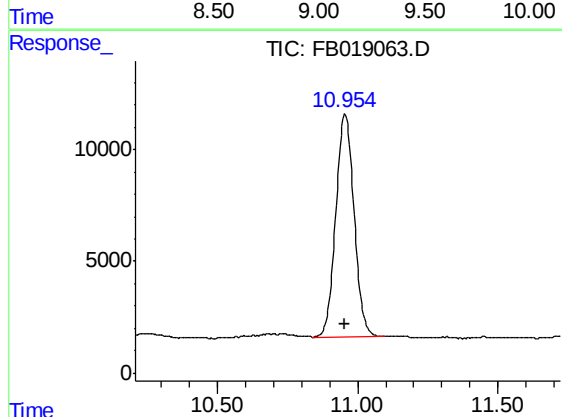


#6 Toluene

R.T.: 10.955 min
Delta R.T.: 0.000 min
Response: 451163
Conc: 29.72 ng/ml

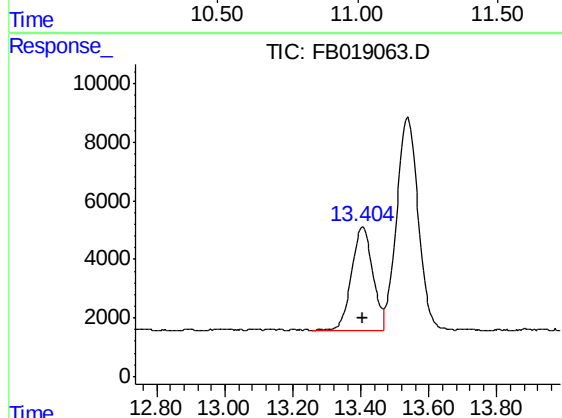


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: 0.000 min
Response: 154508
Conc: 9.95 ng/ml

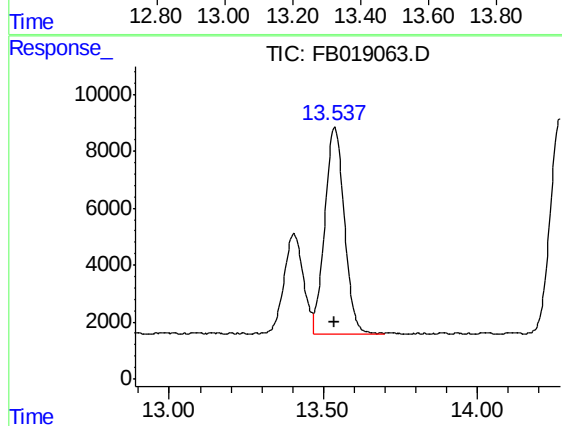


#8 m-Xylene

R.T.: 13.538 min
Delta R.T.: 0.000 min
Response: 324869
Conc: 19.94 ng/ml

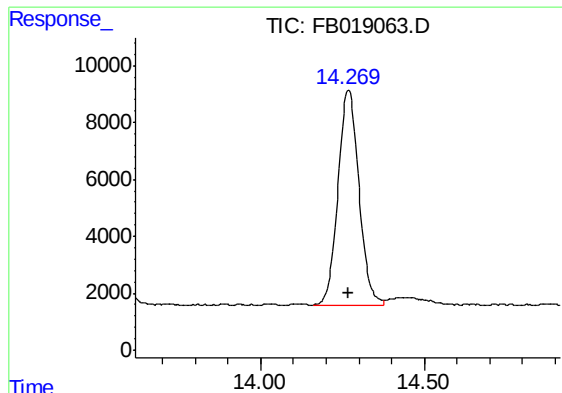

#9 O-Xylene

R.T.: 14.269 min
Delta R.T.: 0.000 min
Response: 338237
Conc: 20.00 ng/ml

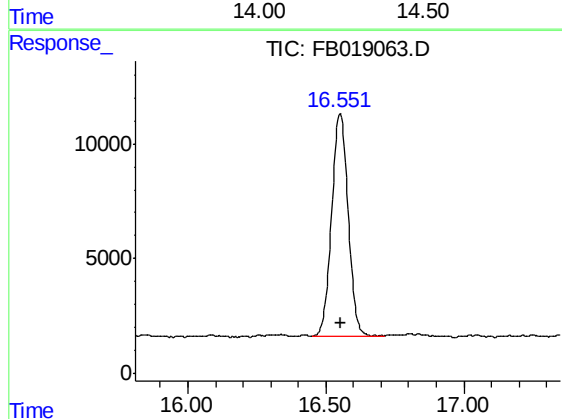

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: 0.000 min
Response: 405345
Conc: 20.03 ng/ml