

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121321\
 Data File : FB026501.D
 Signal(s) : FID2B.CH
 Acq On : 13 Dec 2021 13:33
 Operator : AJ/MA
 Sample : BSF1213S1
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 14 00:36:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	261823	23.304 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	544984	31.309 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	622573	31.393 ng/ml
3) t n-Heptane	7.749	200403	10.469 ng/ml
4) t Benzene	7.885	233751	10.513 ng/ml
6) t Toluene	10.618	680220	31.878 ng/ml
7) t Ethylbenzene	13.055	215245	10.904 ng/ml
8) t m-Xylene	13.188	419130	21.258 ng/ml
9) t O-Xylene	13.915	406159	21.268 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	405797	20.888 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121321\
Data File : FB026501.D
Signal(s) : FID2B.CH
Acq On : 13 Dec 2021 13:33
Operator : AJ/MA
Sample : BSF1213S1
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 14 00:36:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

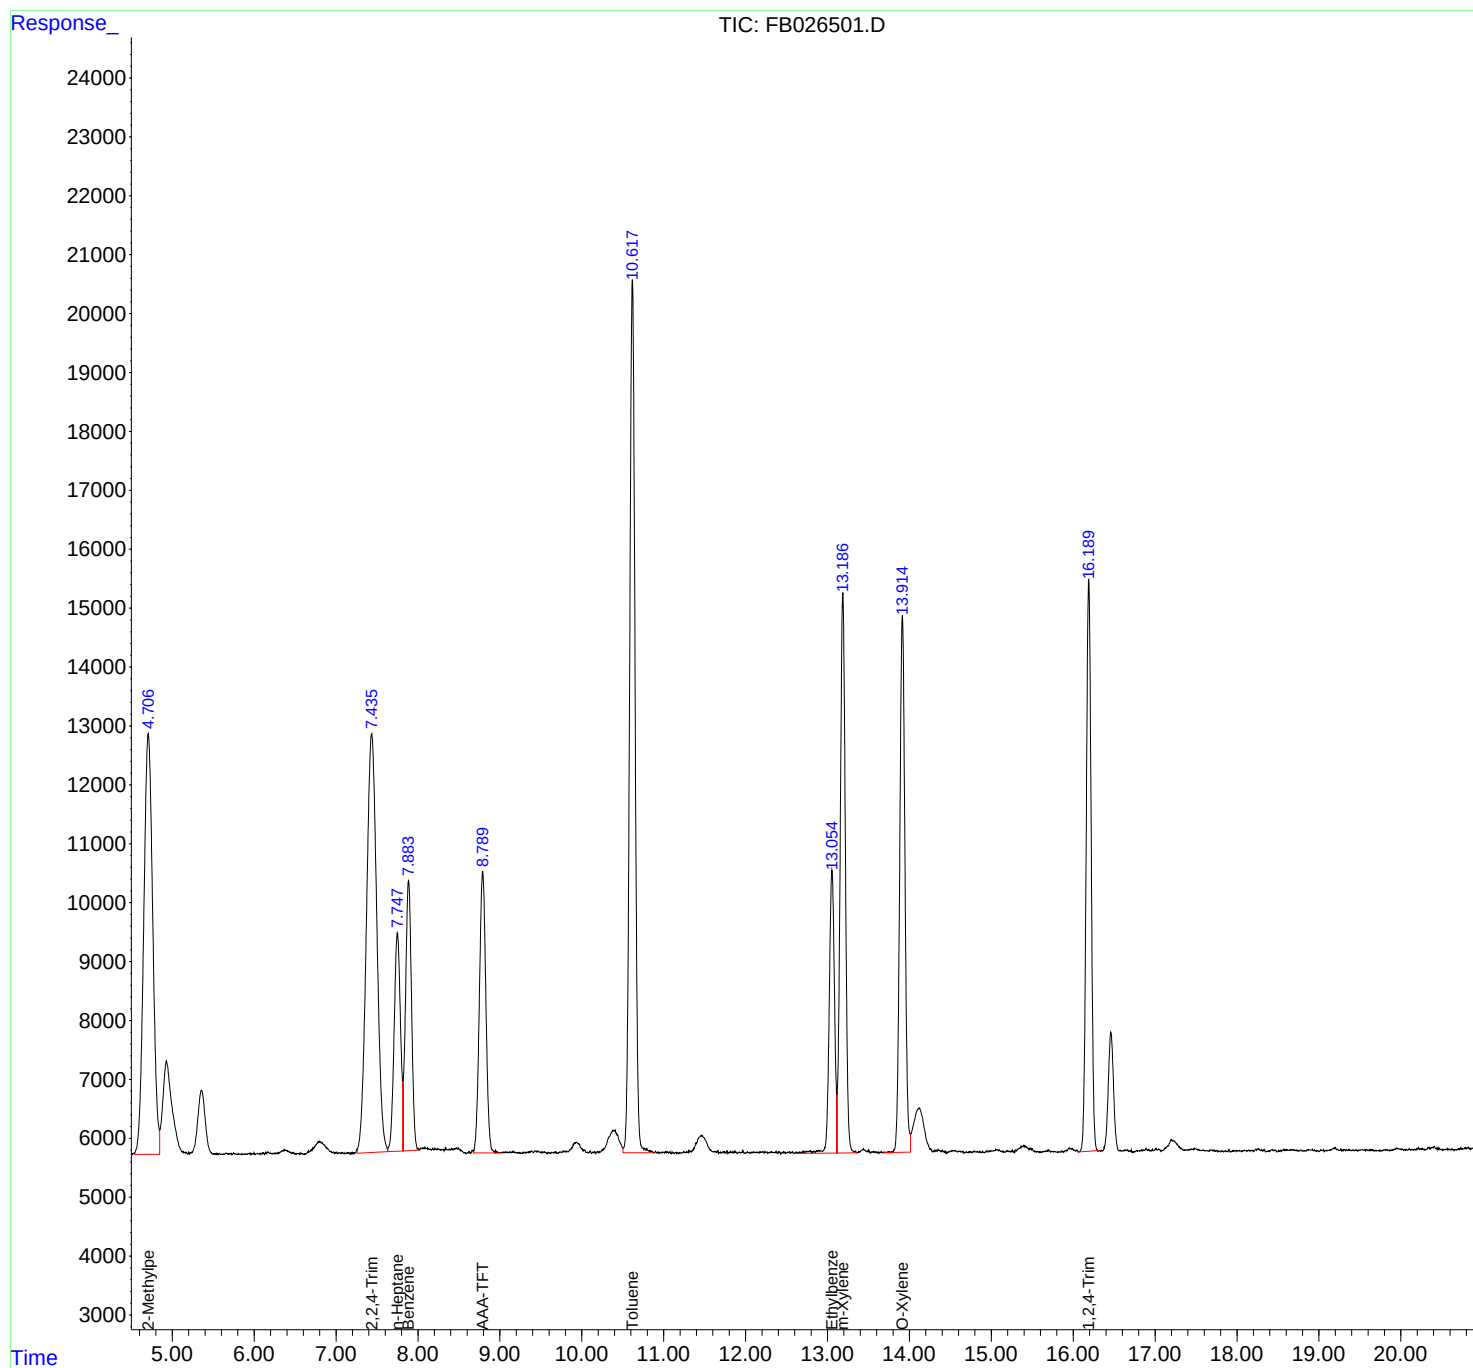

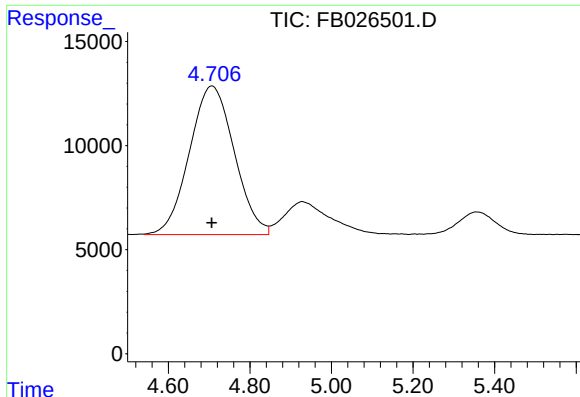


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.002 min
Response: 544984
Conc: 31.31 ng/ml

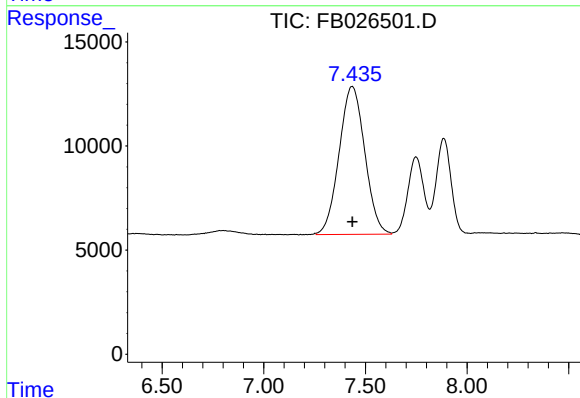


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: 0.000 min
Response: 622573
Conc: 31.39 ng/ml

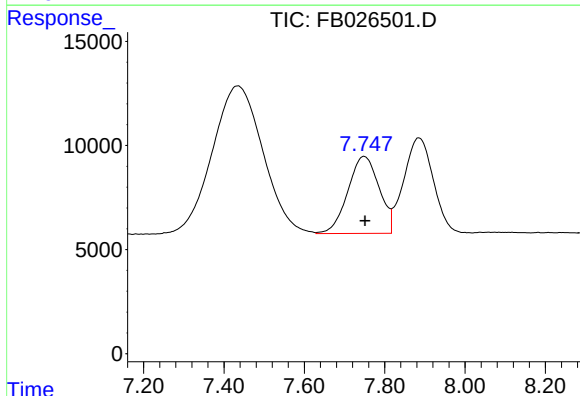


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 200403
Conc: 10.47 ng/ml

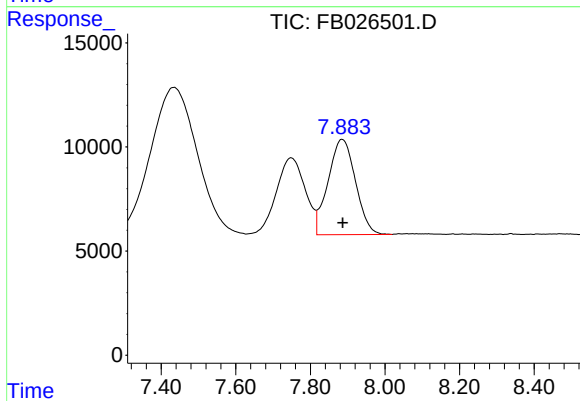


#4 Benzene

R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 233751
Conc: 10.51 ng/ml

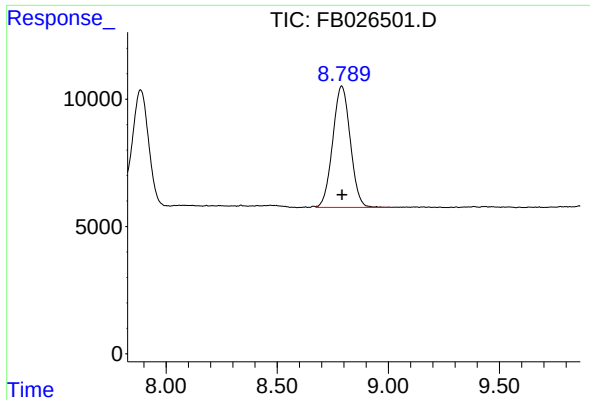


#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: -0.001 min
Response: 261823
Conc: 23.30 ng/ml

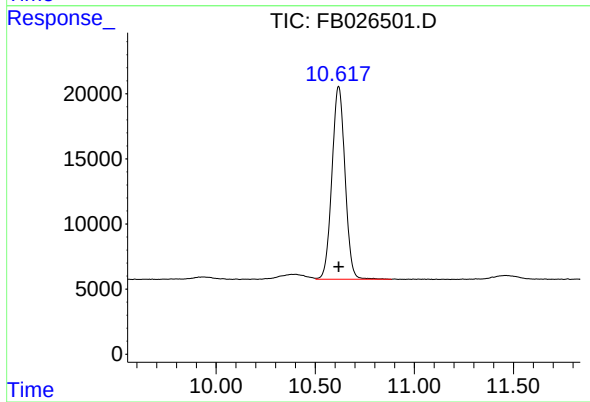


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 680220
Conc: 31.88 ng/ml

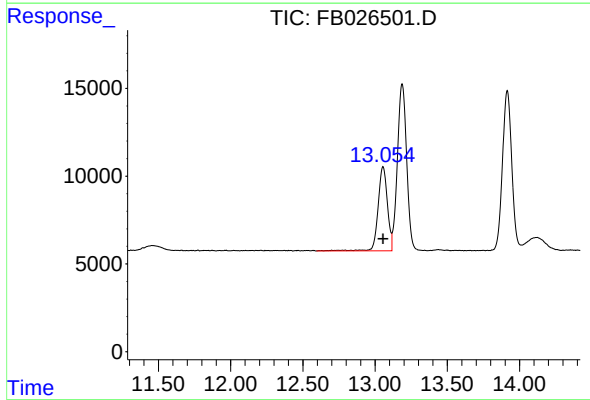


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 215245
Conc: 10.90 ng/ml

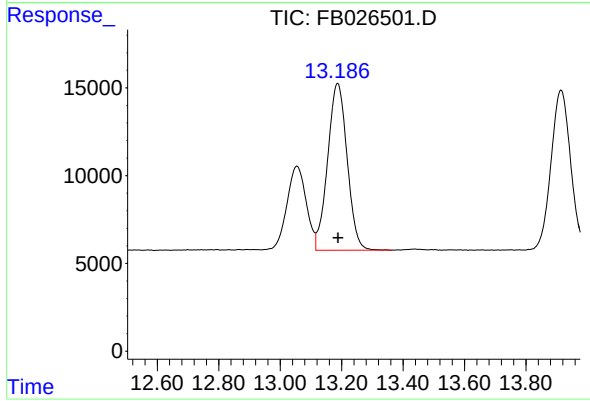


#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: -0.002 min
Response: 419130
Conc: 21.26 ng/ml

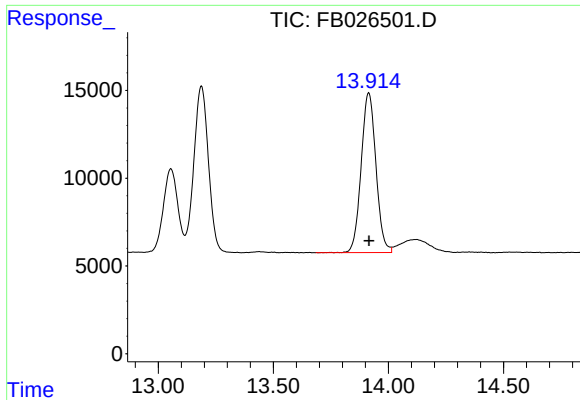

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.001 min
Response: 406159
Conc: 21.27 ng/ml

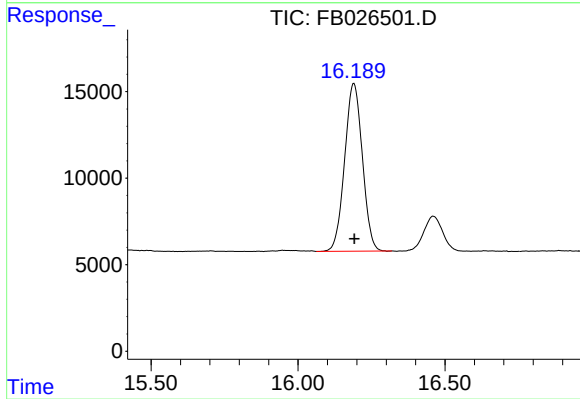

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.002 min
Response: 405797
Conc: 20.89 ng/ml