

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121421\
 Data File : FB026506.D
 Signal(s) : FID2B.CH
 Acq On : 14 Dec 2021 10:56
 Operator : AJ/MA
 Sample : BSF1214S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1214S1

Integration File: Calibration.e
 Quant Time: Dec 15 03:27:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	250759	22.320 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	511019	29.357 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	590153	29.758 ng/ml
3) t n-Heptane	7.748	191145	9.985 ng/ml
4) t Benzene	7.885	223009	10.030 ng/ml
6) t Toluene	10.617	641308	30.055 ng/ml
7) t Ethylbenzene	13.054	194108	9.833 ng/ml
8) t m-Xylene	13.186	391430	19.854 ng/ml
9) t O-Xylene	13.914	384055	20.110 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	381053	19.614 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121421\
Data File : FB026506.D
Signal(s) : FID2B.CH
Acq On : 14 Dec 2021 10:56
Operator : AJ/MA
Sample : BSF1214S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1214S1

Integration File: Calibration.e
Quant Time: Dec 15 03:27:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

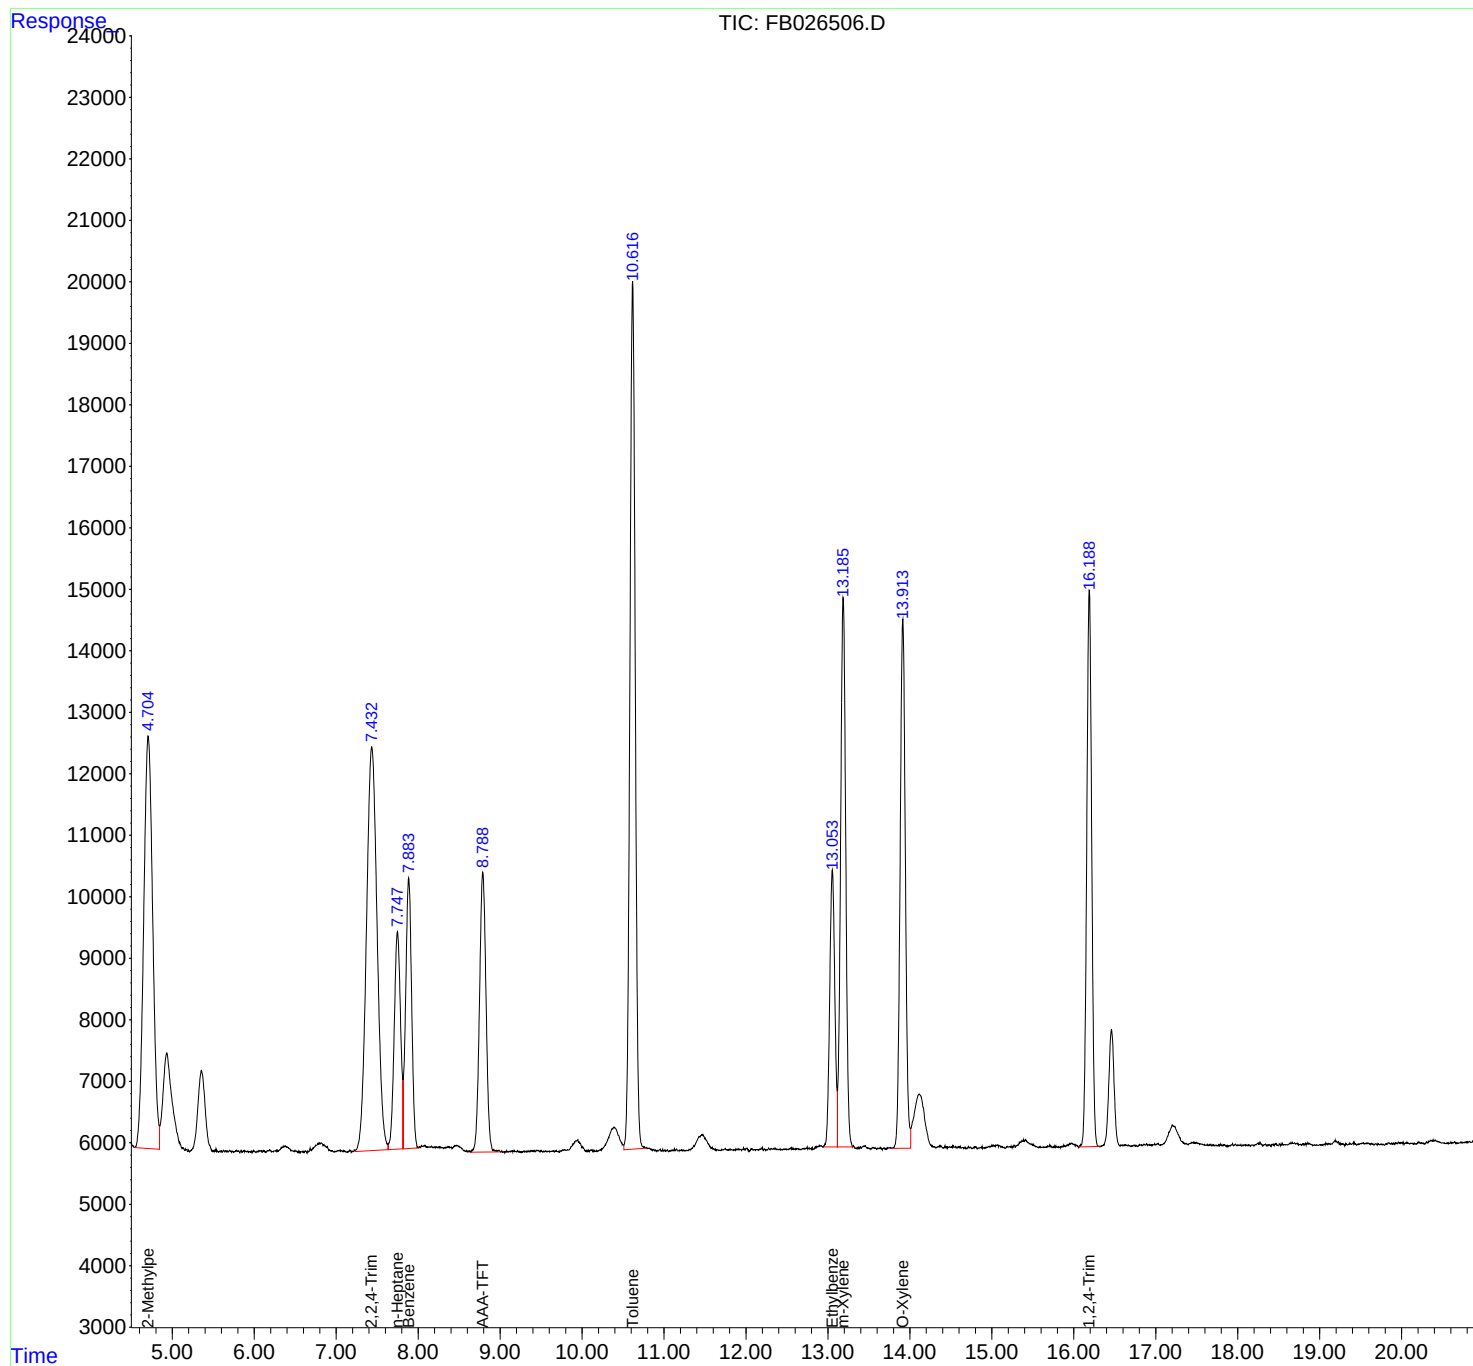


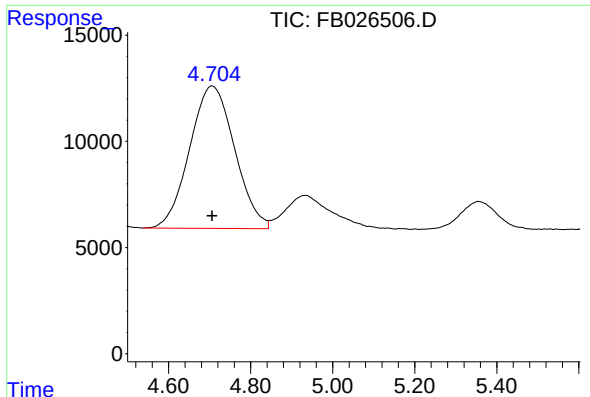

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 511019
Conc: 29.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1214S1

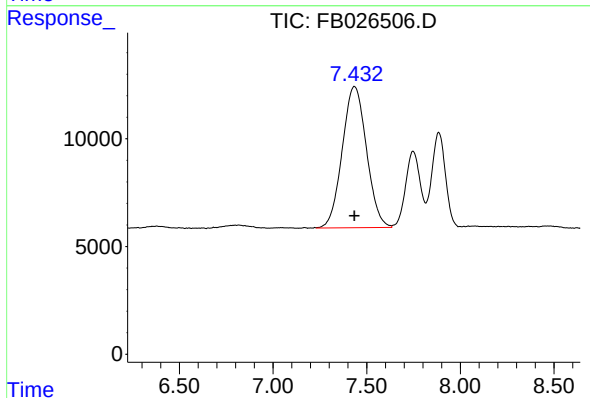


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: -0.002 min
Response: 590153
Conc: 29.76 ng/ml

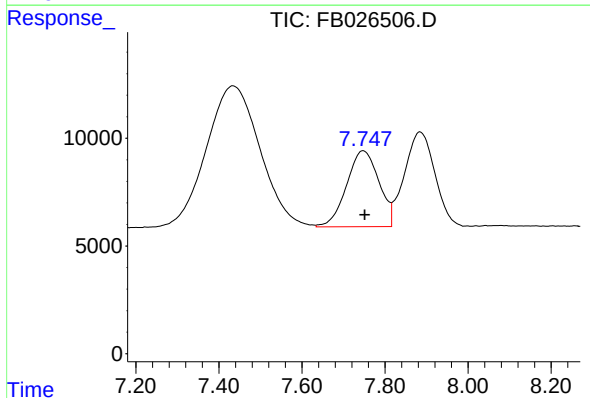


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 191145
Conc: 9.99 ng/ml

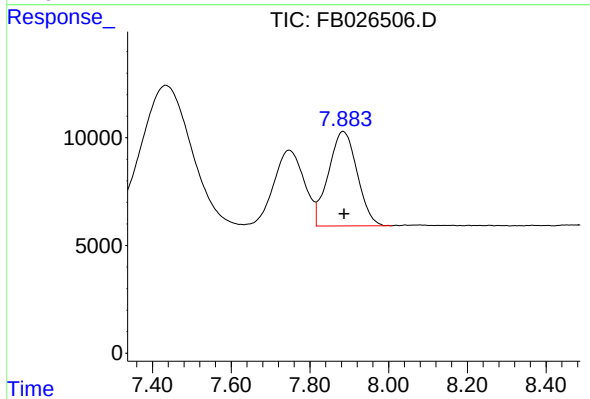

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 223009
Conc: 10.03 ng/ml

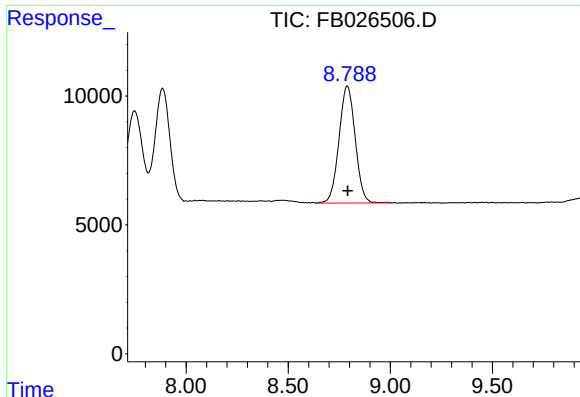

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 250759
Conc: 22.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1214S1

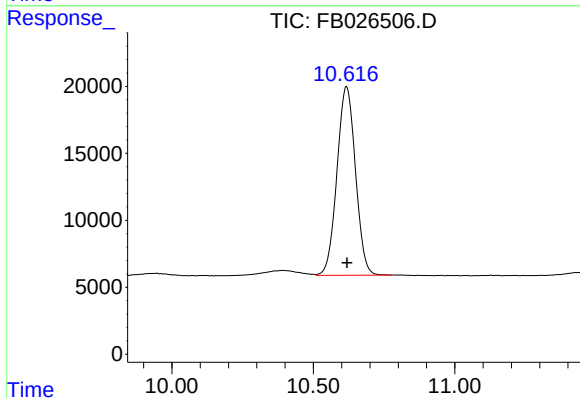


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.001 min
Response: 641308
Conc: 30.05 ng/ml

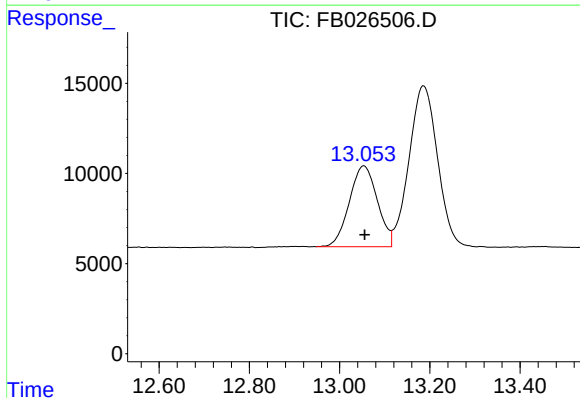


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.001 min
Response: 194108
Conc: 9.83 ng/ml

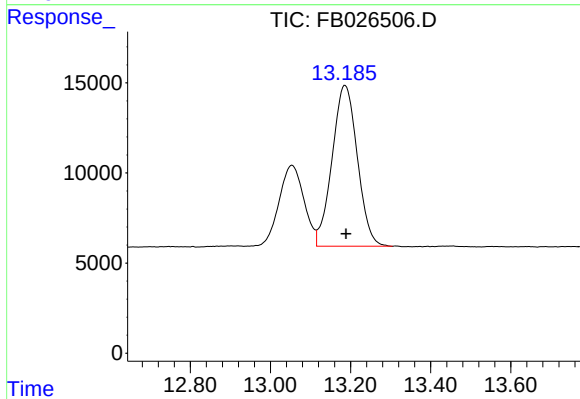

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.003 min
Response: 391430
Conc: 19.85 ng/ml

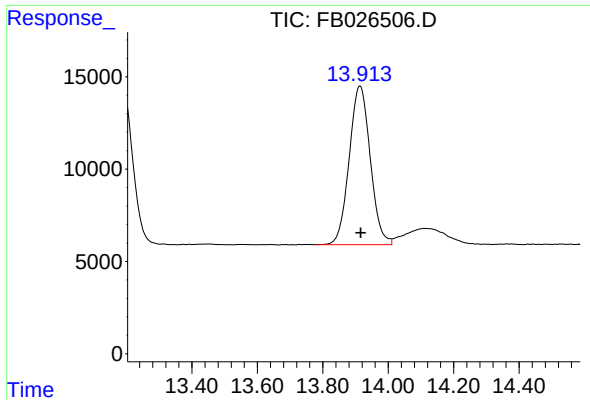

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.002 min
Response: 384055
Conc: 20.11 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1214S1

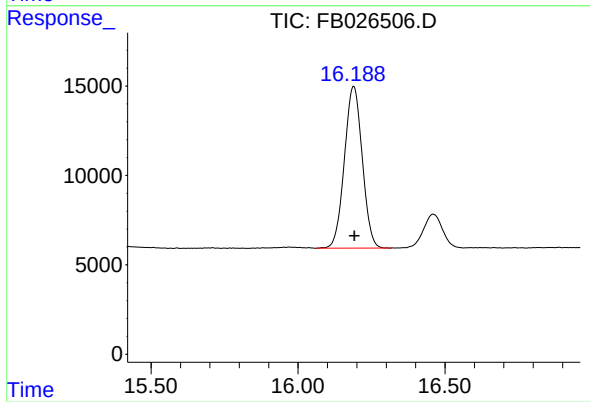

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.003 min
Response: 381053
Conc: 19.61 ng/ml