

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121421\
 Data File : FB026516.D
 Signal(s) : FID2B.CH
 Acq On : 14 Dec 2021 19:45
 Operator : AJ/MA
 Sample : M5074-02MS
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 CS-1MS

Integration File: Calibration.e
 Quant Time: Dec 15 03:28:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	222914	19.841 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	531080	30.510 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	610109	30.764 ng/ml
3) t n-Heptane	7.746	190248	9.939 ng/ml
4) t Benzene	7.882	226960	10.208 ng/ml
6) t Toluene	10.615	660963	30.976 ng/ml
7) t Ethylbenzene	13.052	202469	10.256 ng/ml
8) t m-Xylene	13.185	404956	20.540 ng/ml
9) t O-Xylene	13.912	397520	20.816 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	401330	20.658 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121421\
Data File : FB026516.D
Signal(s) : FID2B.CH
Acq On : 14 Dec 2021 19:45
Operator : AJ/MA
Sample : M5074-02MS
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
CS-1MS

Integration File: Calibration.e
Quant Time: Dec 15 03:28:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

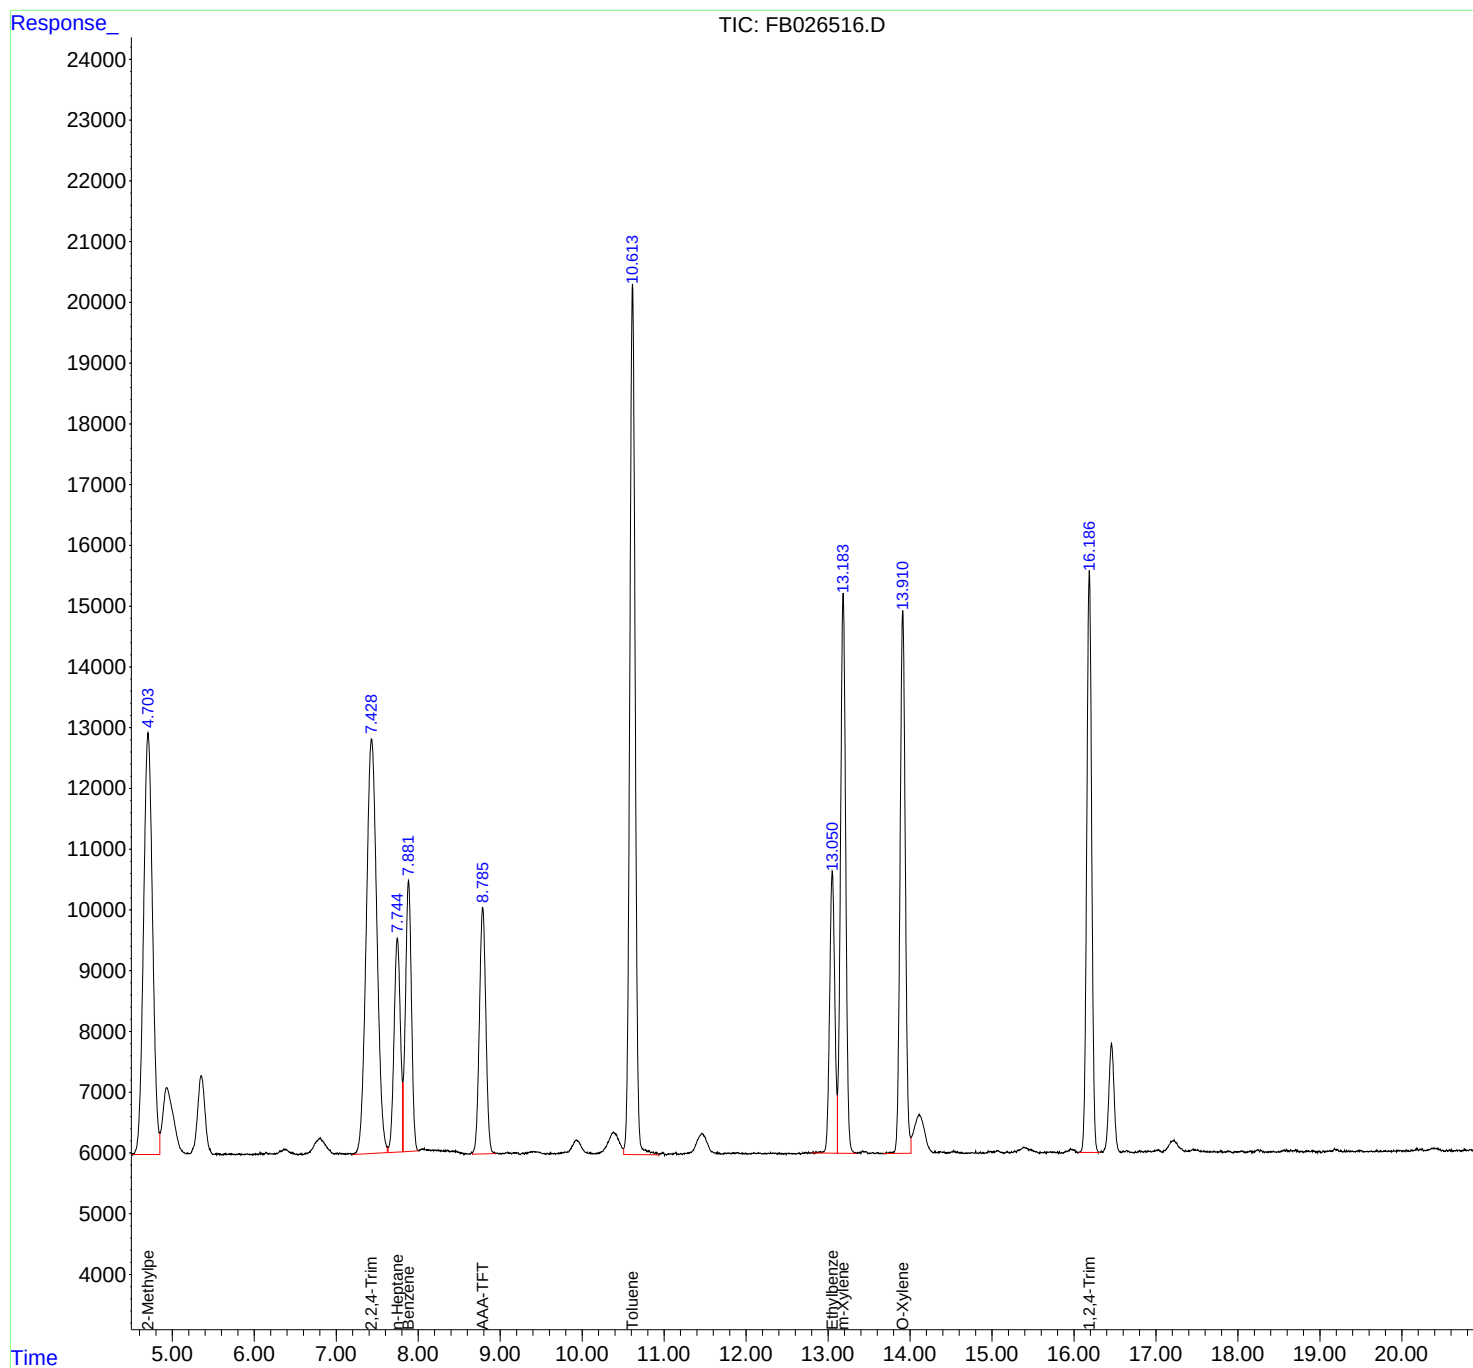


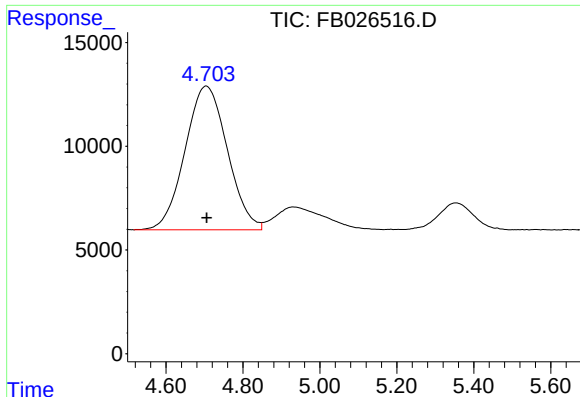

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.001 min
Response: 531080
Conc: 30.51 ng/ml

Instrument :
FID_B
ClientSampleId :
CS-1MS

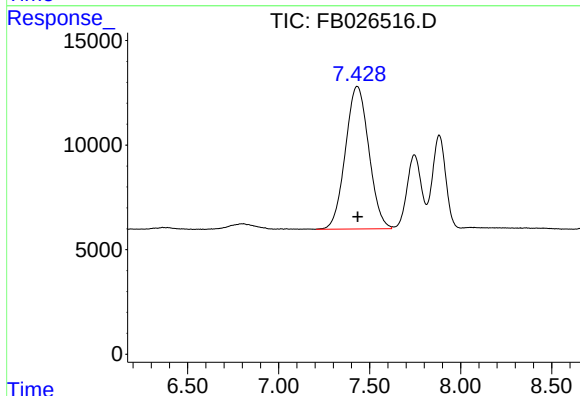


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: -0.005 min
Response: 610109
Conc: 30.76 ng/ml

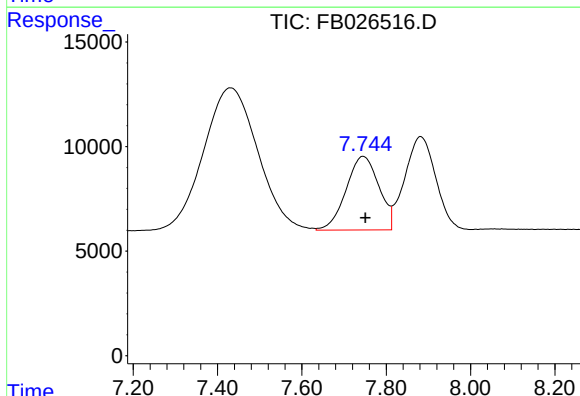


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.005 min
Response: 190248
Conc: 9.94 ng/ml

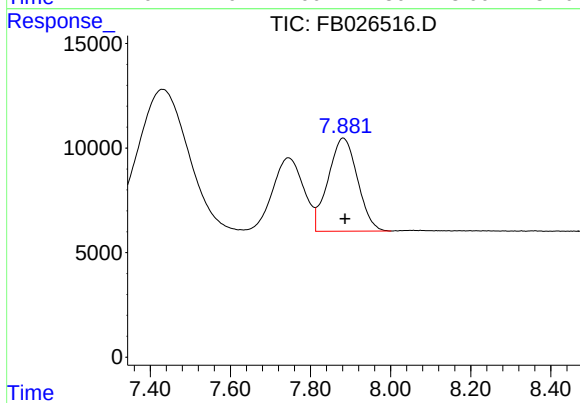

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.005 min
Response: 226960
Conc: 10.21 ng/ml

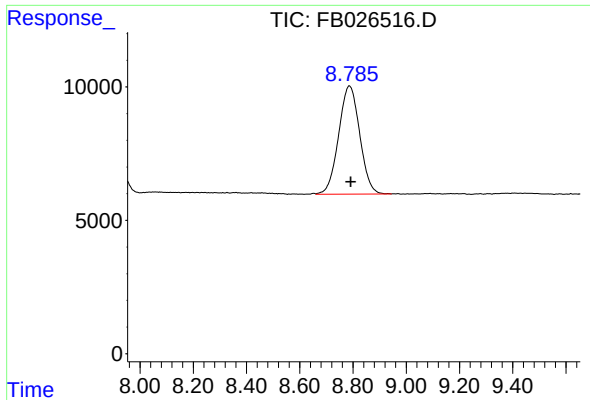

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.005 min
Response: 222914
Conc: 19.84 ng/ml

Instrument :
FID_B
ClientSampleId :
CS-1MS

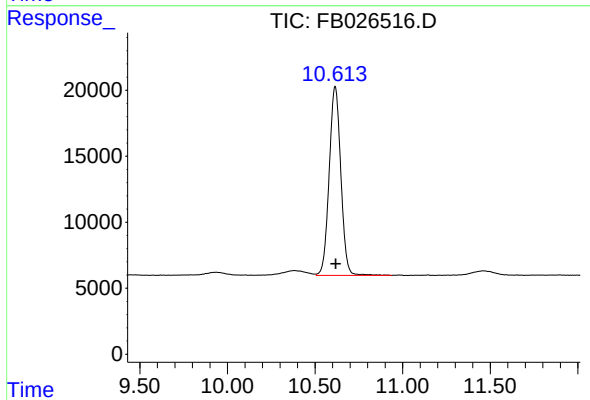


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.004 min
Response: 660963
Conc: 30.98 ng/ml

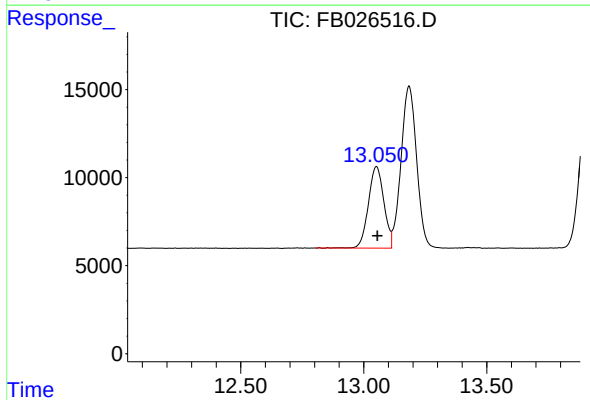


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.004 min
Response: 202469
Conc: 10.26 ng/ml

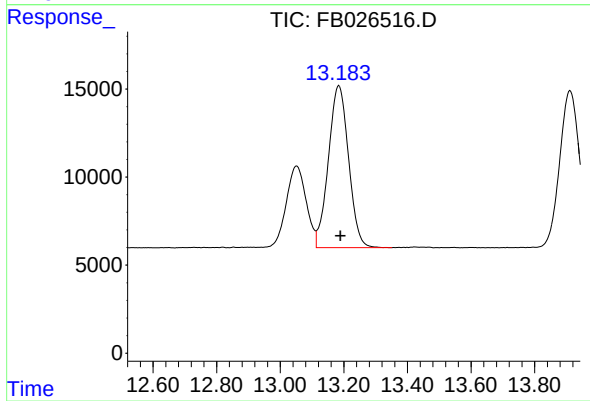

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.005 min
Response: 404956
Conc: 20.54 ng/ml

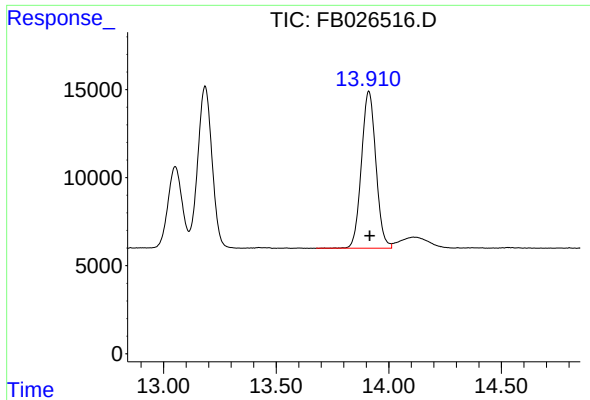

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.004 min
Response: 397520
Conc: 20.82 ng/ml

Instrument :
FID_B
ClientSampleId :
CS-1MS

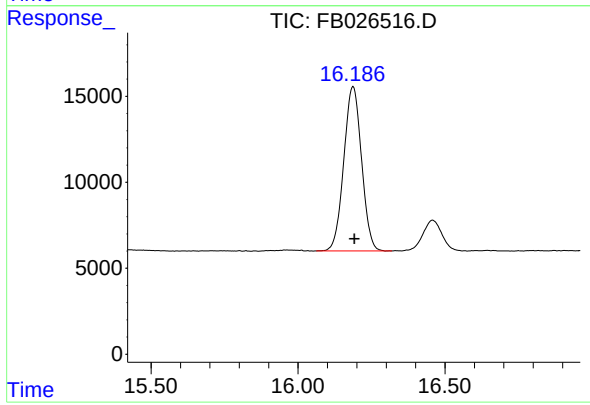

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.005 min
Response: 401330
Conc: 20.66 ng/ml