

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121421\
 Data File : FB026518.D
 Signal(s) : FID2B.CH
 Acq On : 14 Dec 2021 20:57
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Dec 15 03:28:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	223228	19.869 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	515978	29.642 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	605808	30.548 ng/ml
3) t n-Heptane	7.746	186321	9.733 ng/ml
4) t Benzene	7.883	220131	9.901 ng/ml
6) t Toluene	10.615	640857	30.034 ng/ml
7) t Ethylbenzene	13.052	198700	10.065 ng/ml
8) t m-Xylene	13.185	400755	20.326 ng/ml
9) t O-Xylene	13.911	394377	20.651 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	401028	20.643 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121421\
Data File : FB026518.D
Signal(s) : FID2B.CH
Acq On : 14 Dec 2021 20:57
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Dec 15 03:28:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

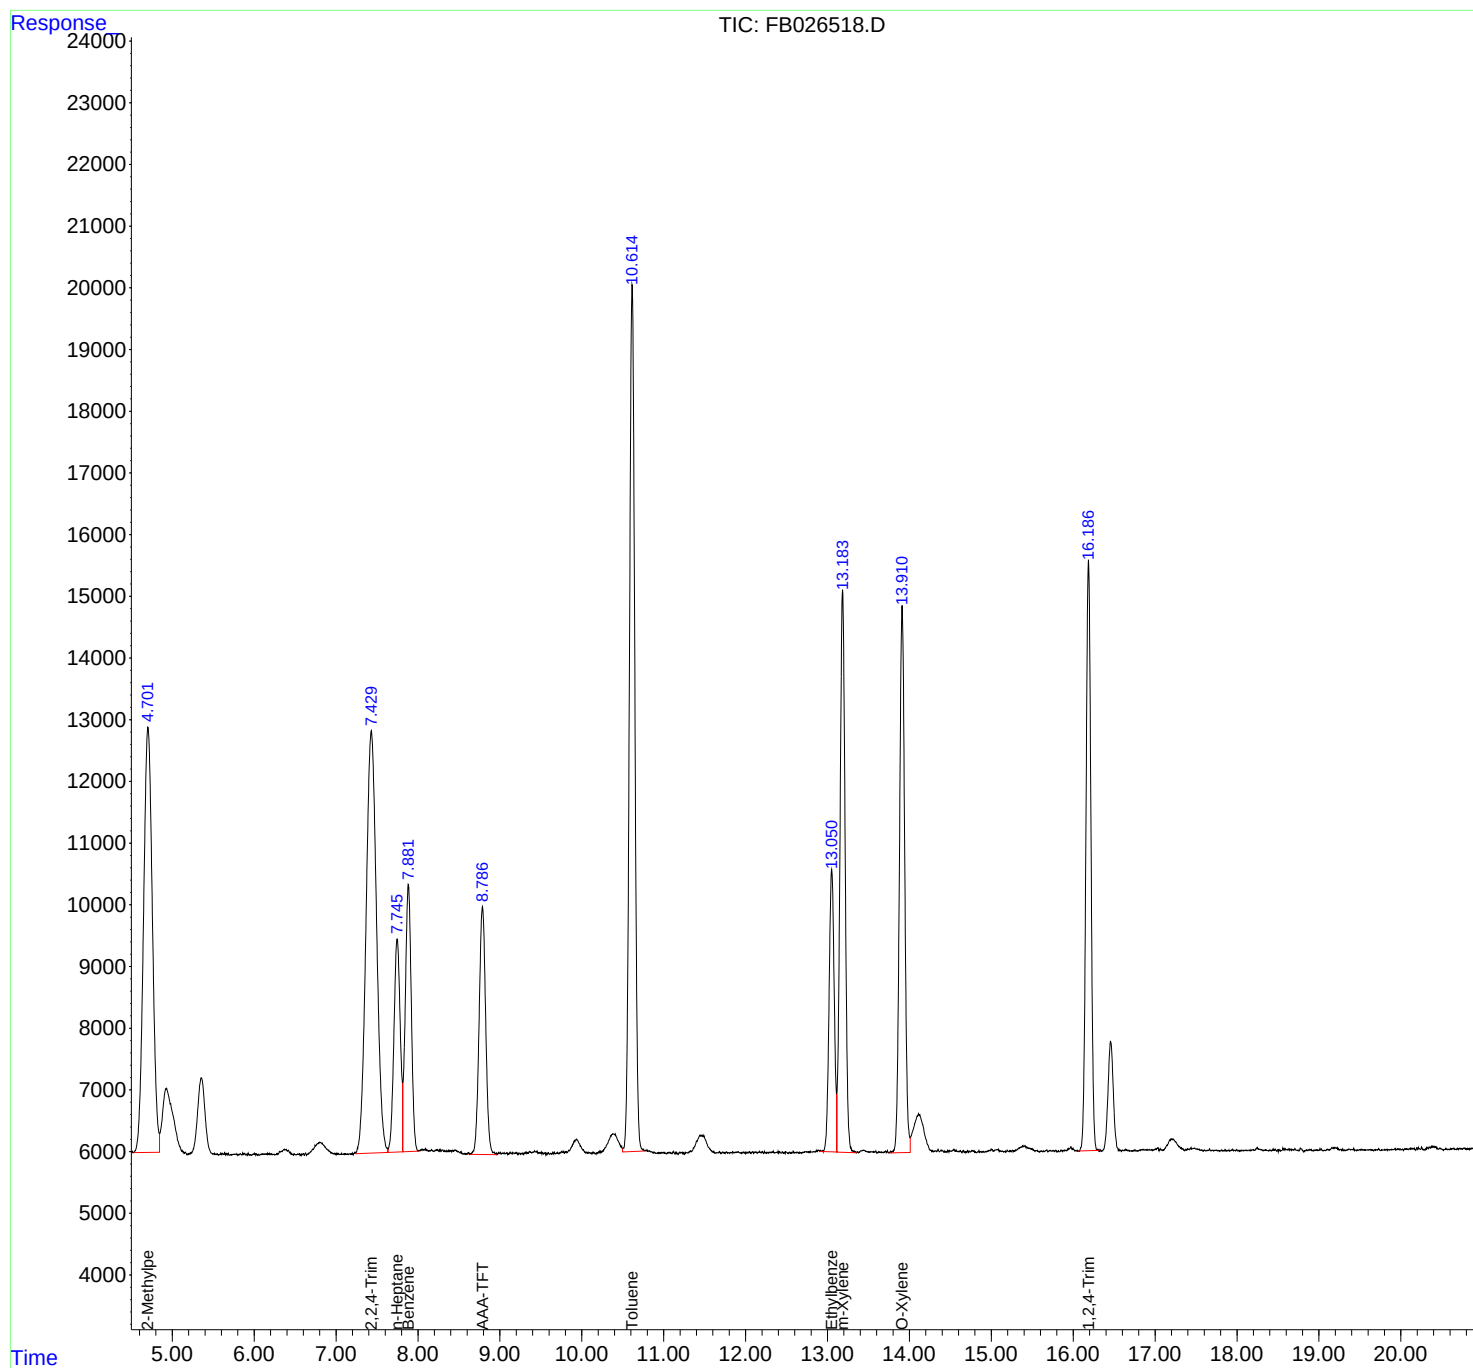


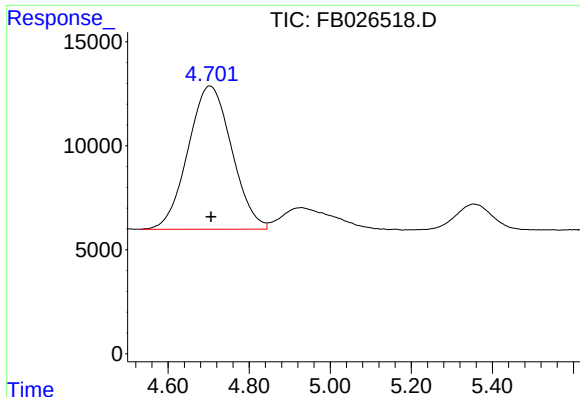

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.003 min
Response: 515978
Conc: 29.64 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

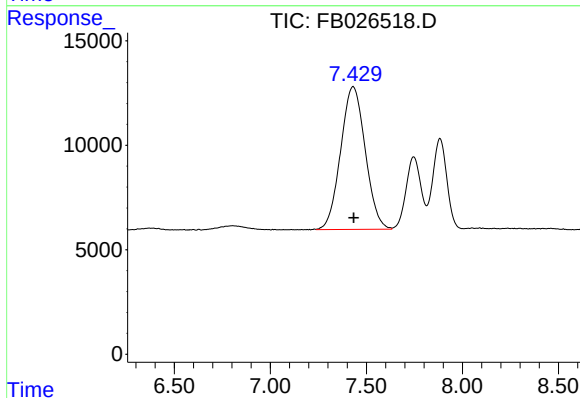


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: -0.005 min
Response: 605808
Conc: 30.55 ng/ml

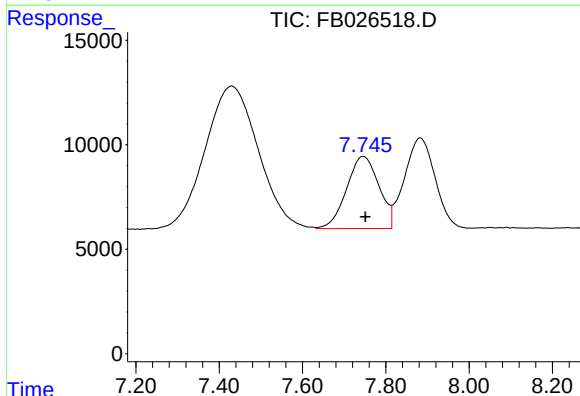


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.005 min
Response: 186321
Conc: 9.73 ng/ml

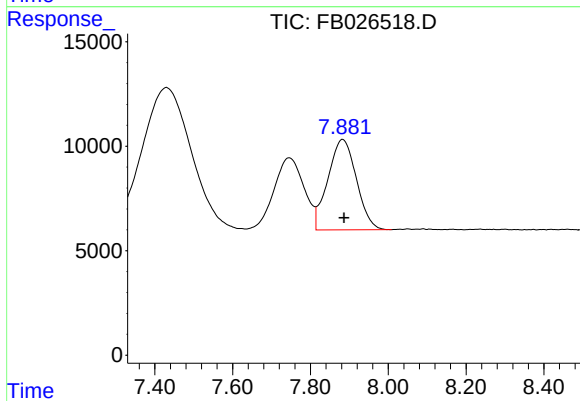

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.004 min
Response: 220131
Conc: 9.90 ng/ml

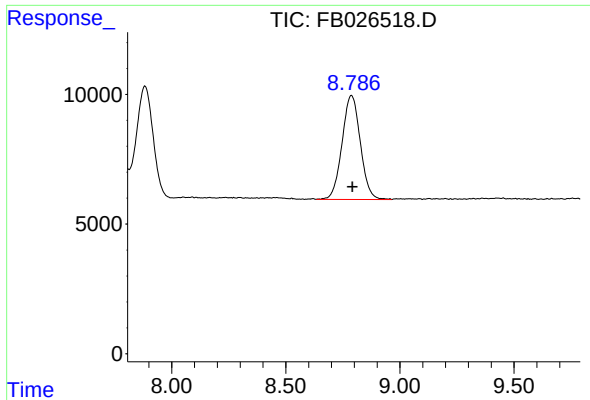

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.004 min
Response: 223228
Conc: 19.87 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

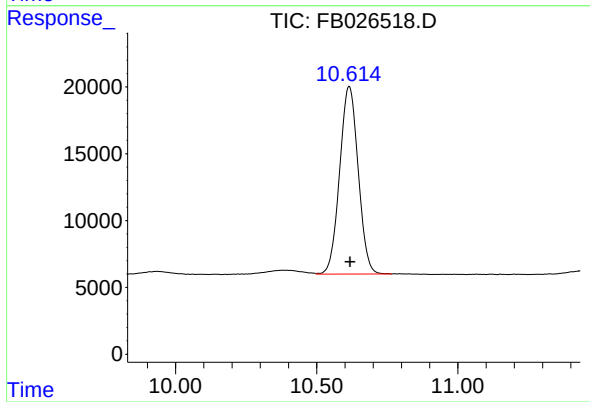


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.003 min
Response: 640857
Conc: 30.03 ng/ml

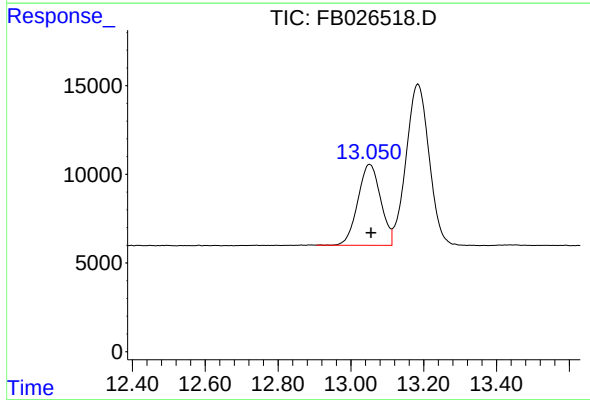


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.004 min
Response: 198700
Conc: 10.07 ng/ml

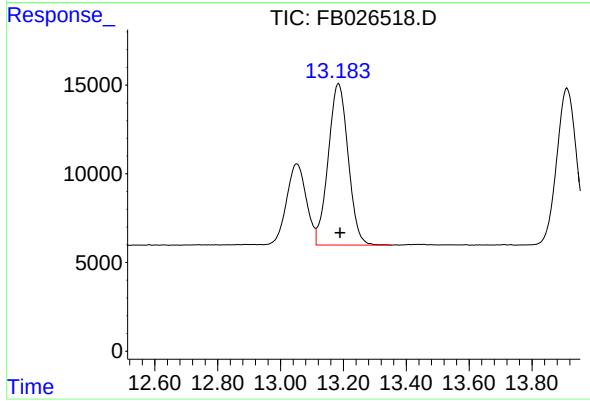

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.005 min
Response: 400755
Conc: 20.33 ng/ml

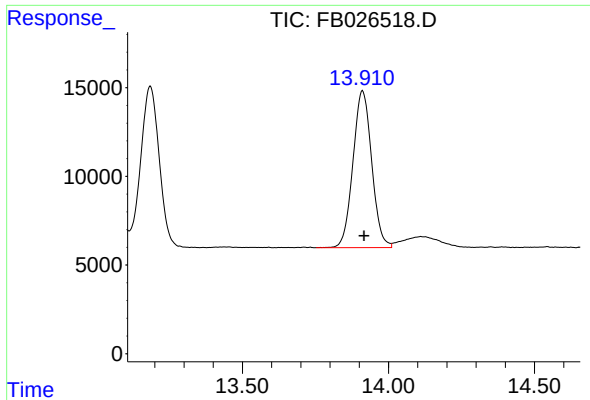

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.005 min
Response: 394377
Conc: 20.65 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

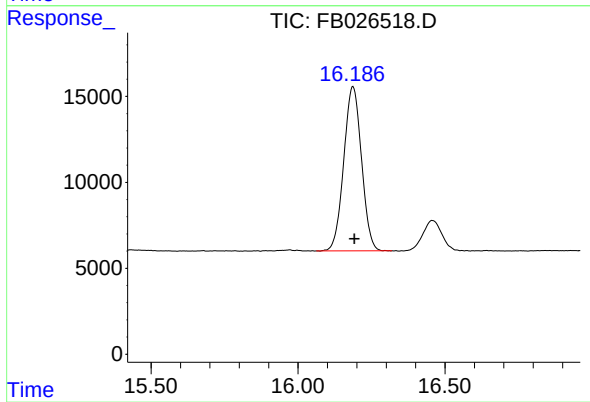

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.005 min
Response: 401028
Conc: 20.64 ng/ml