

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121520\
 Data File : FB025354.D
 Signal(s) : FID2B.CH
 Acq On : 15 Dec 2020 9:04
 Operator : DD/AJ
 Sample : BSF1215S2
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1215S2

Integration File: Calibration.e
 Quant Time: Dec 16 00:26:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	421871	20.067 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	885116	29.441 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	927626	30.829 ng/ml
3) t n-Heptane	7.756	304316	10.277 ng/ml
4) t Benzene	7.891	364781	9.862 ng/ml
6) t Toluene	10.628	1051051	29.910 ng/ml
7) t Ethylbenzene	13.069	323197	9.895 ng/ml
8) t m-Xylene	13.201	647350	20.001 ng/ml
9) t O-Xylene	13.929	623576	19.725 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	538353	19.825 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121520\
Data File : FB025354.D
Signal(s) : FID2B.CH
Acq On : 15 Dec 2020 9:04
Operator : DD/AJ
Sample : BSF1215S2
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1215S2

Integration File: Calibration.e
Quant Time: Dec 16 00:26:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

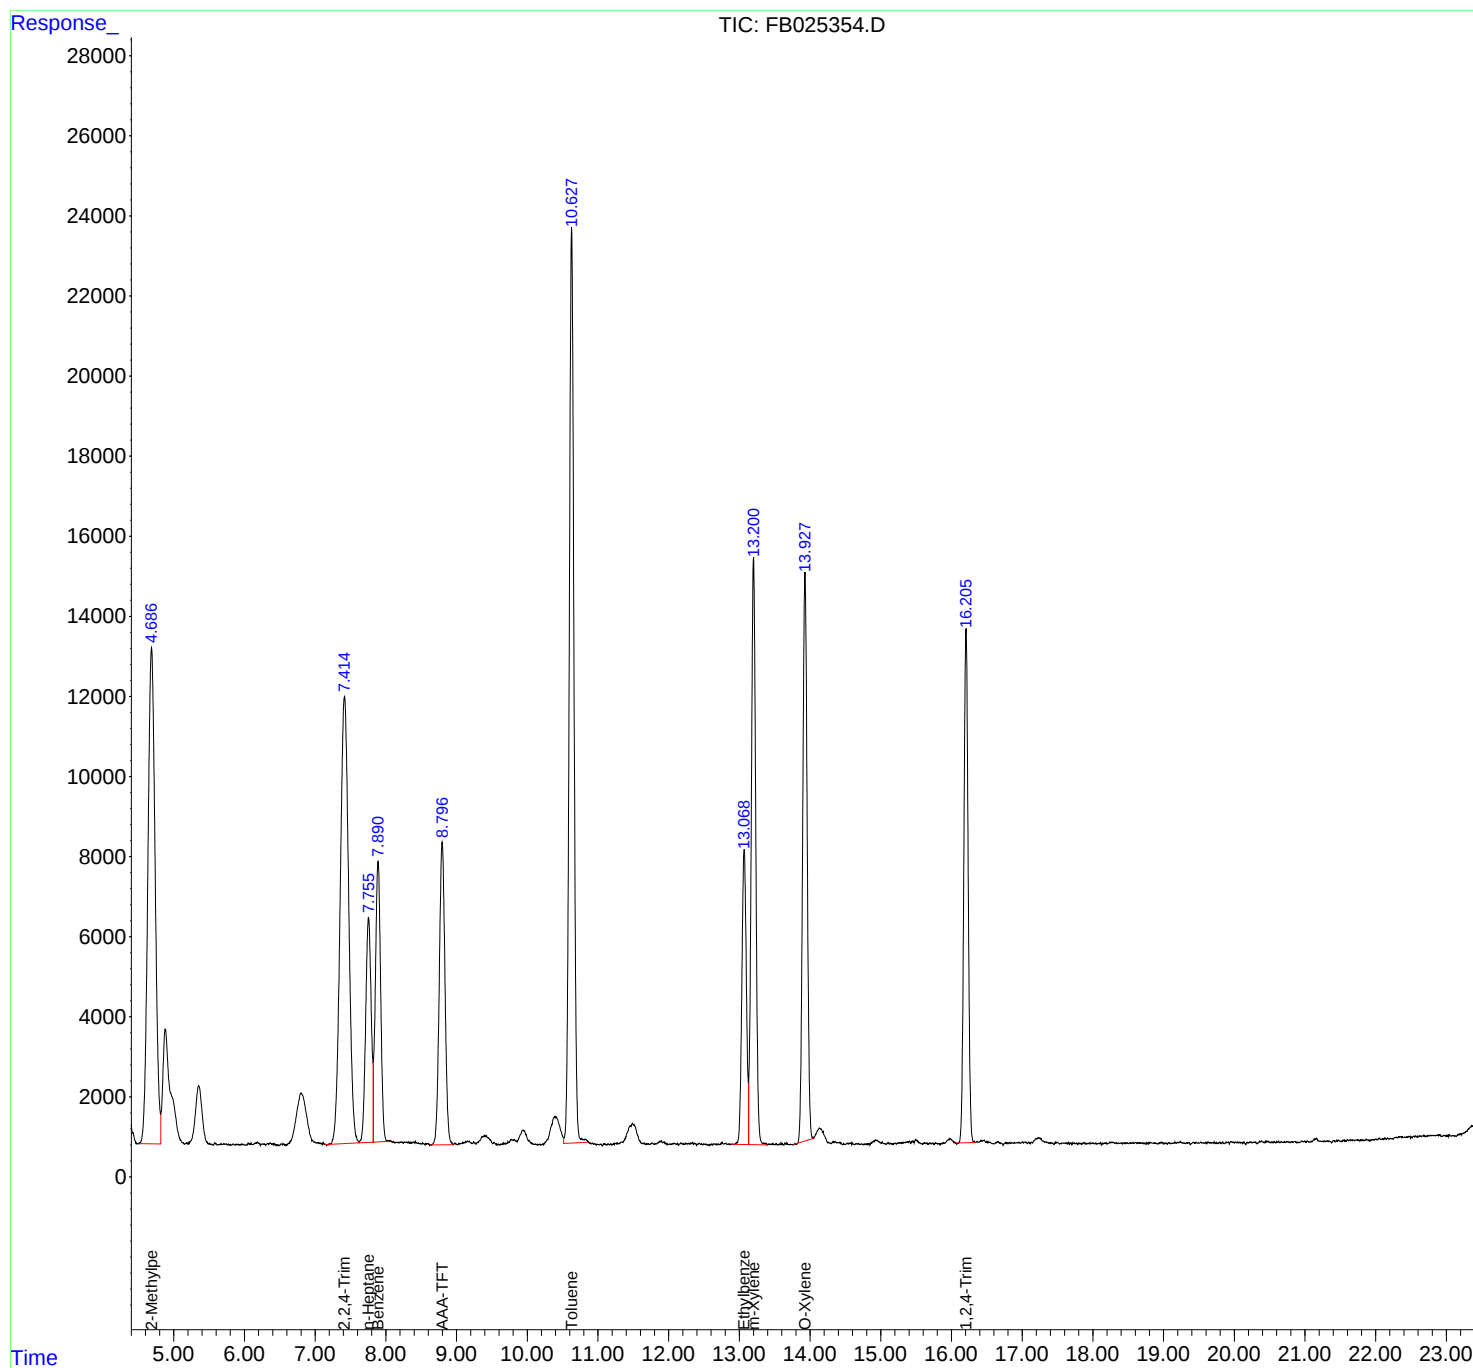


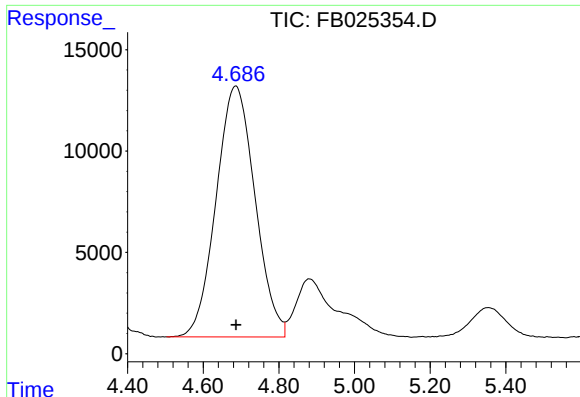

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 885116
Conc: 29.44 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1215S2

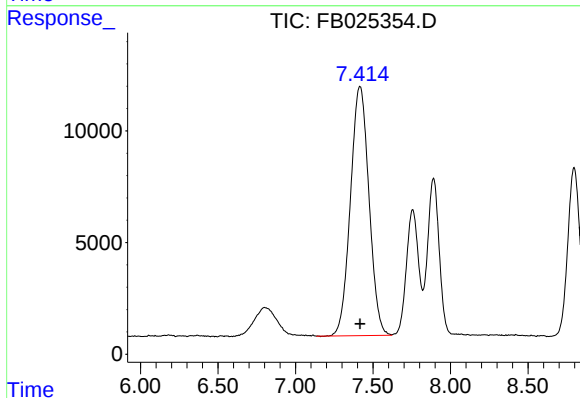


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 927626
Conc: 30.83 ng/ml

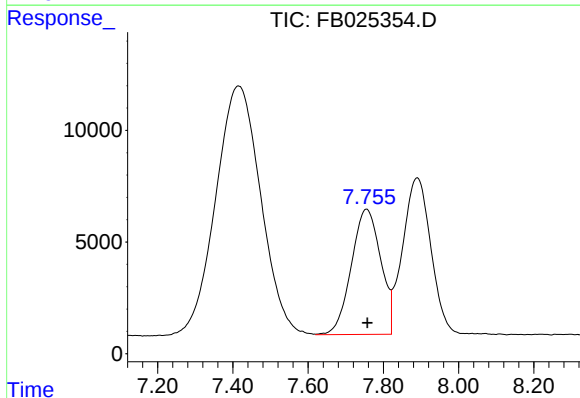


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 304316
Conc: 10.28 ng/ml

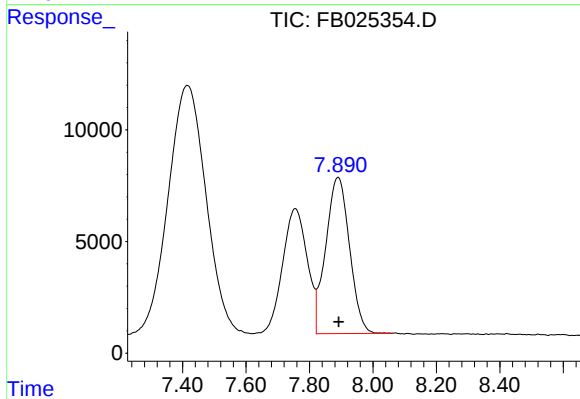

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 364781
Conc: 9.86 ng/ml

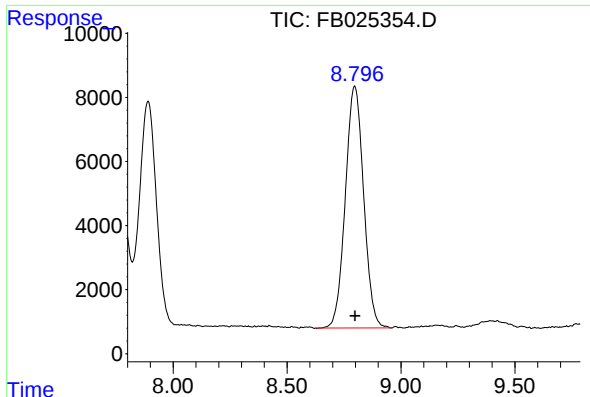

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 421871
Conc: 20.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1215S2

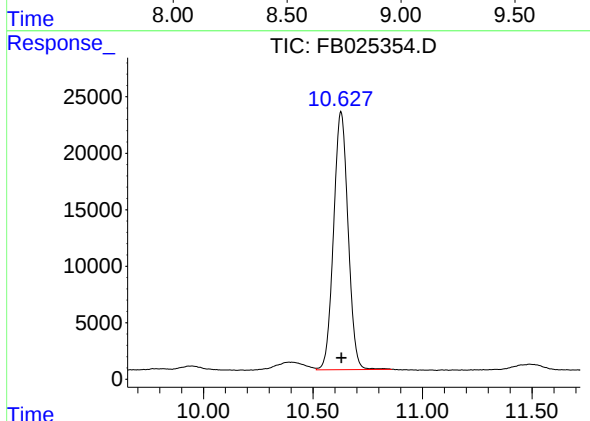


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 1051051
Conc: 29.91 ng/ml

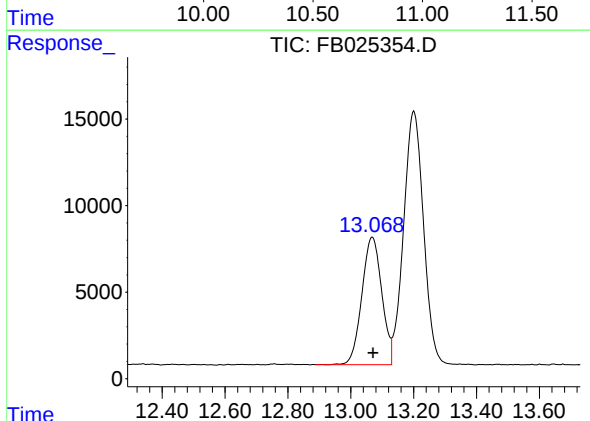


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 323197
Conc: 9.89 ng/ml

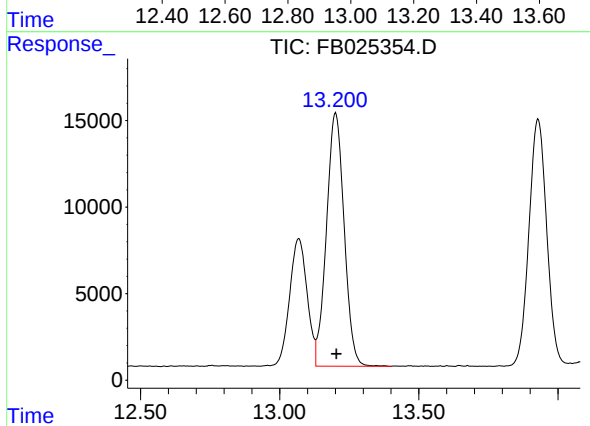

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.003 min
Response: 647350
Conc: 20.00 ng/ml

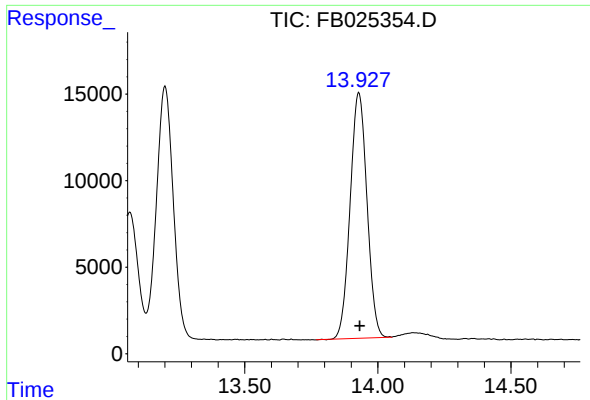

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.003 min
Response: 623576
Conc: 19.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1215S2

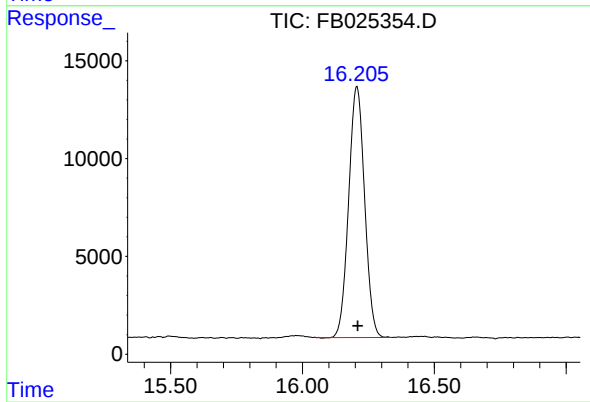

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.003 min
Response: 538353
Conc: 19.82 ng/ml