

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121520\
Data File : FB025356.D
Signal(s) : FID2B.CH
Acq On : 15 Dec 2020 11:01
Operator : DD/AJ
Sample : L5069-02
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-B7-121120-0-4

Integration File: Calibration.e
Quant Time: Dec 16 00:26:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	414355	19.709 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121520\
Data File : FB025356.D
Signal(s) : FID2B.CH
Acq On : 15 Dec 2020 11:01
Operator : DD/AJ
Sample : L5069-02
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-B7-121120-0-4

Integration File: Calibration.e
Quant Time: Dec 16 00:26:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

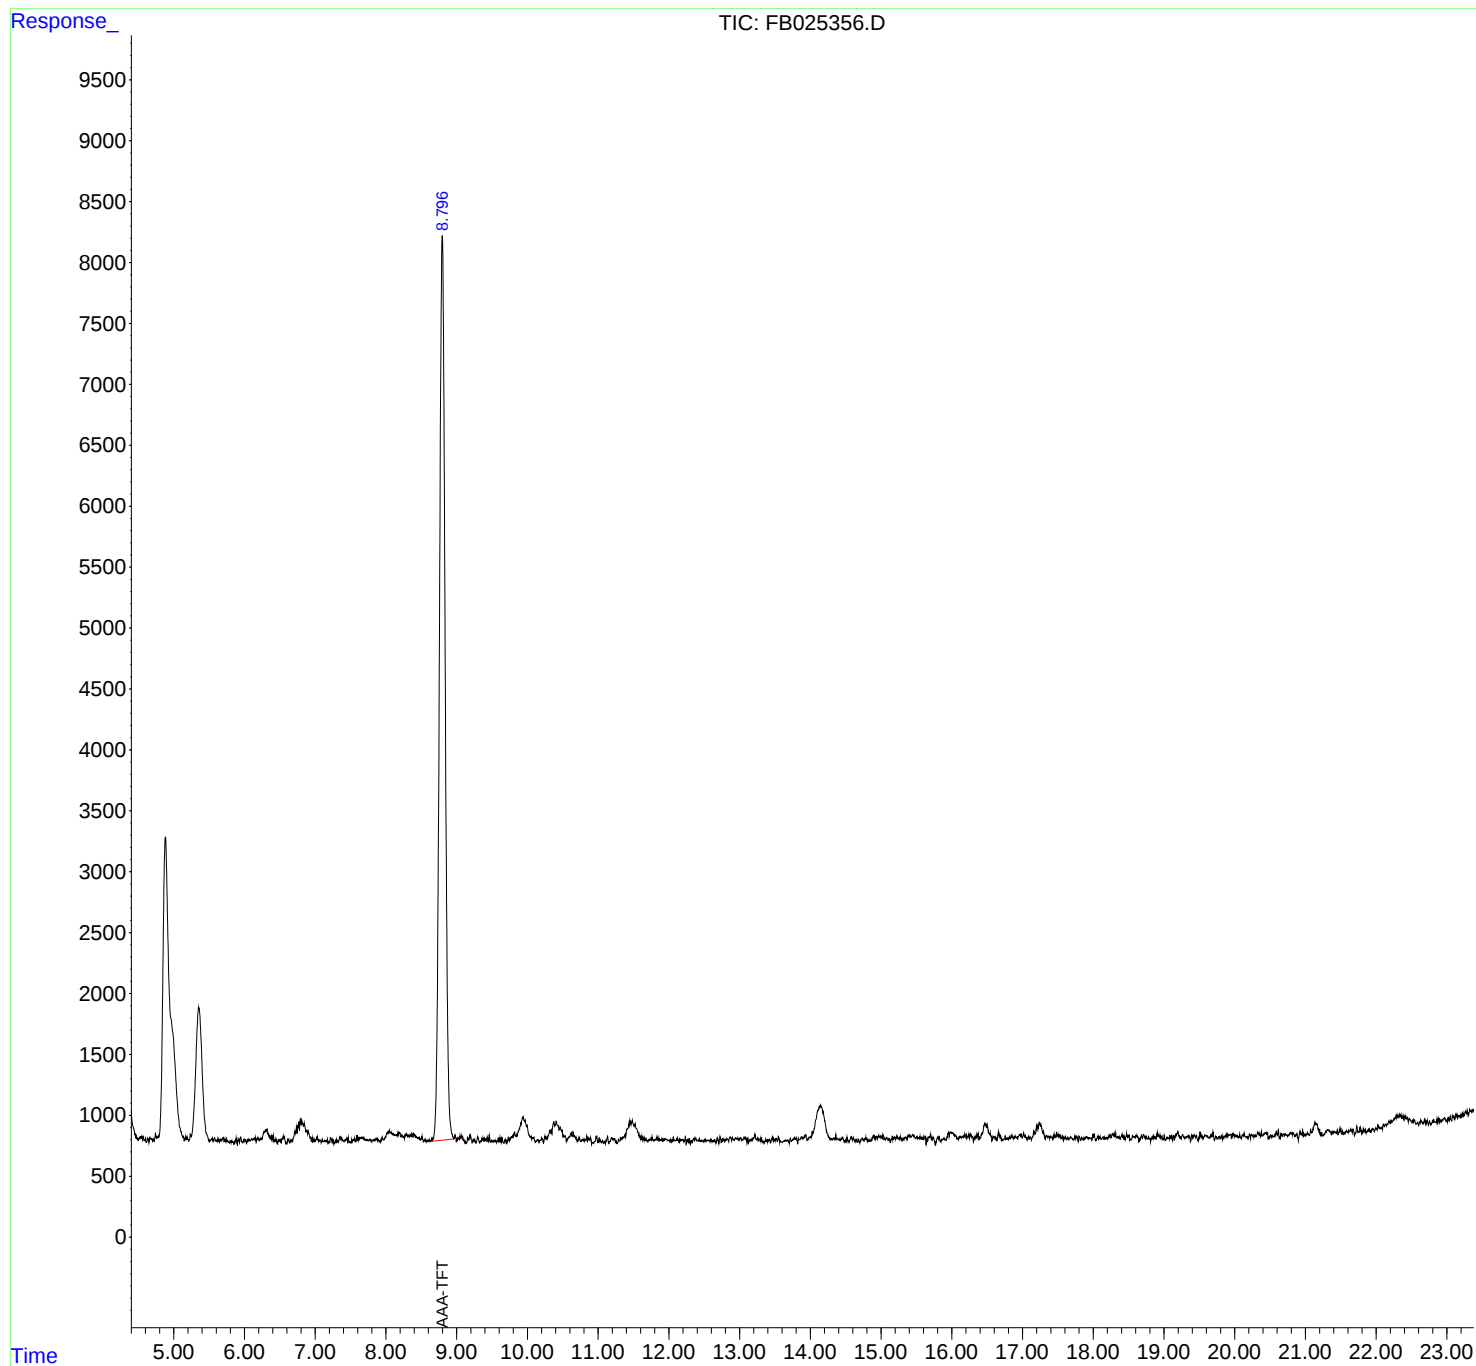

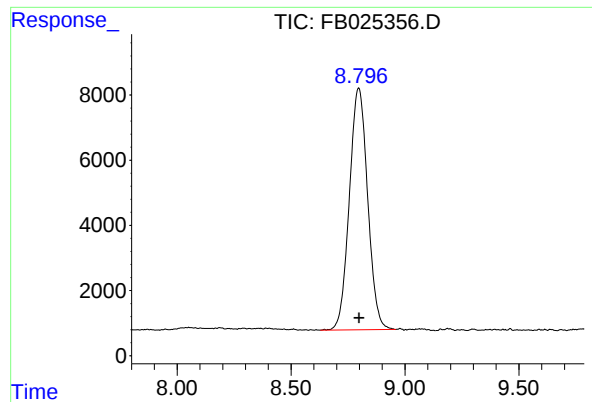

#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.001 min
Response: 414355
Conc: 19.71 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B7-121120-0-4