

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121520\
 Data File : FB025359.D
 Signal(s) : FID2B.CH
 Acq On : 15 Dec 2020 12:32
 Operator : DD/AJ
 Sample : L5069-04MSD
 Misc : 5.08g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 KENS-B7-121120-13-15MSD

Integration File: Calibration.e
 Quant Time: Dec 16 00:26:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	474757	22.583 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	849307	28.250 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	811758	26.978 ng/ml
3) t n-Heptane	7.755	270401	9.131 ng/ml
4) t Benzene	7.890	355573	9.613 ng/ml
6) t Toluene	10.629	1001650	28.504 ng/ml
7) t Ethylbenzene	13.069	302969	9.275 ng/ml
8) t m-Xylene	13.201	609548	18.833 ng/ml
9) t O-Xylene	13.929	591785	18.720 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	512333	18.867 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121520\
Data File : FB025359.D
Signal(s) : FID2B.CH
Acq On : 15 Dec 2020 12:32
Operator : DD/AJ
Sample : L5069-04MSD
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
KENS-B7-121120-13-15MSD

Integration File: Calibration.e
Quant Time: Dec 16 00:26:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

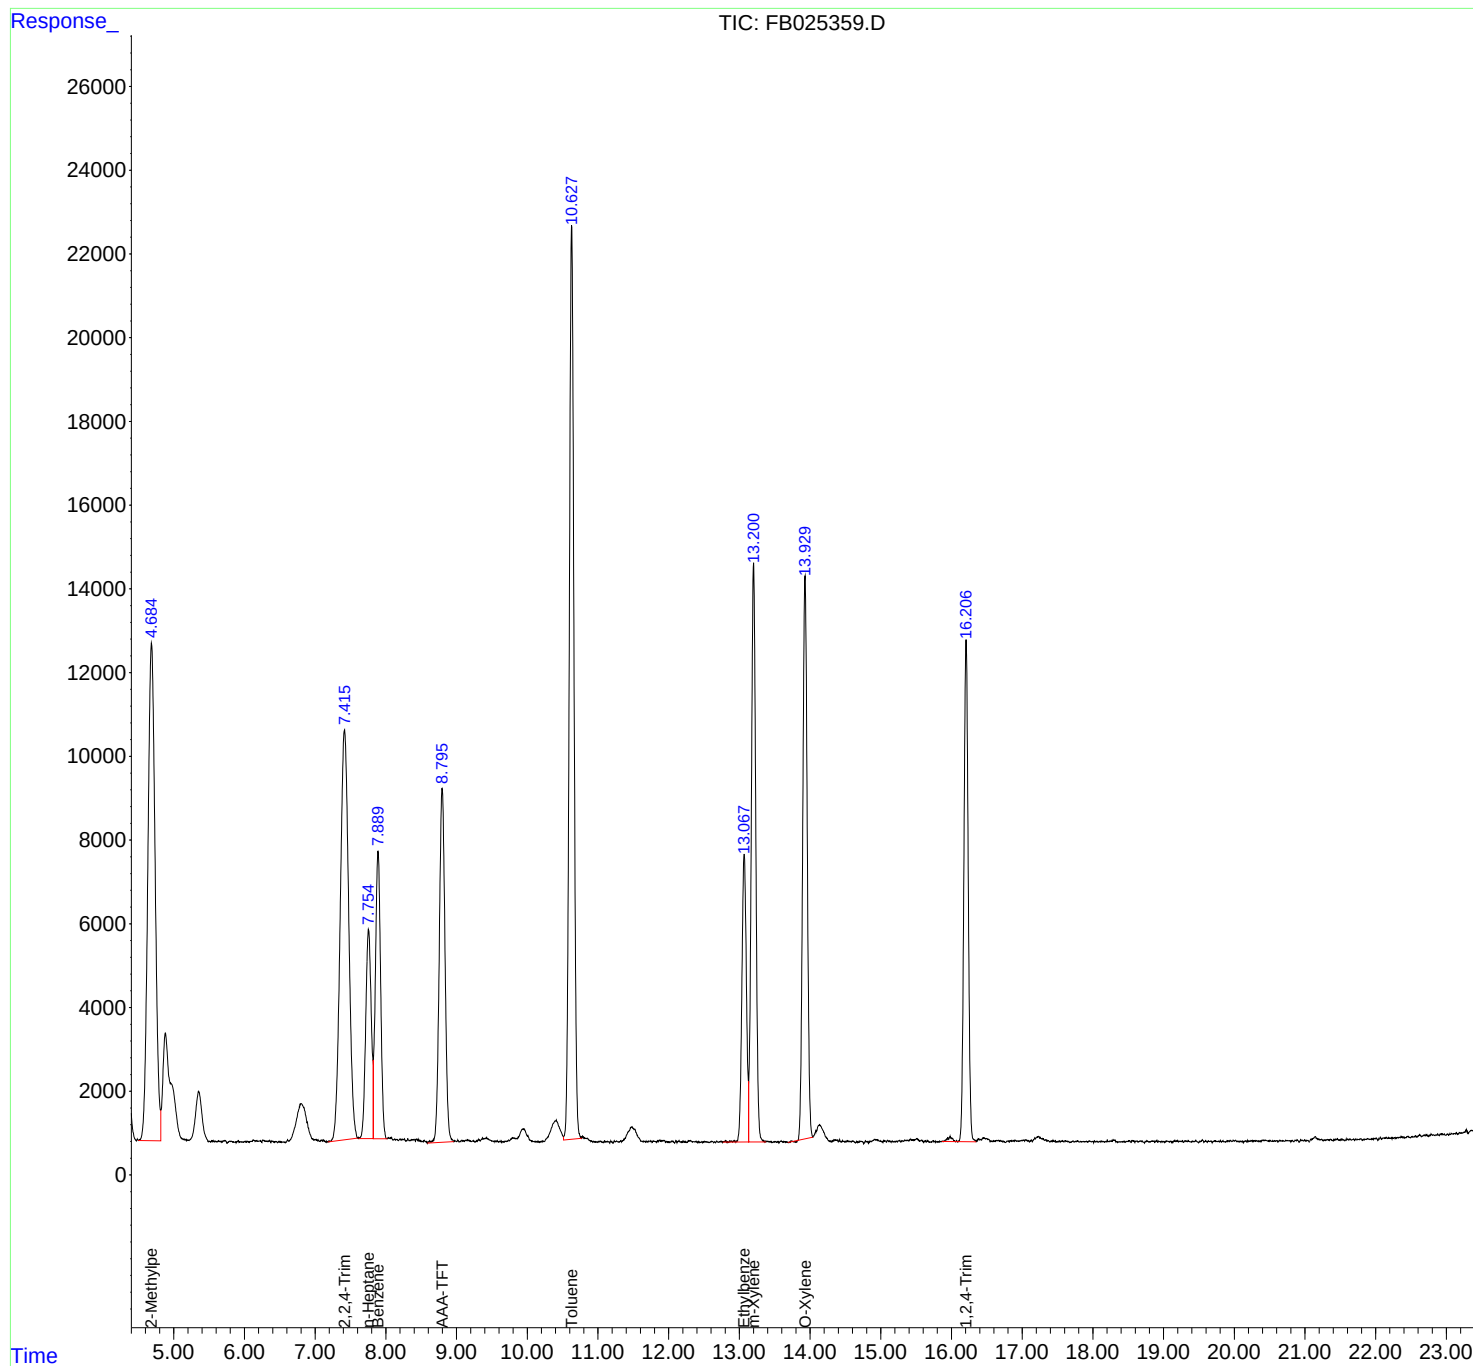


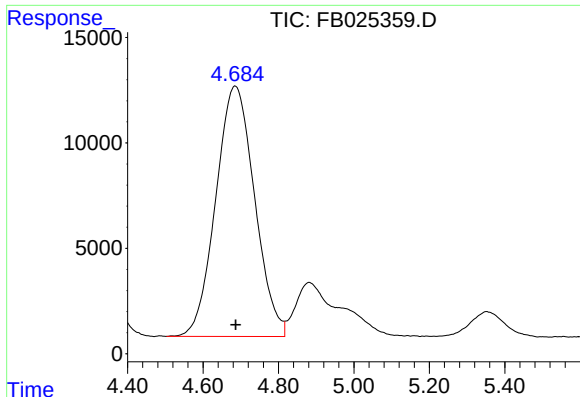

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: -0.001 min
Response: 849307
Conc: 28.25 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B7-121120-13-15MSD

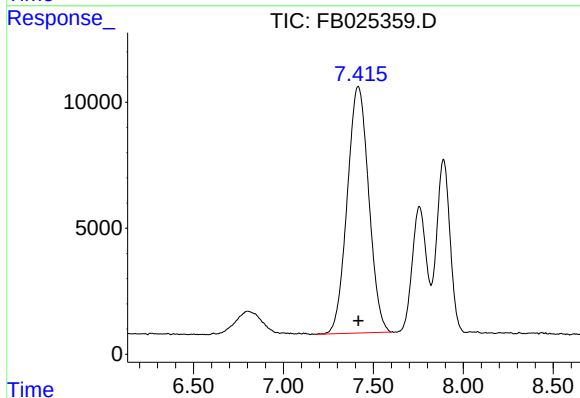


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 811758
Conc: 26.98 ng/ml

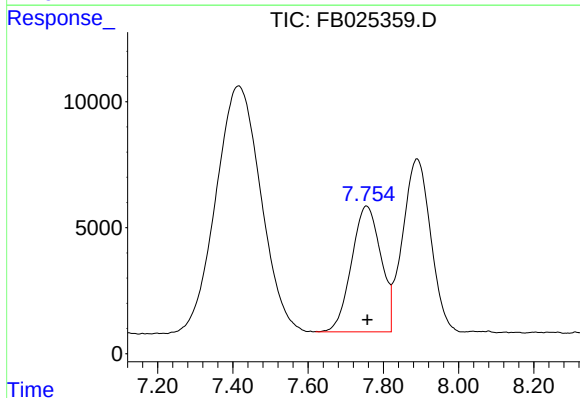


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 270401
Conc: 9.13 ng/ml

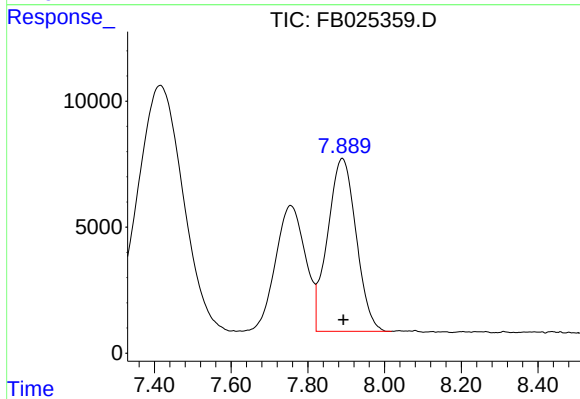

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 355573
Conc: 9.61 ng/ml

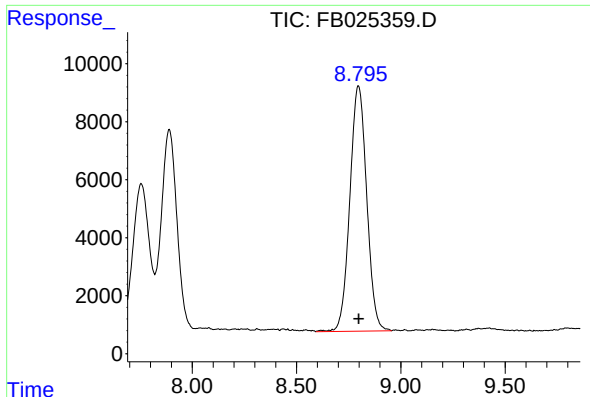

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 474757
Conc: 22.58 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B7-121120-13-15MSD

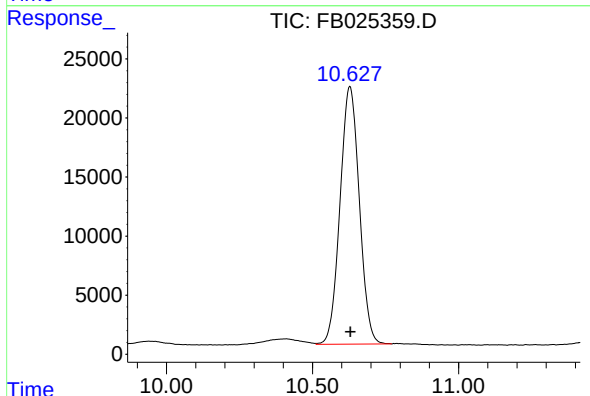


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.002 min
Response: 1001650
Conc: 28.50 ng/ml

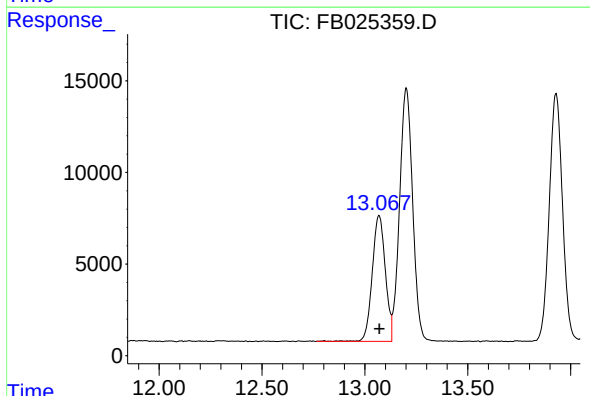


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 302969
Conc: 9.28 ng/ml

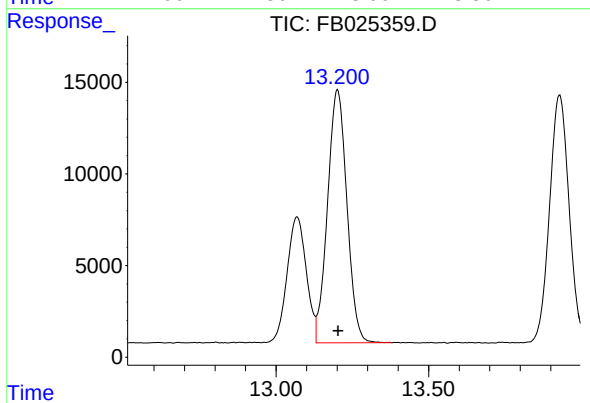

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 609548
Conc: 18.83 ng/ml

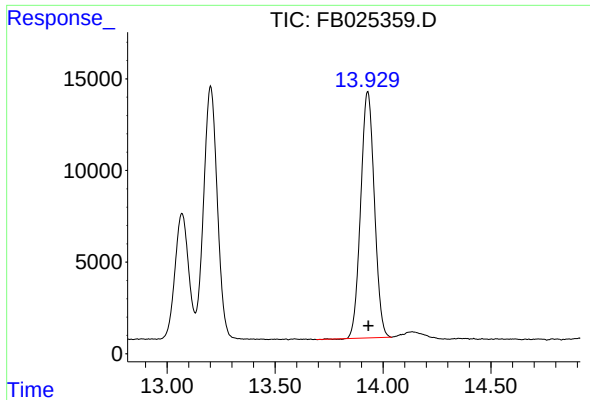

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 591785
Conc: 18.72 ng/ml

Instrument :
FID_B
ClientSampleId :
KENS-B7-121120-13-15MSD

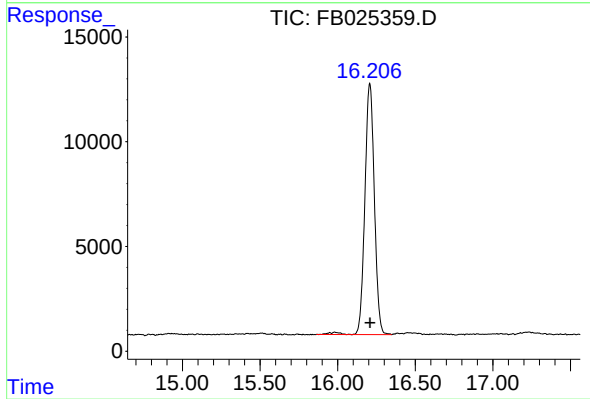

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 512333
Conc: 18.87 ng/ml