

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121521\
 Data File : FB026525.D
 Signal(s) : FID2B.CH
 Acq On : 15 Dec 2021 15:16
 Operator : AJ/MA
 Sample : M5065-01MSD
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 16 00:18:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	146183	13.012 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	281799	16.189 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	295467	14.899 ng/ml
3) t n-Heptane	7.745	100729	5.262 ng/ml
4) t Benzene	7.882	173891	7.821 ng/ml
6) t Toluene	10.615	454385	21.295 ng/ml
7) t Ethylbenzene	13.052	126399	6.403 ng/ml
8) t m-Xylene	13.185	234495	11.894 ng/ml
9) t O-Xylene	13.912	245860	12.874 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	190671	9.815 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121521\
 Data File : FB026525.D
 Signal(s) : FID2B.CH
 Acq On : 15 Dec 2021 15:16
 Operator : AJ/MA
 Sample : M5065-01MSD
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 16 00:18:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

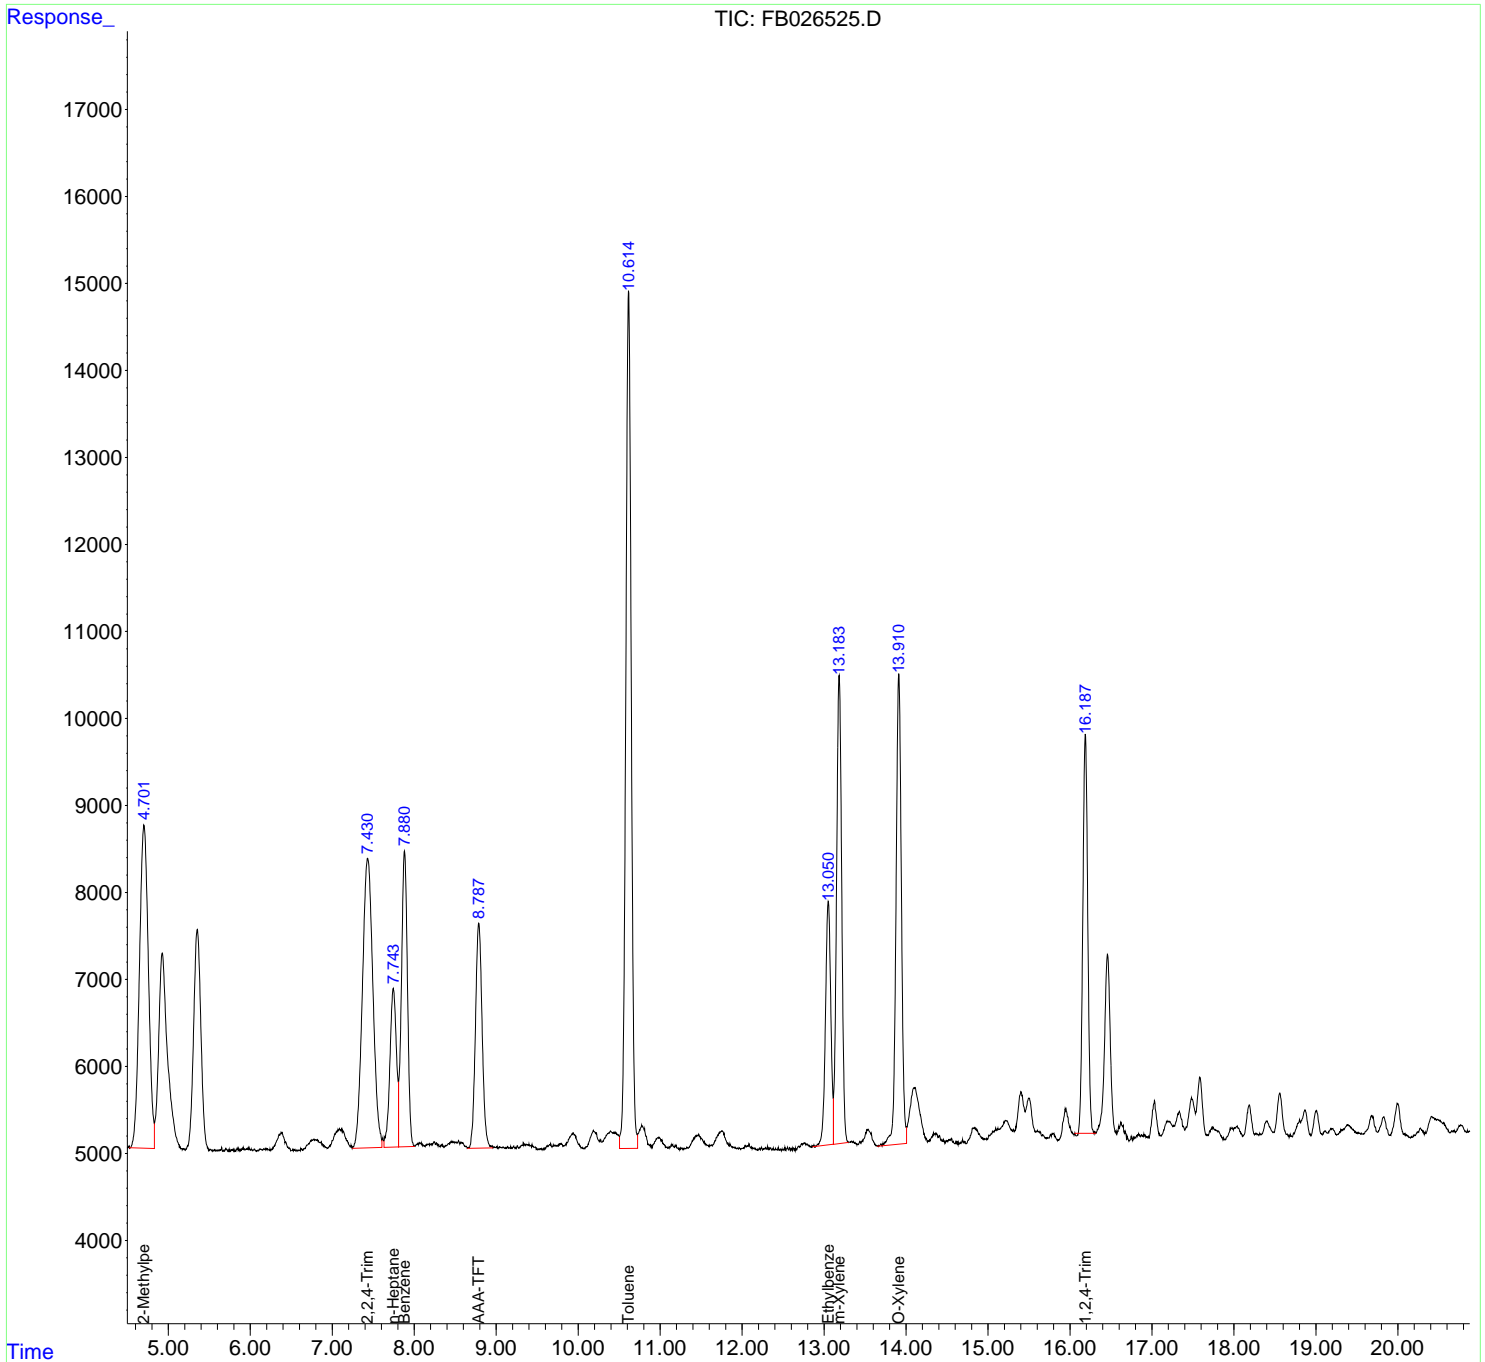


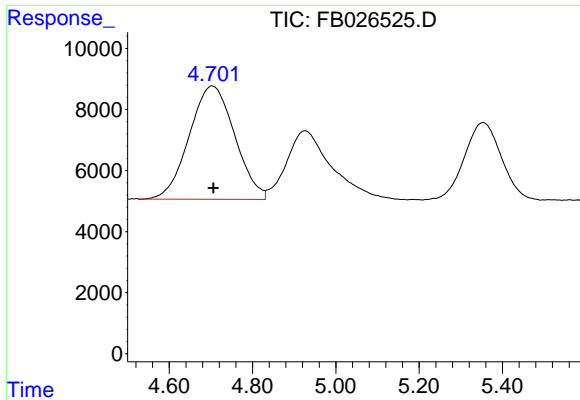

#1 2-Methylpentane


R.T.: 4.703 min
 Delta R.T.: -0.003 min
 Response: 281799
 Conc: 16.19 ng/ml

Instrument :
 FID_B
 ClientSampleId :

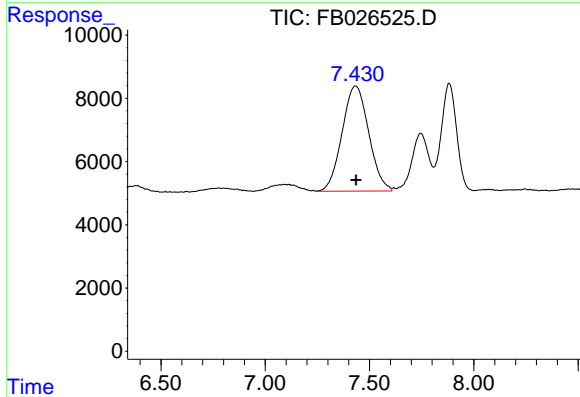


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
 Delta R.T.: -0.003 min
 Response: 295467
 Conc: 14.90 ng/ml

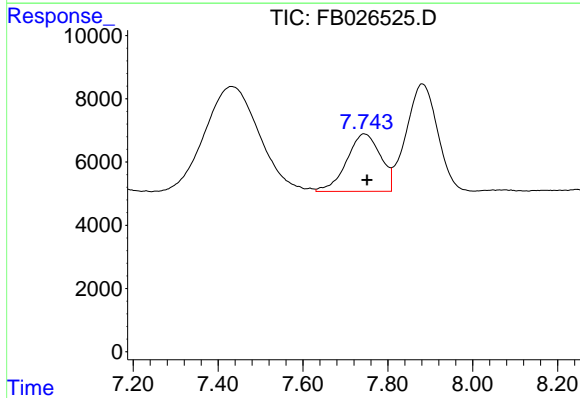


#3 n-Heptane

R.T.: 7.745 min
 Delta R.T.: -0.006 min
 Response: 100729
 Conc: 5.26 ng/ml

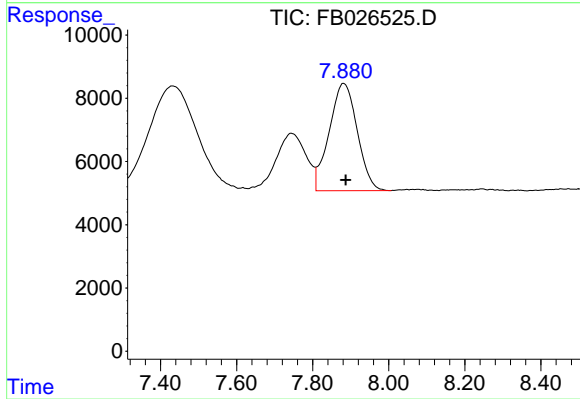

#4 Benzene


R.T.: 7.882 min
 Delta R.T.: -0.005 min
 Response: 173891
 Conc: 7.82 ng/ml

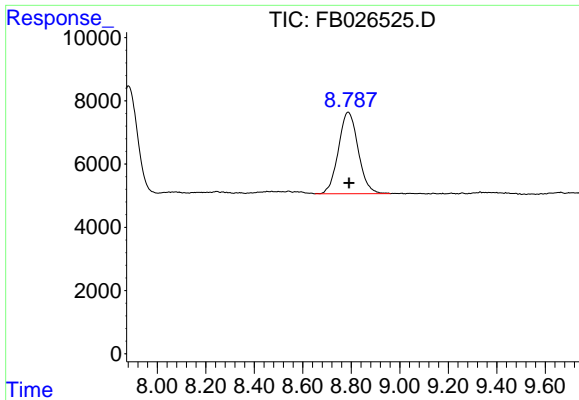

#5 AAA-TFT


R.T.: 8.788 min
 Delta R.T.: -0.004 min
 Response: 146183
 Conc: 13.01 ng/ml

Instrument :
 FID_B
 ClientSampleId :

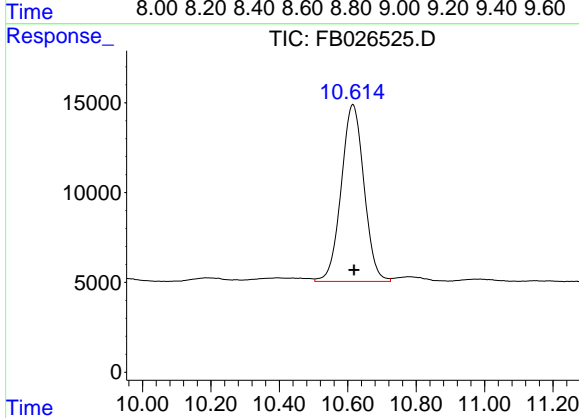


#6 Toluene

R.T.: 10.615 min
 Delta R.T.: -0.003 min
 Response: 454385
 Conc: 21.29 ng/ml

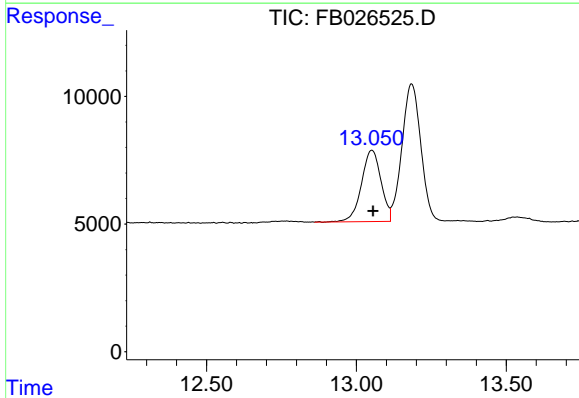


#7 Ethylbenzene

R.T.: 13.052 min
 Delta R.T.: -0.003 min
 Response: 126399
 Conc: 6.40 ng/ml

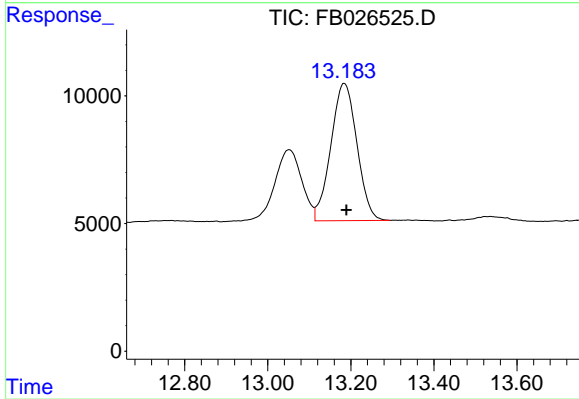


#8 m-Xylene

R.T.: 13.185 min
 Delta R.T.: -0.005 min
 Response: 234495
 Conc: 11.89 ng/ml

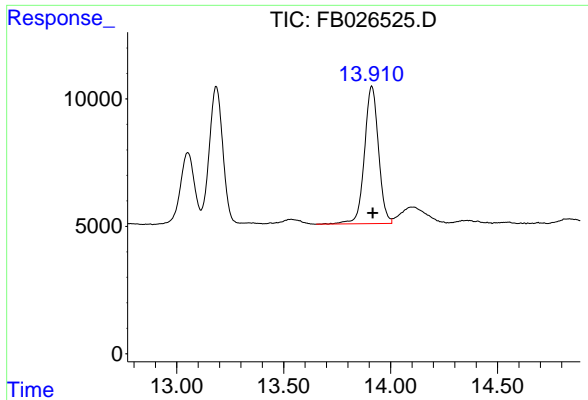

#9 O-Xylene
R.T.: 13.912 min
Delta R.T.: -0.004 min
Response: 245860
Conc: 12.87 ng/ml

Instrument :
FID_B
ClientSampleId :

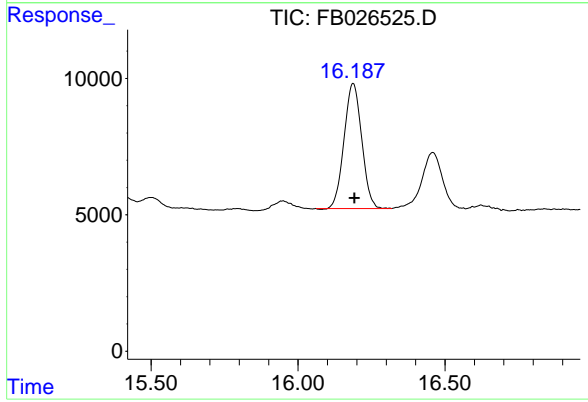

#10 1,2,4-Trimethylbenzene
R.T.: 16.188 min
Delta R.T.: -0.004 min
Response: 190671
Conc: 9.81 ng/ml