

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121521\
 Data File : FB026521.D
 Signal(s) : FID2B.CH
 Acq On : 15 Dec 2021 11:37
 Operator : AJ/MA
 Sample : BSF1215S1
 Misc : 5.01G/5.00ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1215S1

Integration File: Calibration.e
 Quant Time: Dec 15 13:53:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	261058	23.236 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	535915	30.788 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	609770	30.747 ng/ml
3) t n-Heptane	7.745	197330	10.308 ng/ml
4) t Benzene	7.882	230066	10.348 ng/ml
6) t Toluene	10.615	656406	30.762 ng/ml
7) t Ethylbenzene	13.052	206111	10.441 ng/ml
8) t m-Xylene	13.185	408842	20.737 ng/ml
9) t O-Xylene	13.912	397957	20.838 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	398325	20.504 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121521\
Data File : FB026521.D
Signal(s) : FID2B.CH
Acq On : 15 Dec 2021 11:37
Operator : AJ/MA
Sample : BSF1215S1
Misc : 5.01G/5.00ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1215S1

Integration File: Calibration.e
Quant Time: Dec 15 13:53:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

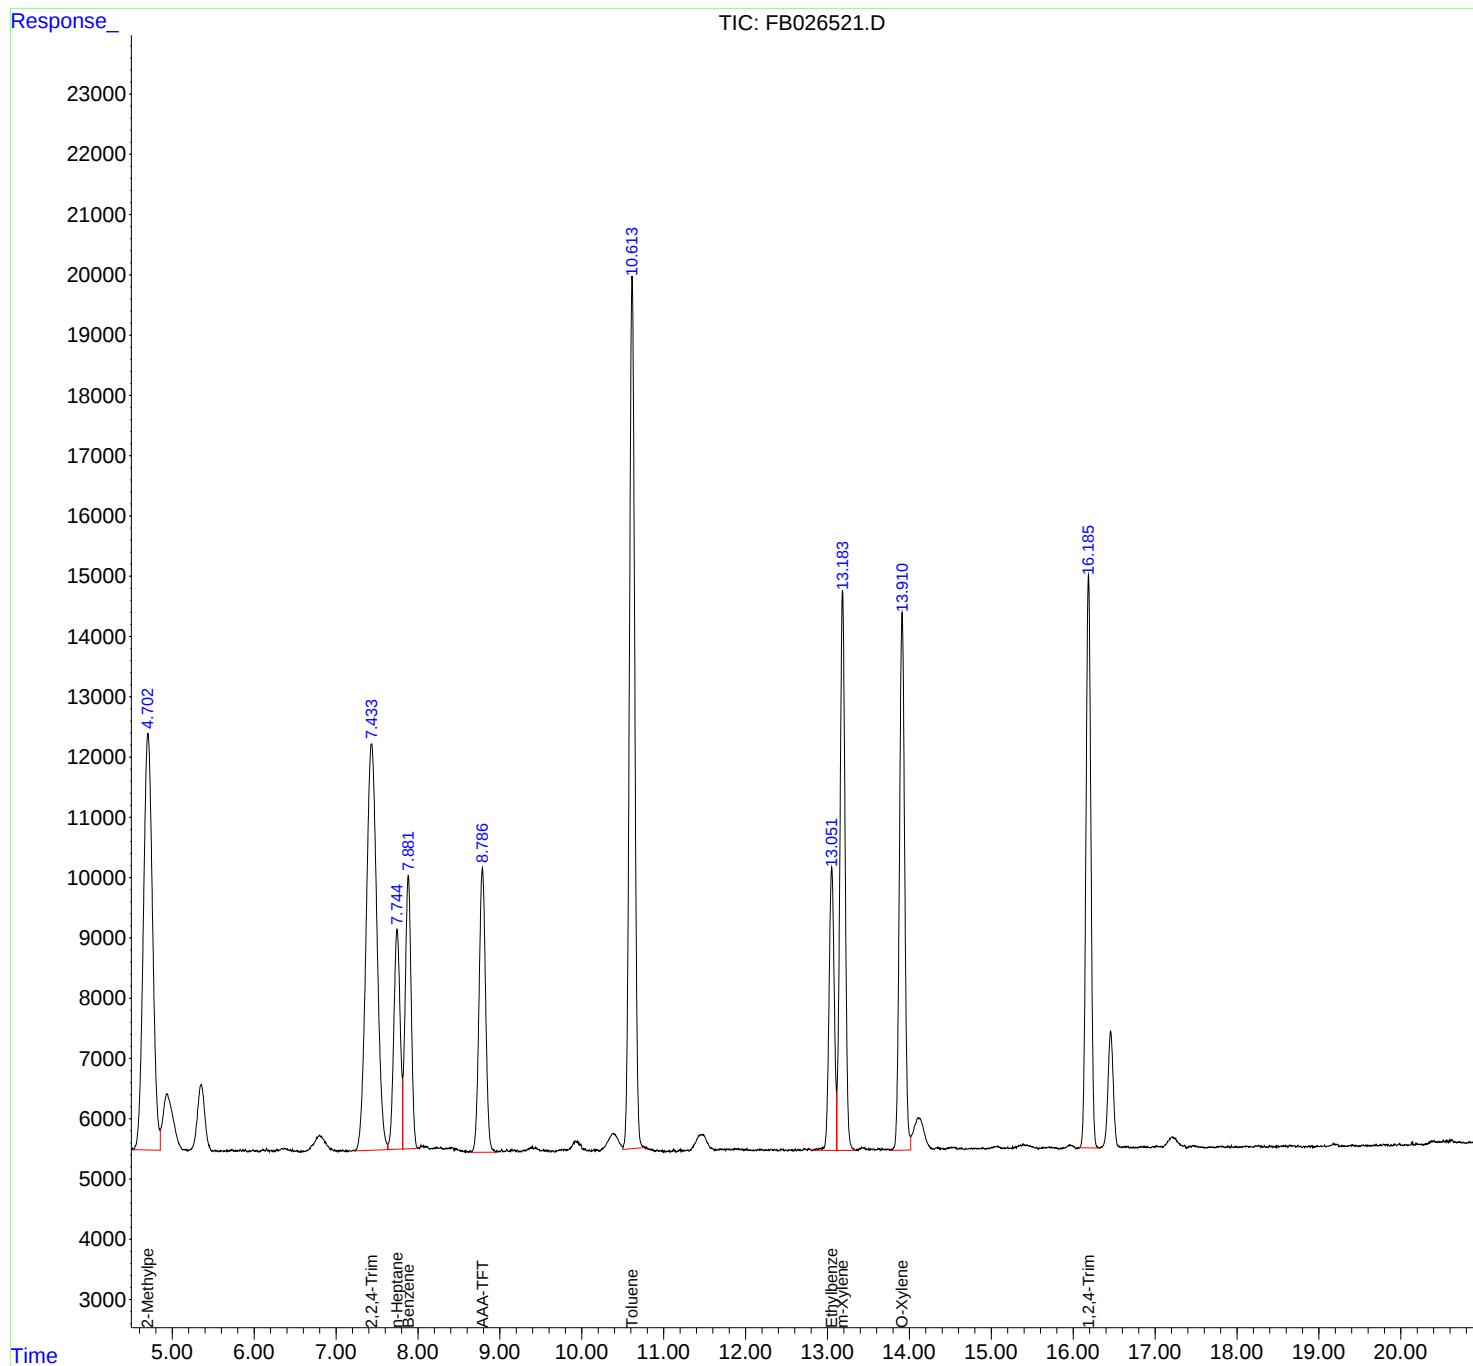


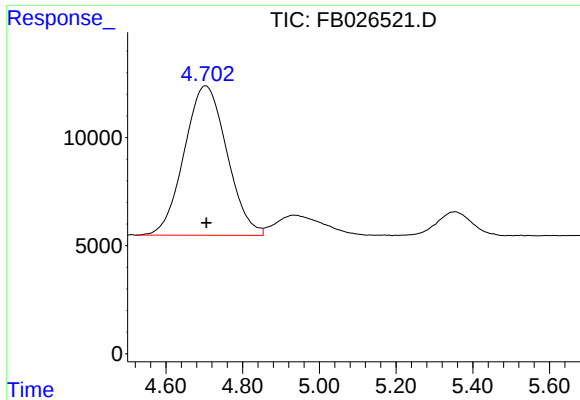

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.003 min
Response: 535915
Conc: 30.79 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1215S1

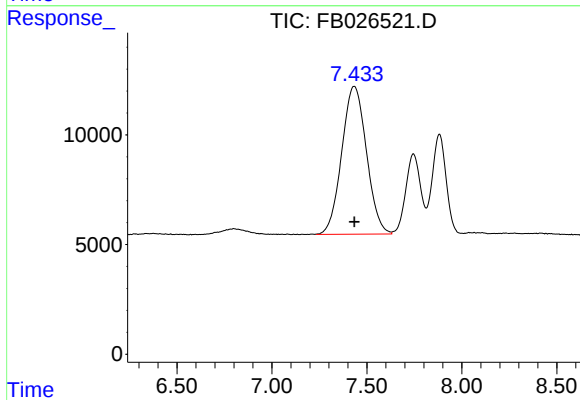


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.000 min
Response: 609770
Conc: 30.75 ng/ml

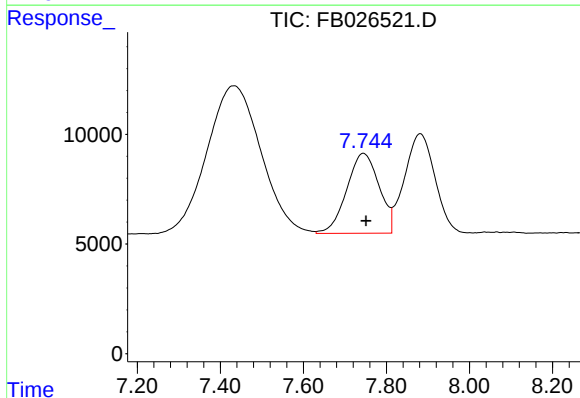


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.006 min
Response: 197330
Conc: 10.31 ng/ml

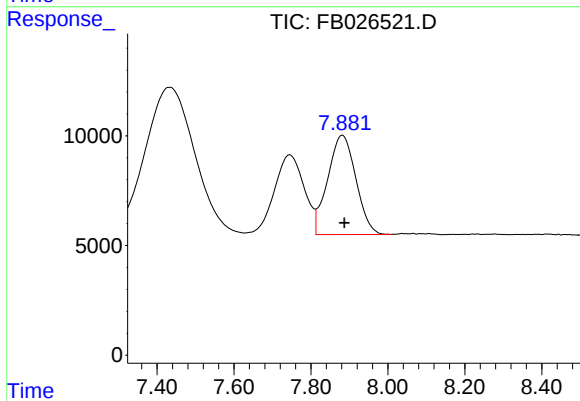

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.005 min
Response: 230066
Conc: 10.35 ng/ml

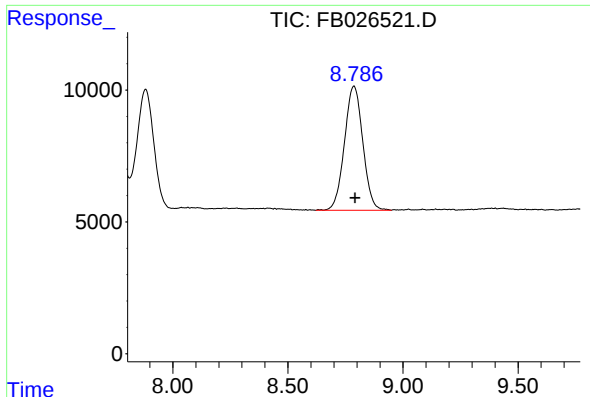

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.004 min
Response: 261058
Conc: 23.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1215S1

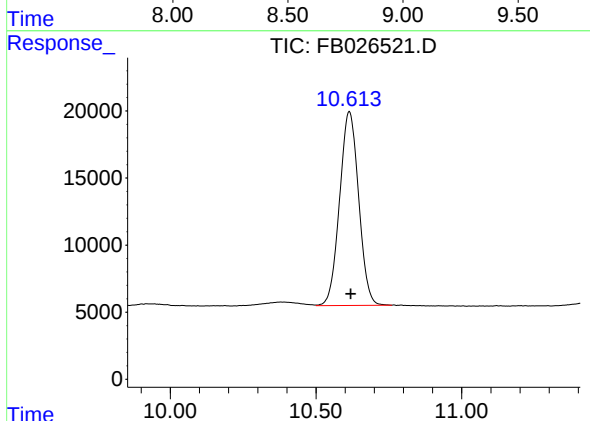


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.004 min
Response: 656406
Conc: 30.76 ng/ml

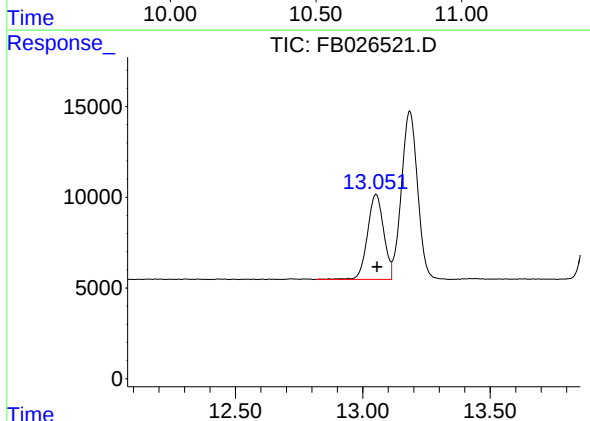


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.003 min
Response: 206111
Conc: 10.44 ng/ml

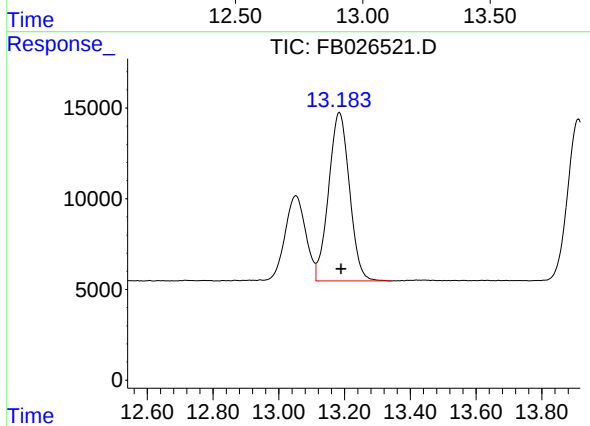

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.005 min
Response: 408842
Conc: 20.74 ng/ml

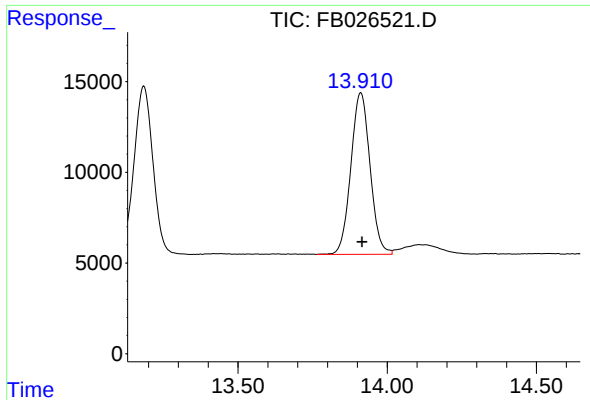

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.004 min
Response: 397957
Conc: 20.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1215S1

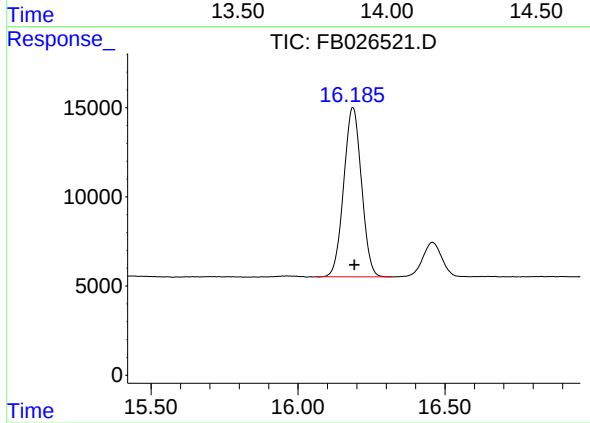

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.005 min
Response: 398325
Conc: 20.50 ng/ml