

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121521\
 Data File : FB026524.D
 Signal(s) : FID2B.CH
 Acq On : 15 Dec 2021 14:00
 Operator : AJ/MA
 Sample : M5065-01MS
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 UV-1WCMS

Integration File: Calibration.e
 Quant Time: Dec 16 00:18:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	176747	15.732 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	191320	10.991 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	155224	7.827 ng/ml
3) t n-Heptane	7.748	59449	3.106 ng/ml
4) t Benzene	7.884	168420	7.575 ng/ml
6) t Toluene	10.616	422183	19.785 ng/ml
7) t Ethylbenzene	13.052	125734	6.369 ng/ml
8) t m-Xylene	13.185	227861	11.557 ng/ml
9) t O-Xylene	13.913	235569	12.335 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	178192	9.172 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121521\
Data File : FB026524.D
Signal(s) : FID2B.CH
Acq On : 15 Dec 2021 14:00
Operator : AJ/MA
Sample : M5065-01MS
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
UV-1WCMS

Integration File: Calibration.e
Quant Time: Dec 16 00:18:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

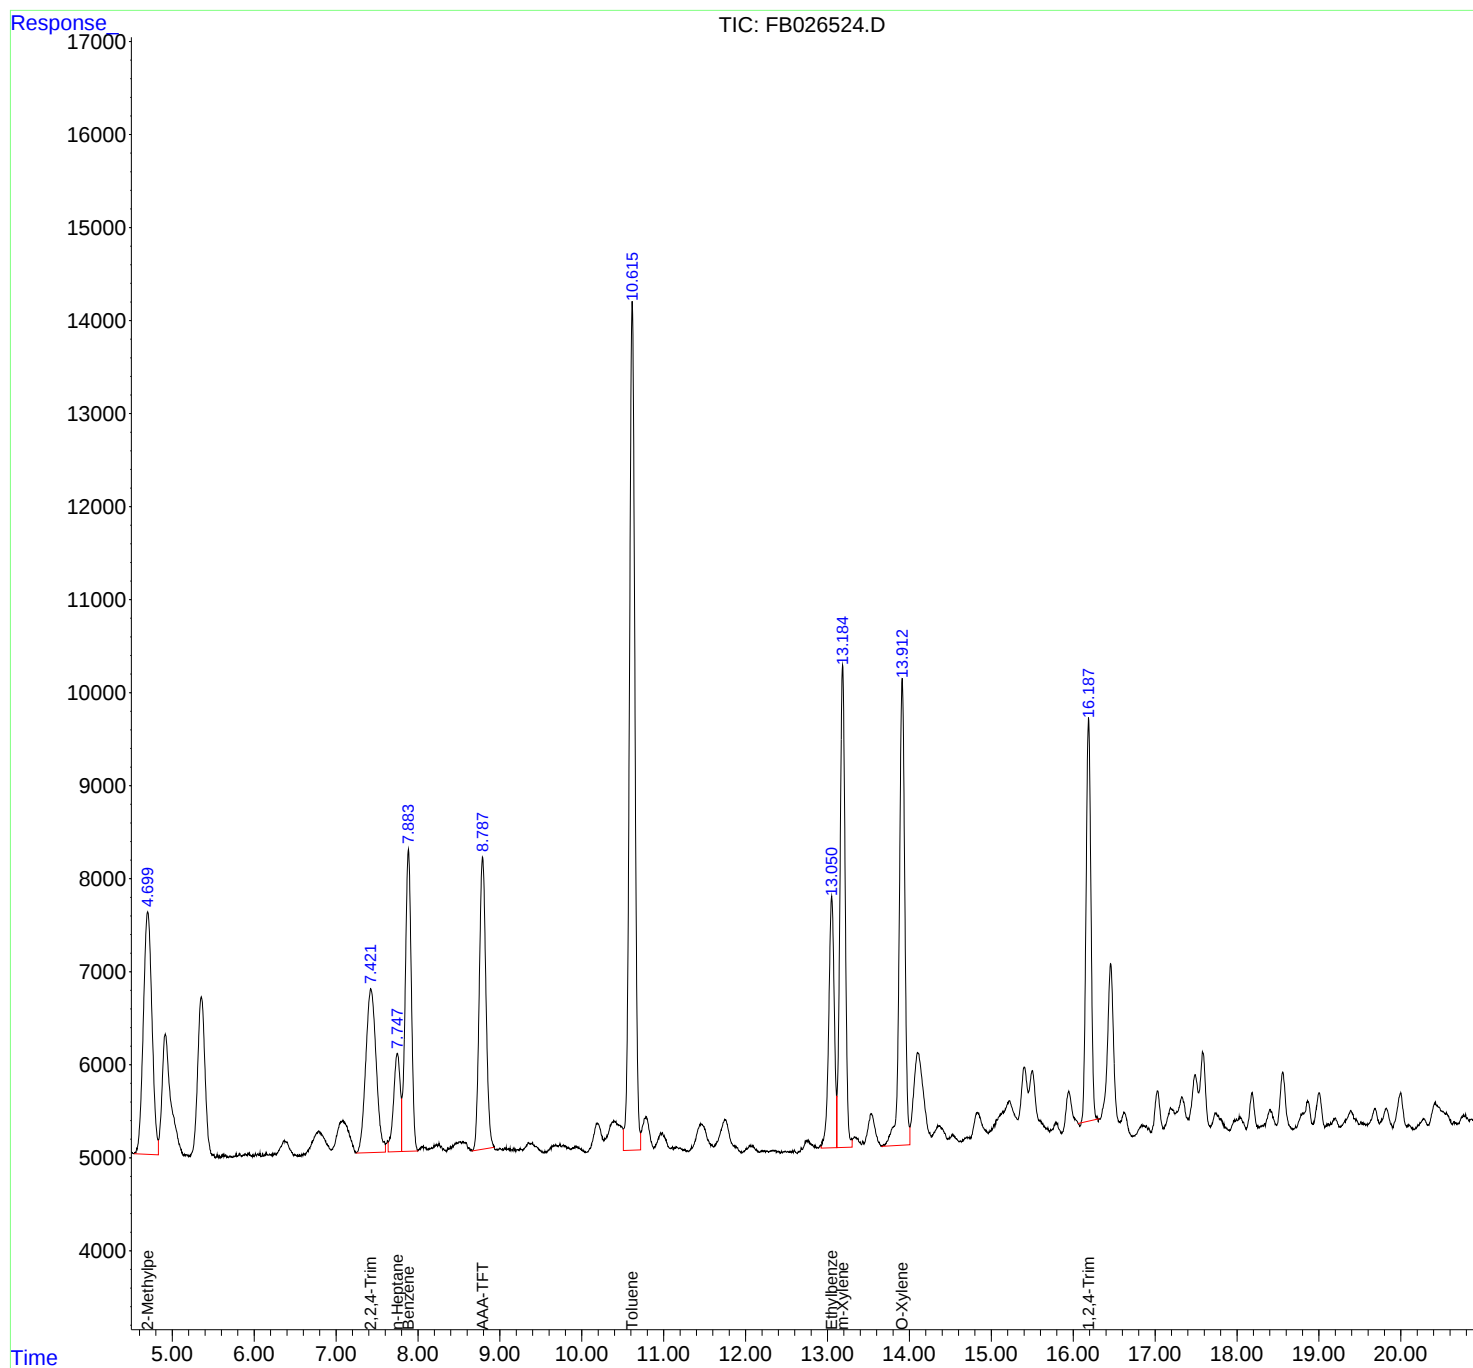


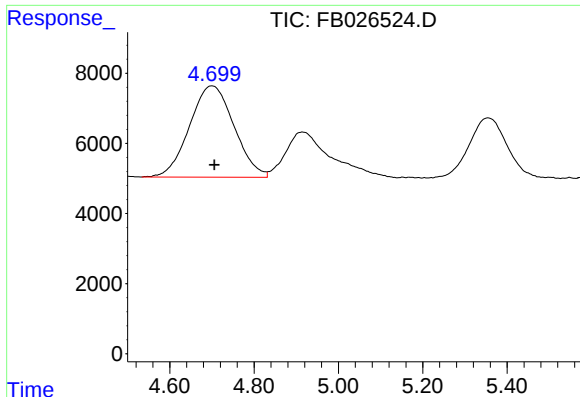

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.005 min
Response: 191320
Conc: 10.99 ng/ml

Instrument :
FID_B
ClientSampleId :
UV-1WCMS

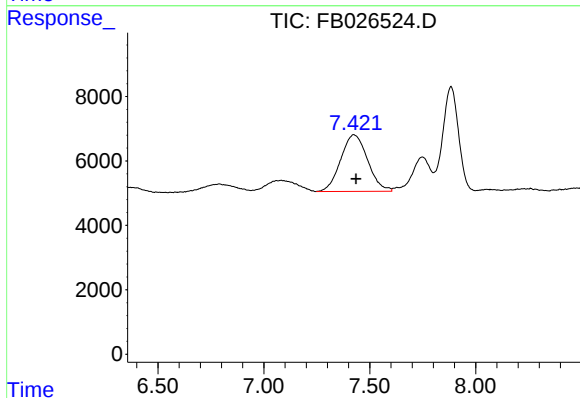


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.012 min
Response: 155224
Conc: 7.83 ng/ml

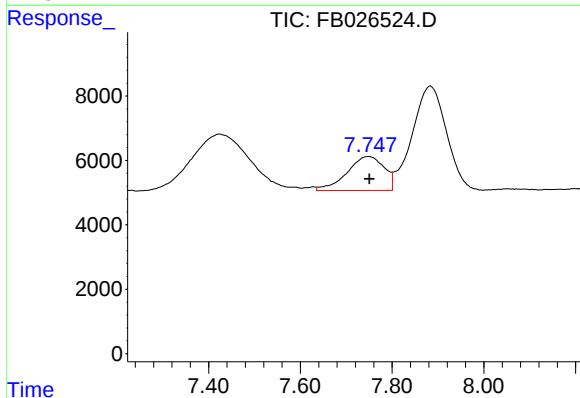


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 59449
Conc: 3.11 ng/ml

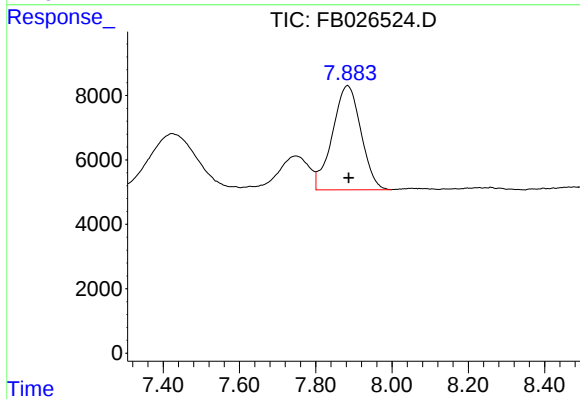

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.003 min
Response: 168420
Conc: 7.57 ng/ml

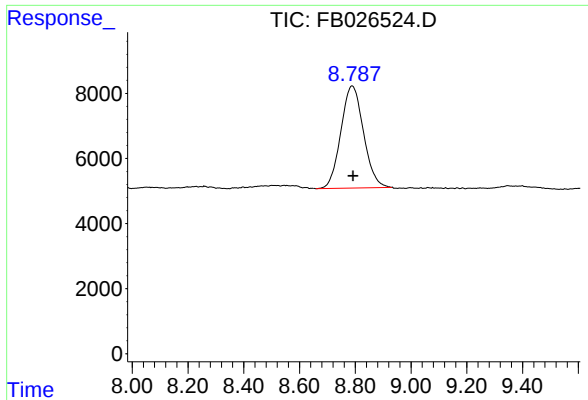

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 176747
Conc: 15.73 ng/ml

Instrument :
FID_B
ClientSampleId :
UV-1WCMS

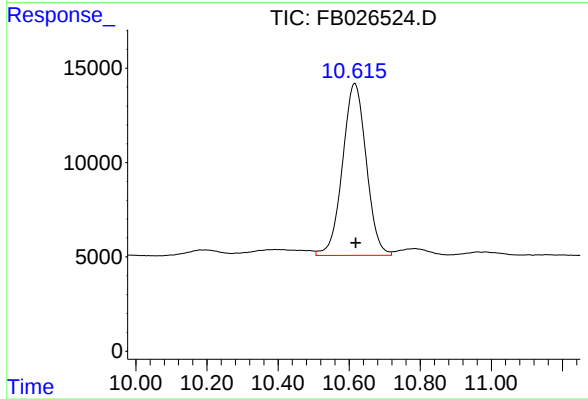


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.003 min
Response: 422183
Conc: 19.79 ng/ml

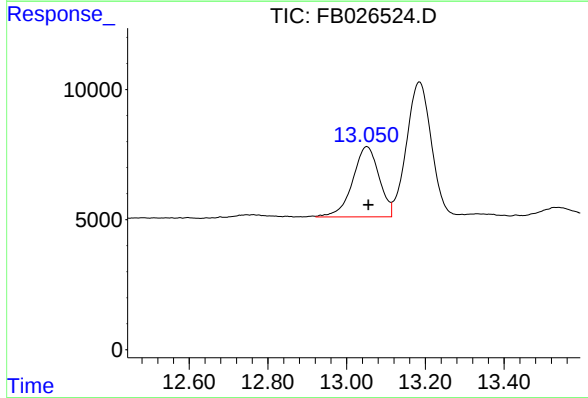


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.004 min
Response: 125734
Conc: 6.37 ng/ml

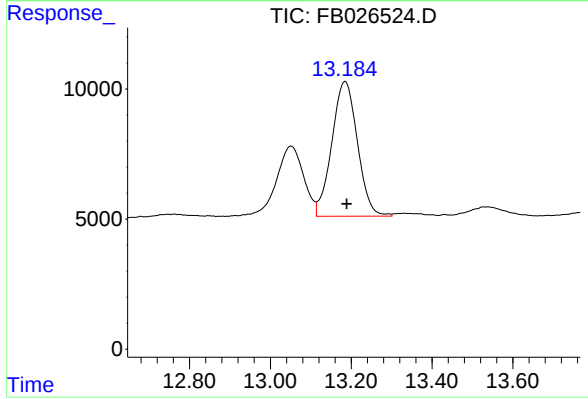

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.004 min
Response: 227861
Conc: 11.56 ng/ml

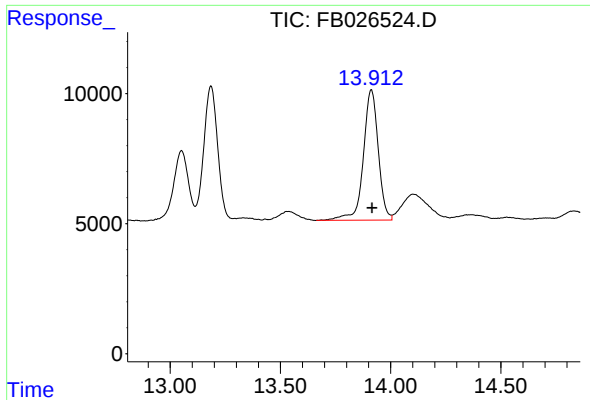

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.004 min
Response: 235569
Conc: 12.34 ng/ml

Instrument :
FID_B
ClientSampleId :
UV-1WCMS

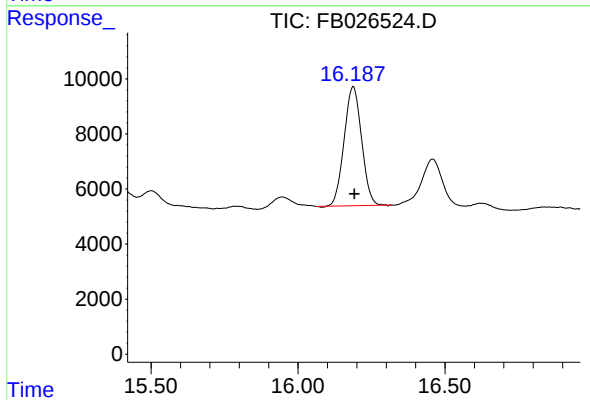

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.004 min
Response: 178192
Conc: 9.17 ng/ml