

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121619\
 Data File : FB023223.D
 Signal(s) : FID2B.CH
 Acq On : 16 Dec 2019 9:28
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 16 15:14:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	494054	20.113 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	930873	28.486 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	1031500	29.581 ng/ml
3) t n-Heptane	7.750	338464	9.844 ng/ml
4) t Benzene	7.884	417234	10.014 ng/ml
6) t Toluene	10.622	1193030	29.616 ng/ml
7) t Ethylbenzene	13.062	373766	9.686 ng/ml
8) t m-Xylene	13.195	709551	19.499 ng/ml
9) t O-Xylene	13.923	688006	19.815 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	570661	20.349 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121619\
Data File : FB023223.D
Signal(s) : FID2B.CH
Acq On : 16 Dec 2019 9:28
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 16 15:14:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

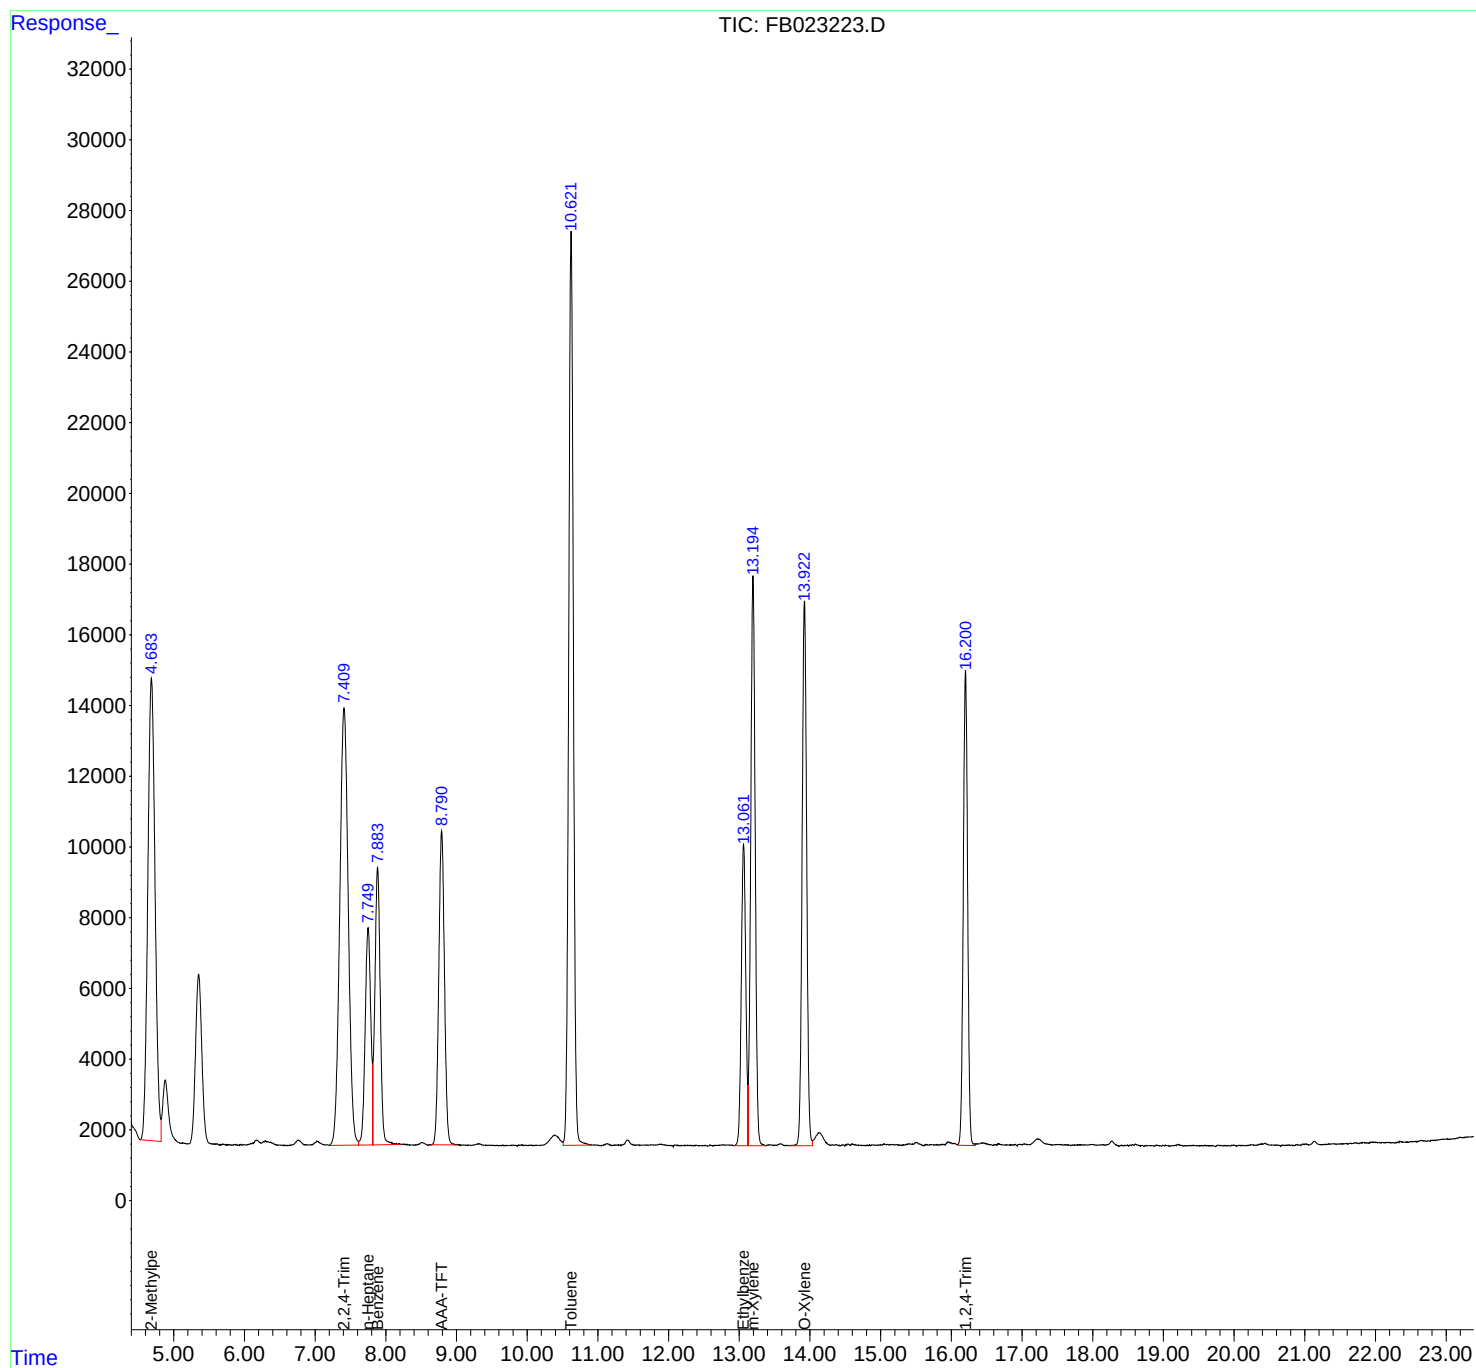

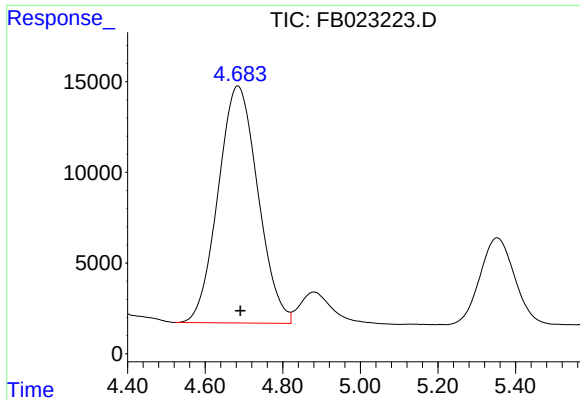


#1 2-Methylpentane

R.T.: 4.684 min

Delta R.T.: -0.007 min

Response: 930873

Conc: 28.49 ng/ml

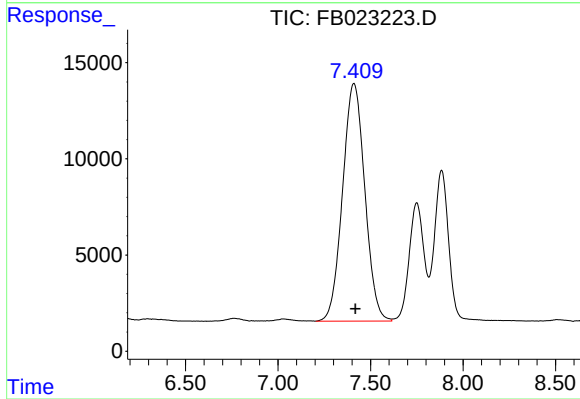


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min

Delta R.T.: -0.007 min

Response: 1031500

Conc: 29.58 ng/ml

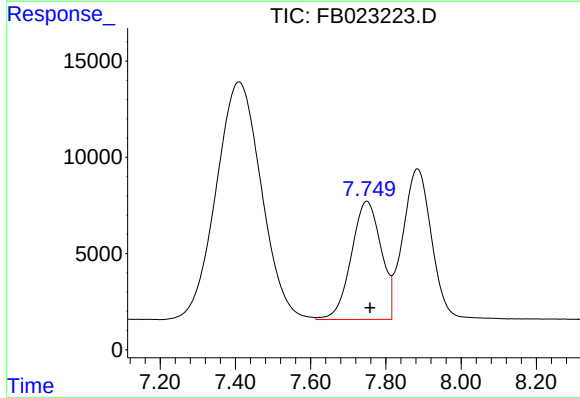


#3 n-Heptane

R.T.: 7.750 min

Delta R.T.: -0.008 min

Response: 338464

Conc: 9.84 ng/ml

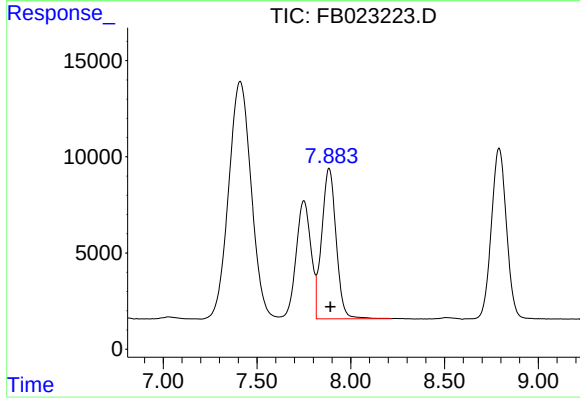


#4 Benzene

R.T.: 7.884 min

Delta R.T.: -0.008 min


Response: 417234

Conc: 10.01 ng/ml

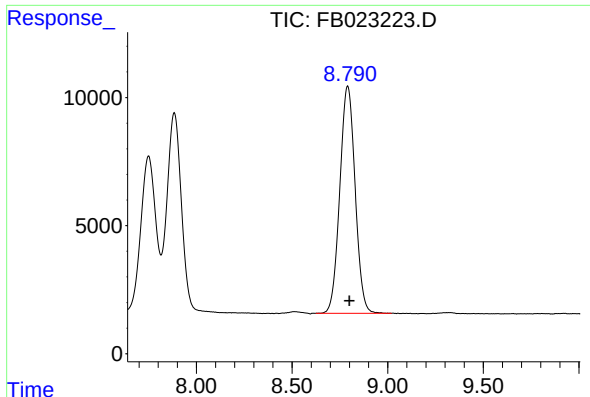


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.008 min
Response: 494054
Conc: 20.11 ng/ml

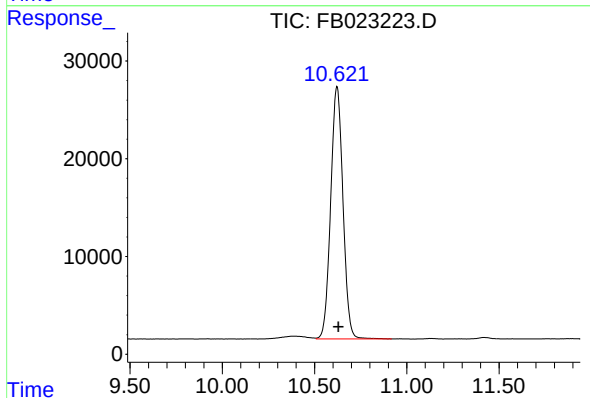


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.008 min
Response: 1193030
Conc: 29.62 ng/ml

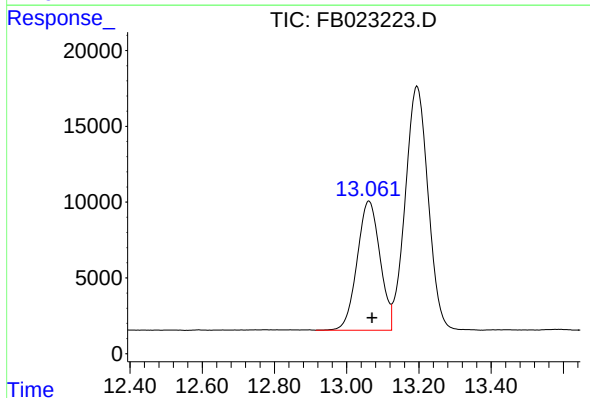


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.008 min
Response: 373766
Conc: 9.69 ng/ml

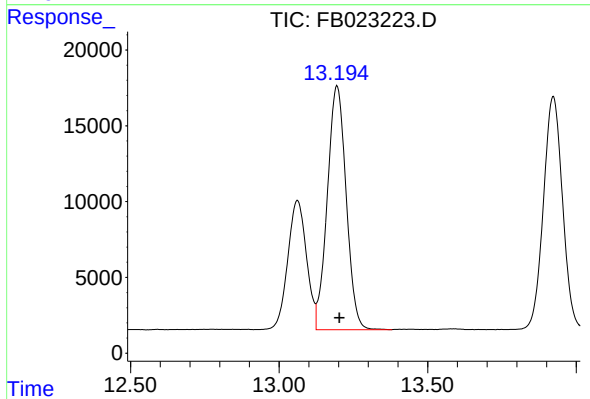


#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: -0.008 min
Response: 709551
Conc: 19.50 ng/ml

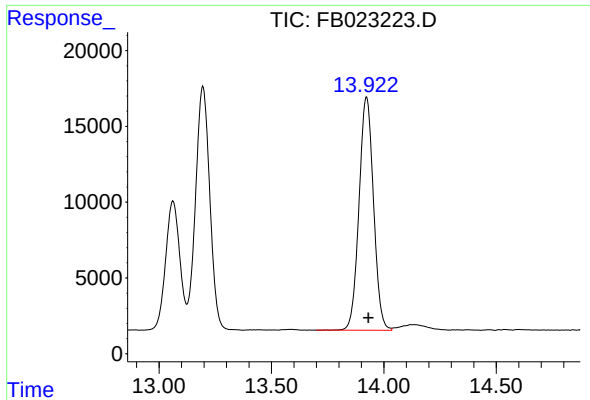

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.009 min
Response: 688006
Conc: 19.82 ng/ml

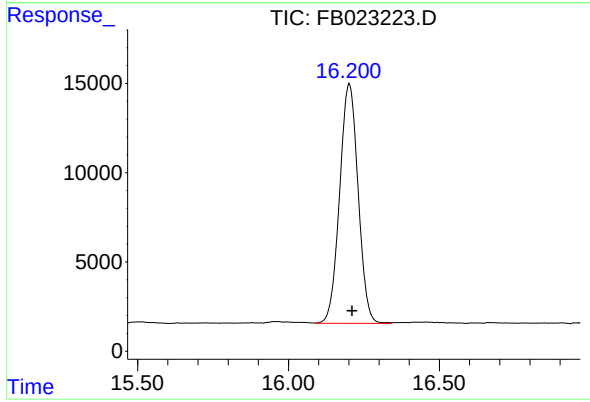

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: -0.009 min
Response: 570661
Conc: 20.35 ng/ml