

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121619\
 Data File : FB023225.D
 Signal(s) : FID2B.CH
 Acq On : 16 Dec 2019 10:38
 Operator : DD/AJ
 Sample : BSF1216S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 16 15:14:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	451084	18.364 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	827995	25.338 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	921526	26.427 ng/ml
3) t n-Heptane	7.754	298247	8.674 ng/ml
4) t Benzene	7.888	357122	8.571 ng/ml
6) t Toluene	10.625	1052209	26.120 ng/ml
7) t Ethylbenzene	13.065	328387	8.510 ng/ml
8) t m-Xylene	13.198	623022	17.121 ng/ml
9) t O-Xylene	13.926	602117	17.342 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	498097	17.762 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121619\
Data File : FB023225.D
Signal(s) : FID2B.CH
Acq On : 16 Dec 2019 10:38
Operator : DD/AJ
Sample : BSF1216S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 16 15:14:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

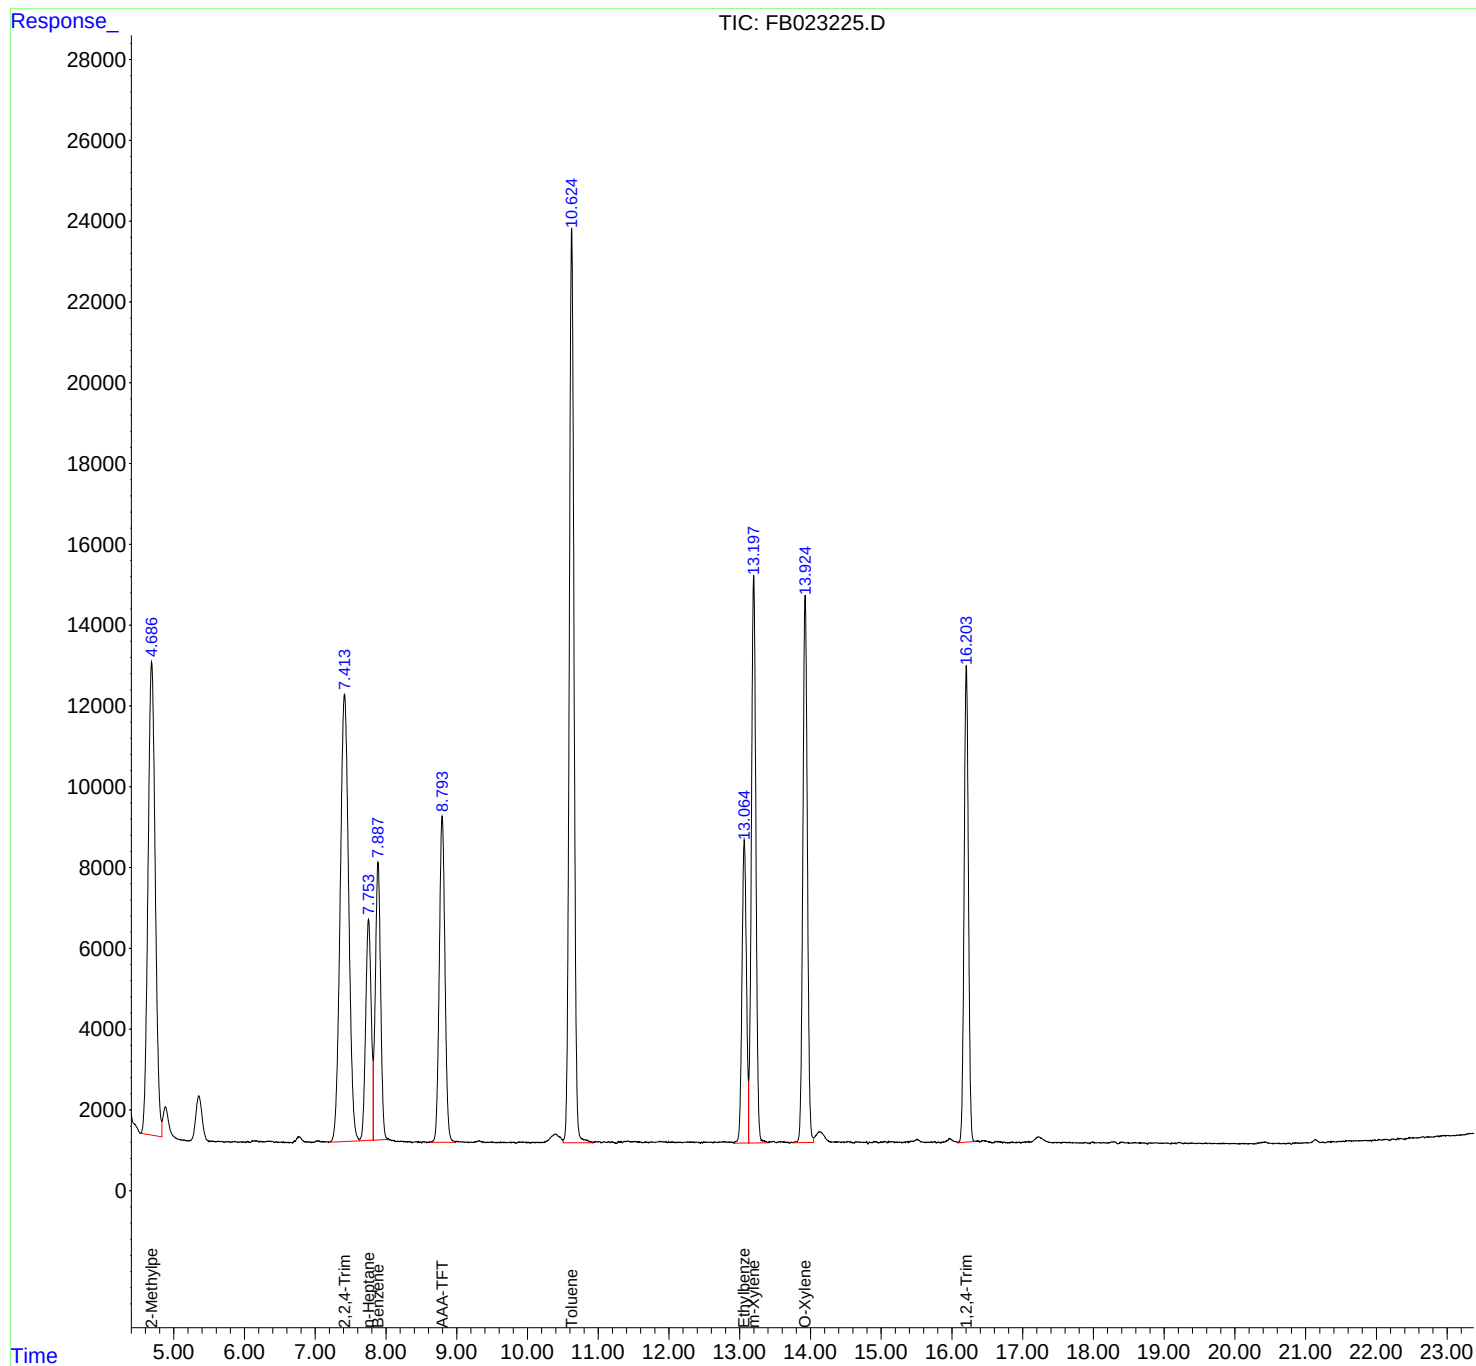

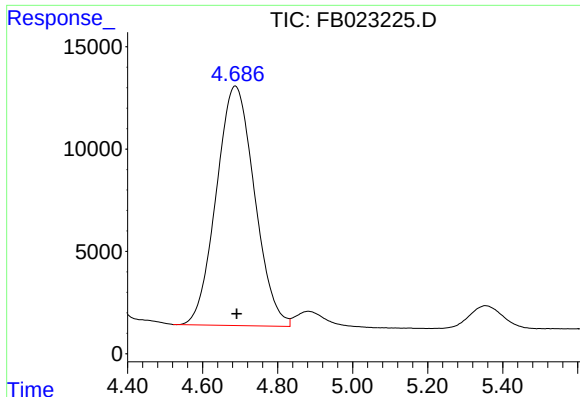


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 827995
Conc: 25.34 ng/ml

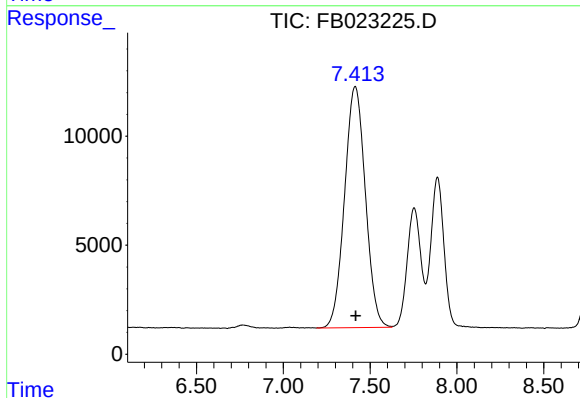


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 921526
Conc: 26.43 ng/ml

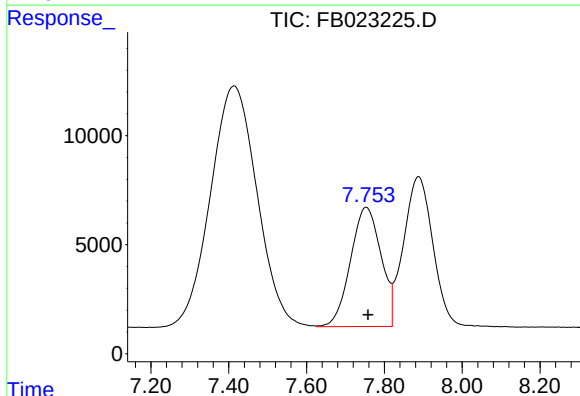


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 298247
Conc: 8.67 ng/ml

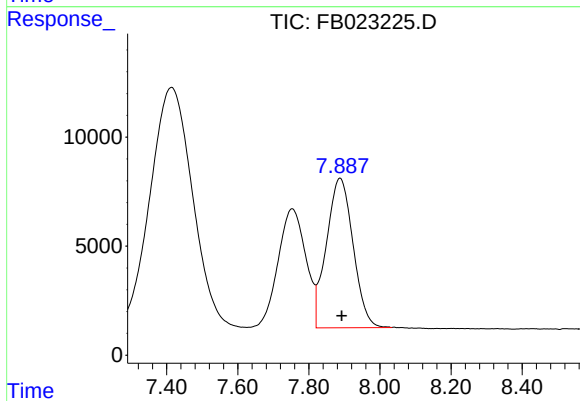


#4 Benzene

R.T.: 7.888 min
Delta R.T.: -0.004 min
Response: 357122
Conc: 8.57 ng/ml

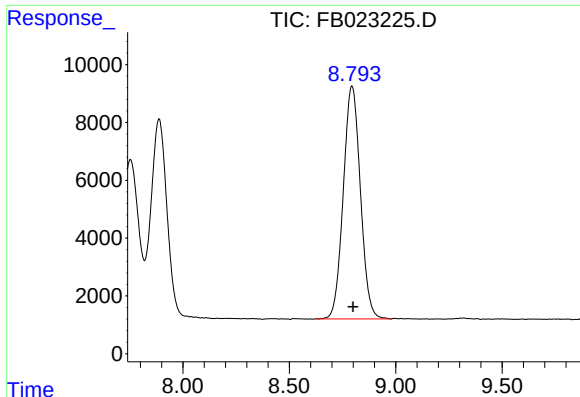


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: -0.005 min
Response: 451084
Conc: 18.36 ng/ml

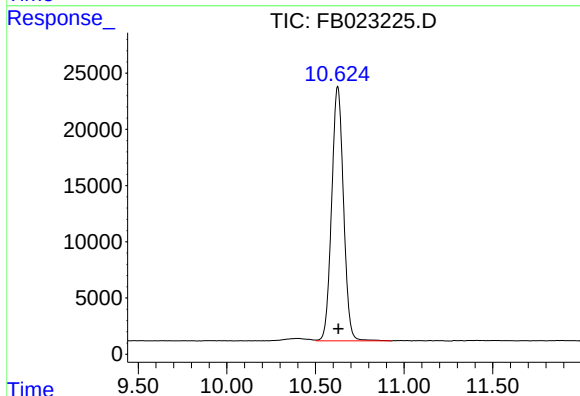


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.005 min
Response: 1052209
Conc: 26.12 ng/ml

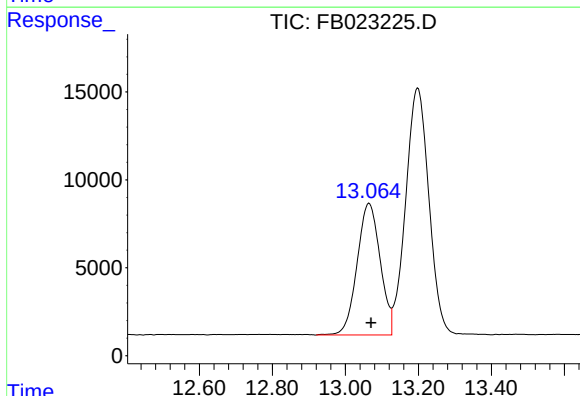


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.005 min
Response: 328387
Conc: 8.51 ng/ml

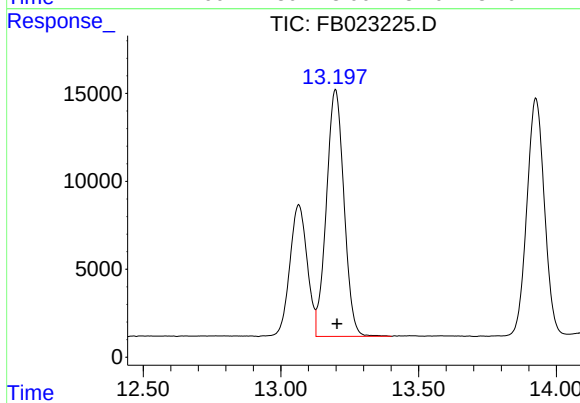


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: -0.005 min
Response: 623022
Conc: 17.12 ng/ml

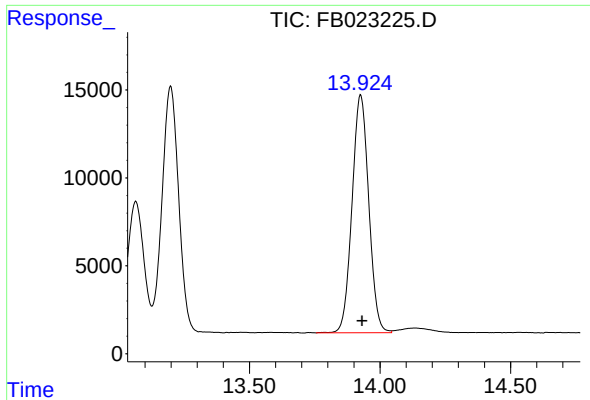

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.005 min
Response: 602117
Conc: 17.34 ng/ml

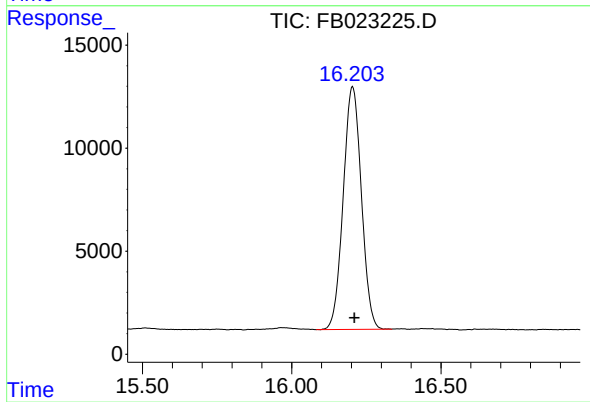

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: -0.006 min
Response: 498097
Conc: 17.76 ng/ml