

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121624\
 Data File : FB031290.D
 Signal(s) : FID2B.CH
 Acq On : 16 Dec 2024 13:31
 Operator : YP/AJ
 Sample : FB121624GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB121624GROICV

Integration File: Calibration.e
 Quant Time: Dec 16 12:22:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121624.M
 Quant Title :
 QLast Update : Mon Dec 16 11:52:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	553269	20.971 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.716	1015172	31.932 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	1215610	31.512 ng/ml
3) t n-Heptane	7.749	345142	9.859 ng/ml
4) t Benzene	7.887	454885	10.323 ng/ml
6) t Toluene	10.616	1285001	30.826 ng/ml
7) t Ethylbenzene	13.052	385355	10.451 ng/ml
8) t m-Xylene	13.186	832695	20.887 ng/ml
9) t O-Xylene	13.914	784345	21.345 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	647425	21.701 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121624\
Data File : FB031290.D
Signal(s) : FID2B.CH
Acq On : 16 Dec 2024 13:31
Operator : YP/AJ
Sample : FB121624GROICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB121624GROICV

Integration File: Calibration.e
Quant Time: Dec 16 12:22:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121624.M
Quant Title :
QLast Update : Mon Dec 16 11:52:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

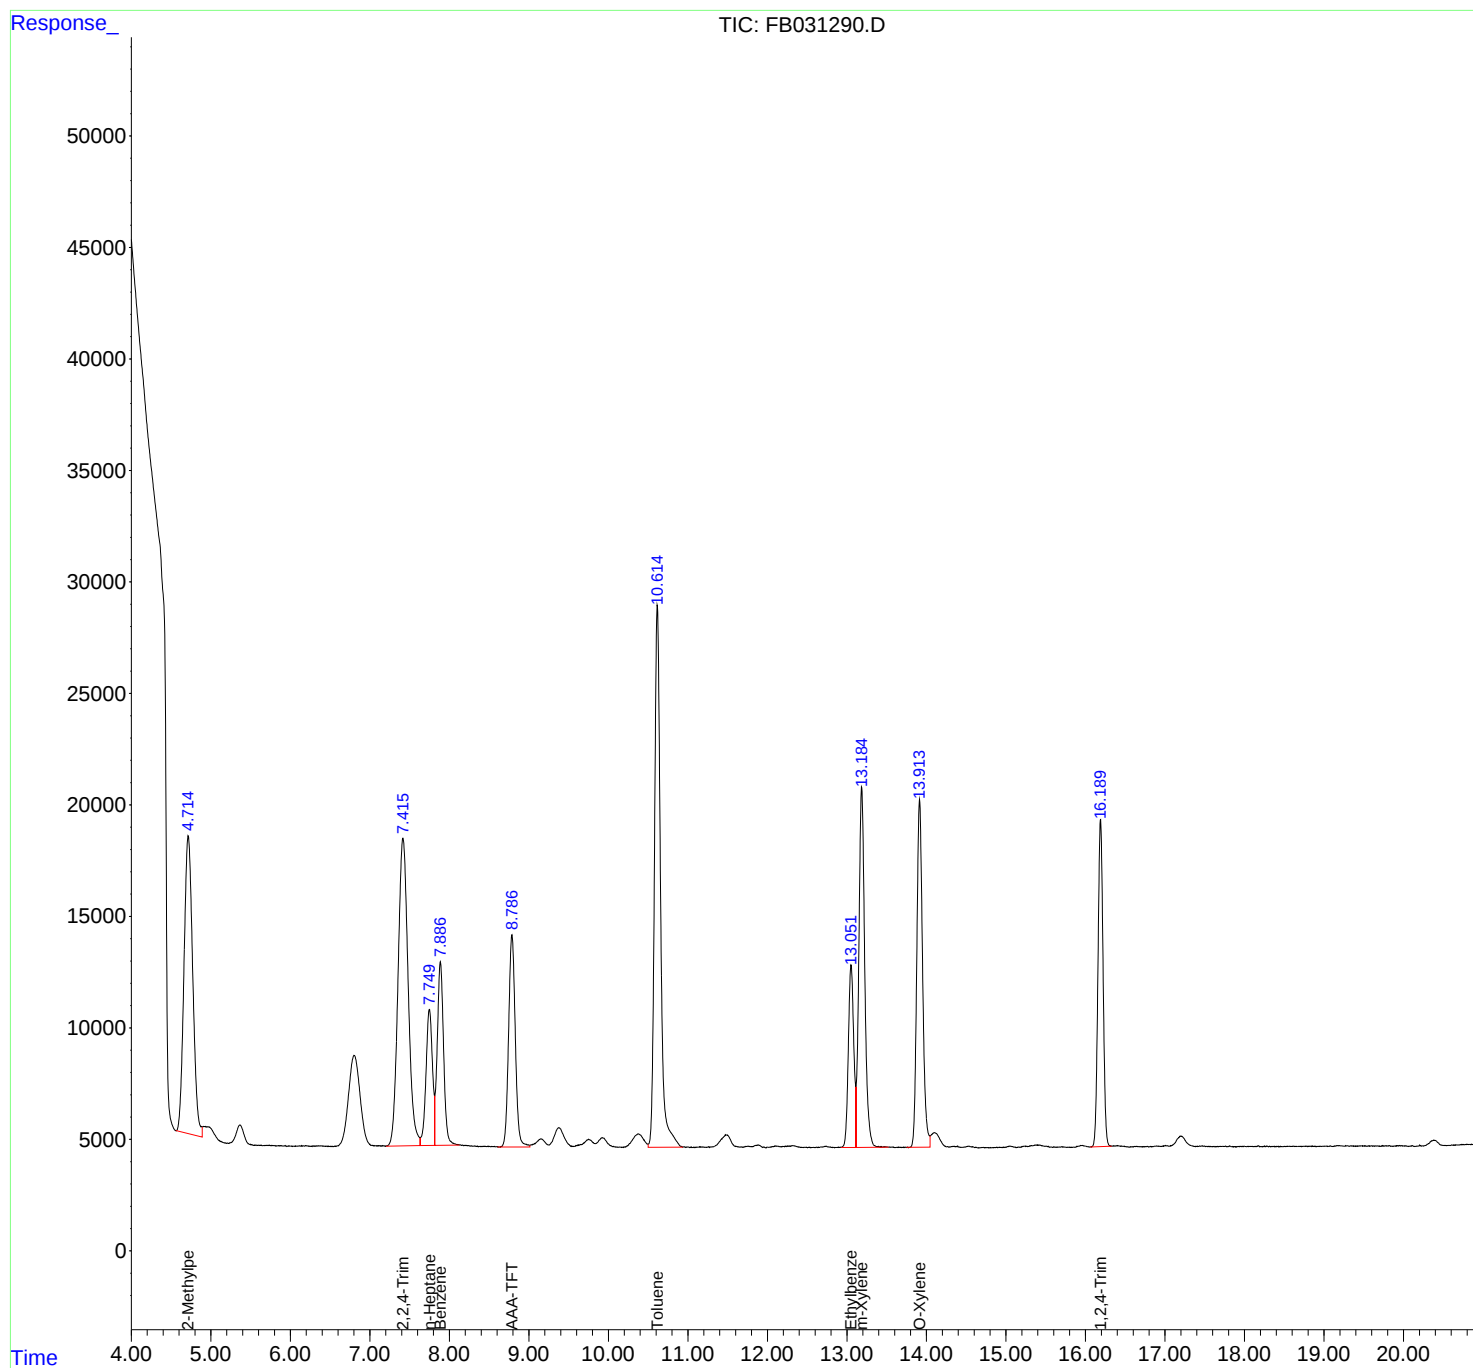


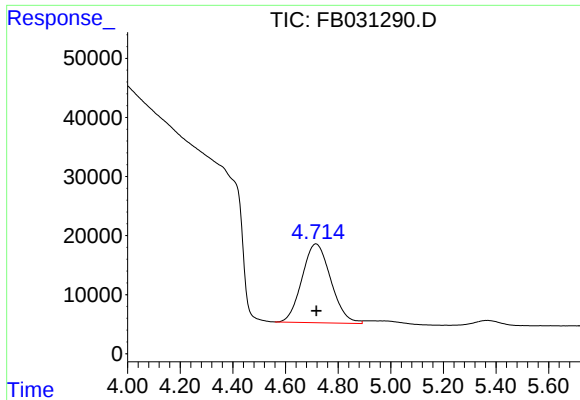

#1 2-Methylpentane


R.T.: 4.716 min
Delta R.T.: -0.001 min
Response: 1015172
Conc: 31.93 ng/ml

Instrument :
FID_B
ClientSampleId :
FB121624GROICV

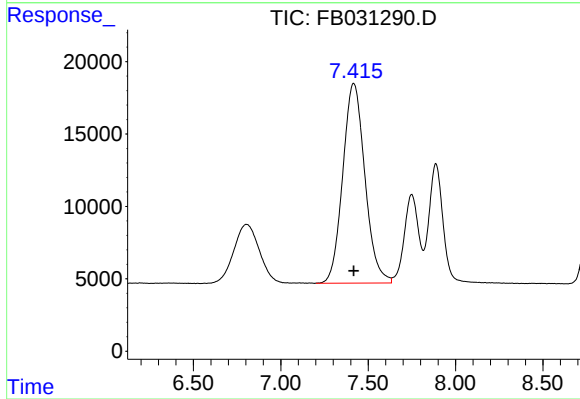


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.002 min
Response: 1215610
Conc: 31.51 ng/ml

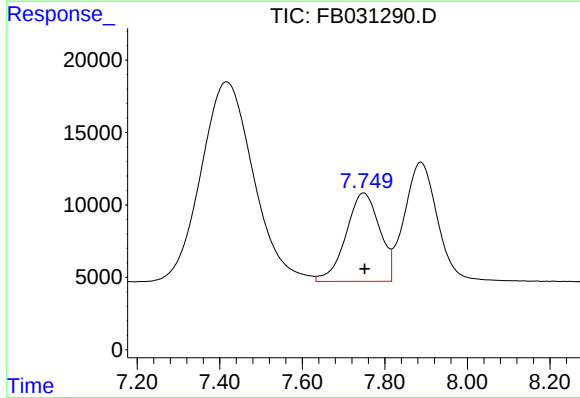


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.001 min
Response: 345142
Conc: 9.86 ng/ml

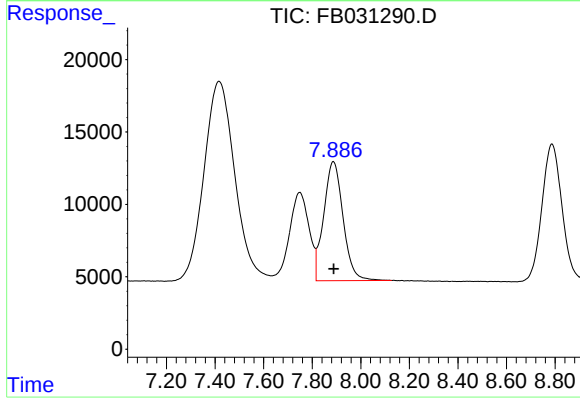

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.001 min
Response: 454885
Conc: 10.32 ng/ml

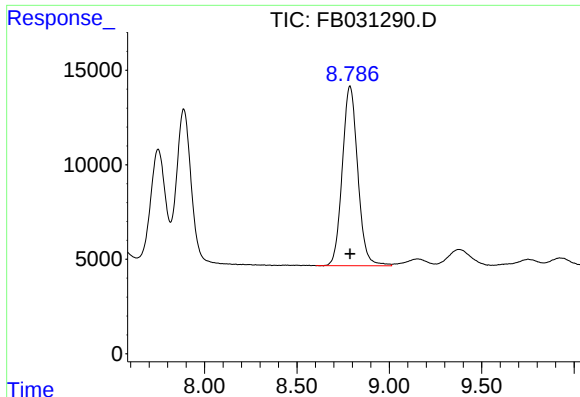

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.001 min
Response: 553269
Conc: 20.97 ng/ml

Instrument :
FID_B
ClientSampleId :
FB121624GROICV

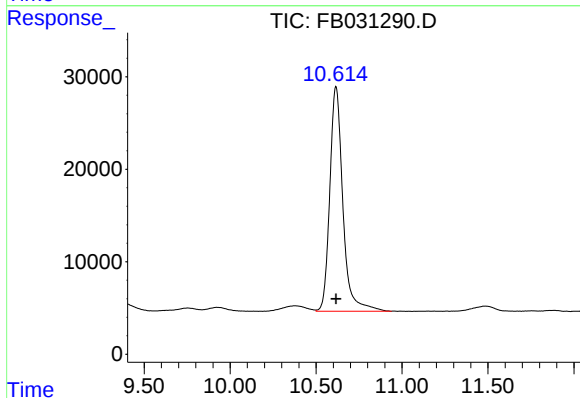


#6 Toluene

R.T.: 10.616 min
Delta R.T.: 0.000 min
Response: 1285001
Conc: 30.83 ng/ml

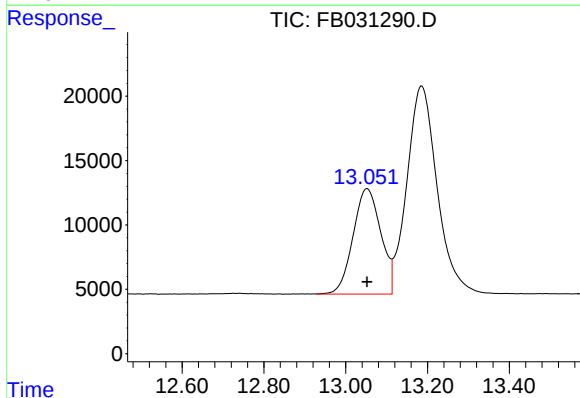


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: 0.000 min
Response: 385355
Conc: 10.45 ng/ml

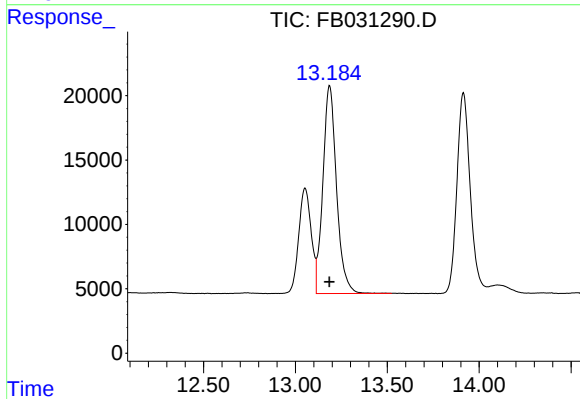

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: 0.000 min
Response: 832695
Conc: 20.89 ng/ml

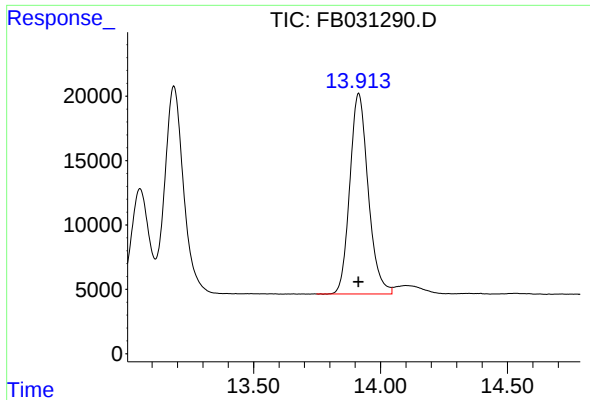

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.000 min
Response: 784345
Conc: 21.34 ng/ml

Instrument :
FID_B
ClientSampleId :
FB121624GROICV

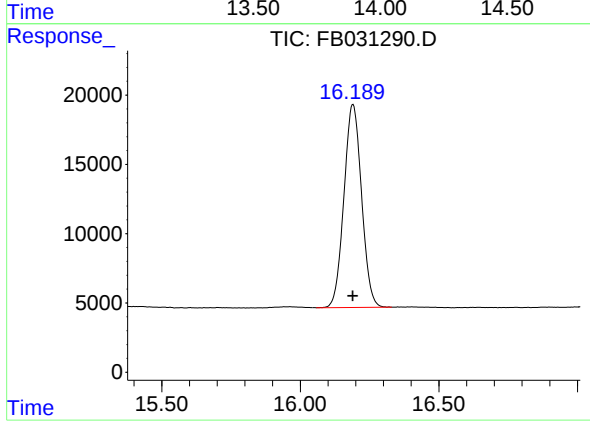

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.000 min
Response: 647425
Conc: 21.70 ng/ml