

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121719\
 Data File : FB023250.D
 Signal(s) : FID2B.CH
 Acq On : 17 Dec 2019 9:00
 Operator : DD/AJ
 Sample : VBF1217S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 VBF1217S1

Integration File: Calibration.e
 Quant Time: Dec 18 00:56:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	459176	18.693 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.412	2179	0.062 ng/ml
6) t Toluene	10.611	2251	0.056 ng/ml
8) t m-Xylene	13.203	683	0.019 ng/ml
9) t O-Xylene	13.936	1881	0.054 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	2800	0.100 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121719\
Data File : FB023250.D
Signal(s) : FID2B.CH
Acq On : 17 Dec 2019 9:00
Operator : DD/AJ
Sample : VBF1217S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1217S1

Integration File: Calibration.e
Quant Time: Dec 18 00:56:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

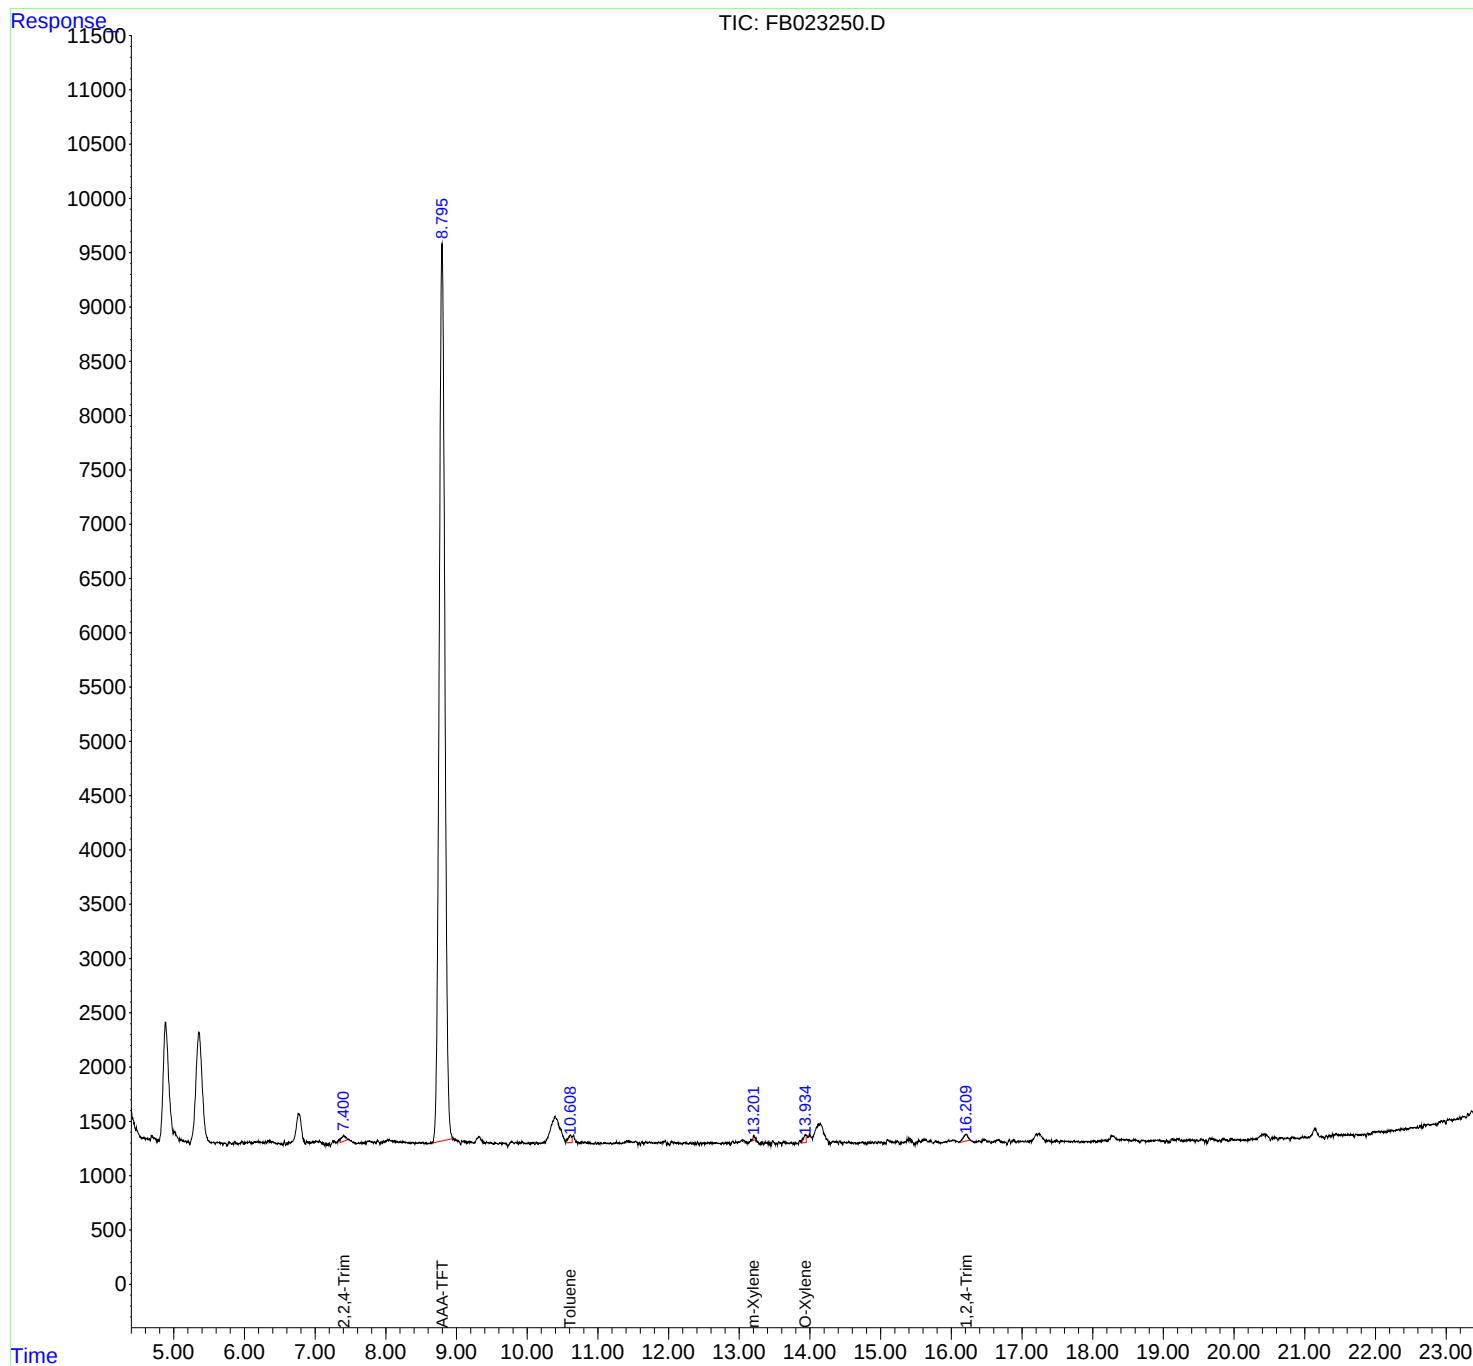


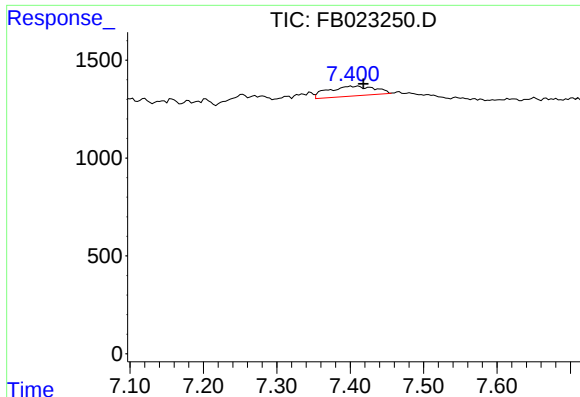

#2 2,2,4-Trimethylpentane


R.T.: 7.412 min
Delta R.T.: -0.007 min
Response: 2179
Conc: 0.06 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1217S1

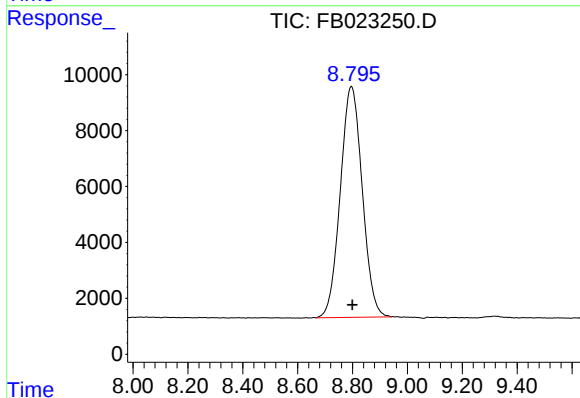


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.003 min
Response: 459176
Conc: 18.69 ng/ml

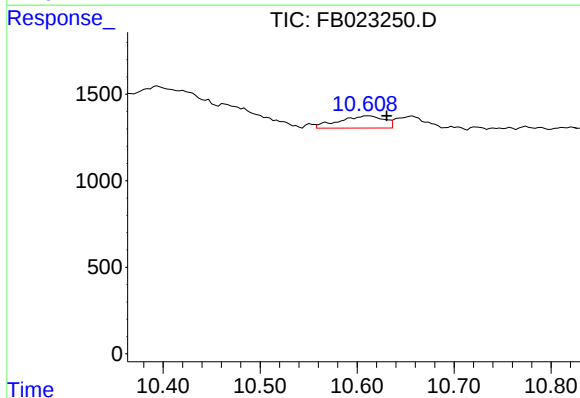


#6 Toluene

R.T.: 10.611 min
Delta R.T.: -0.019 min
Response: 2251
Conc: 0.06 ng/ml

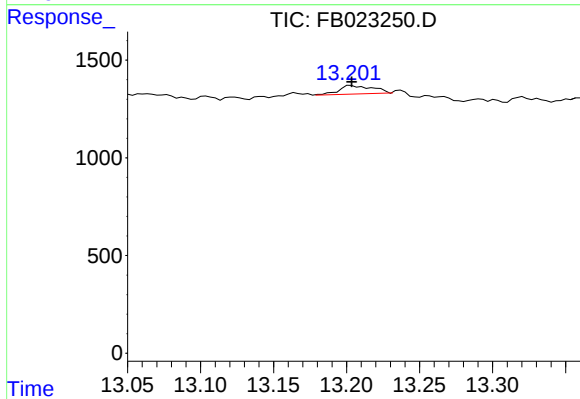

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 683
Conc: 0.02 ng/ml

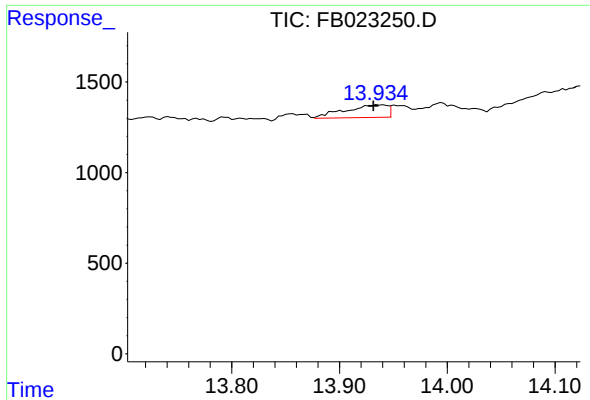

#9 O-Xylene

R.T.: 13.936 min
Delta R.T.: 0.004 min
Response: 1881
Conc: 0.05 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1217S1

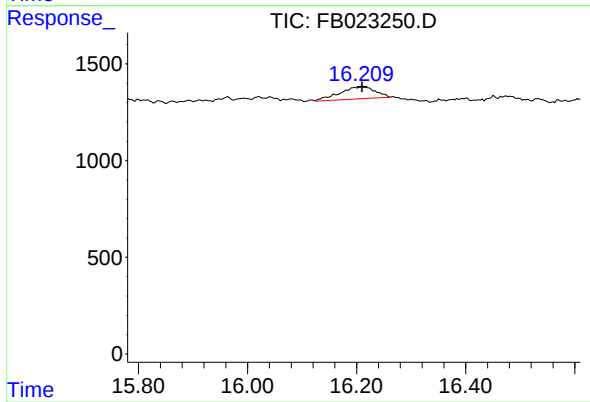

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 2800
Conc: 0.10 ng/ml