

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121719\
Data File : FB023252.D
Signal(s) : FID2B.CH
Acq On : 17 Dec 2019 10:00
Operator : DD/AJ
Sample : VBF1217S2
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 18 00:57:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	469258	19.104 ng/ml
Target Compounds			
6) t Toluene	10.623	1493	0.037 ng/ml
9) t O-Xylene	13.972	3712	0.107 ng/ml
10) t 1,2,4-Trimethylbenzene	16.213	3657	0.130 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121719\
Data File : FB023252.D
Signal(s) : FID2B.CH
Acq On : 17 Dec 2019 10:00
Operator : DD/AJ
Sample : VBF1217S2
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 18 00:57:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

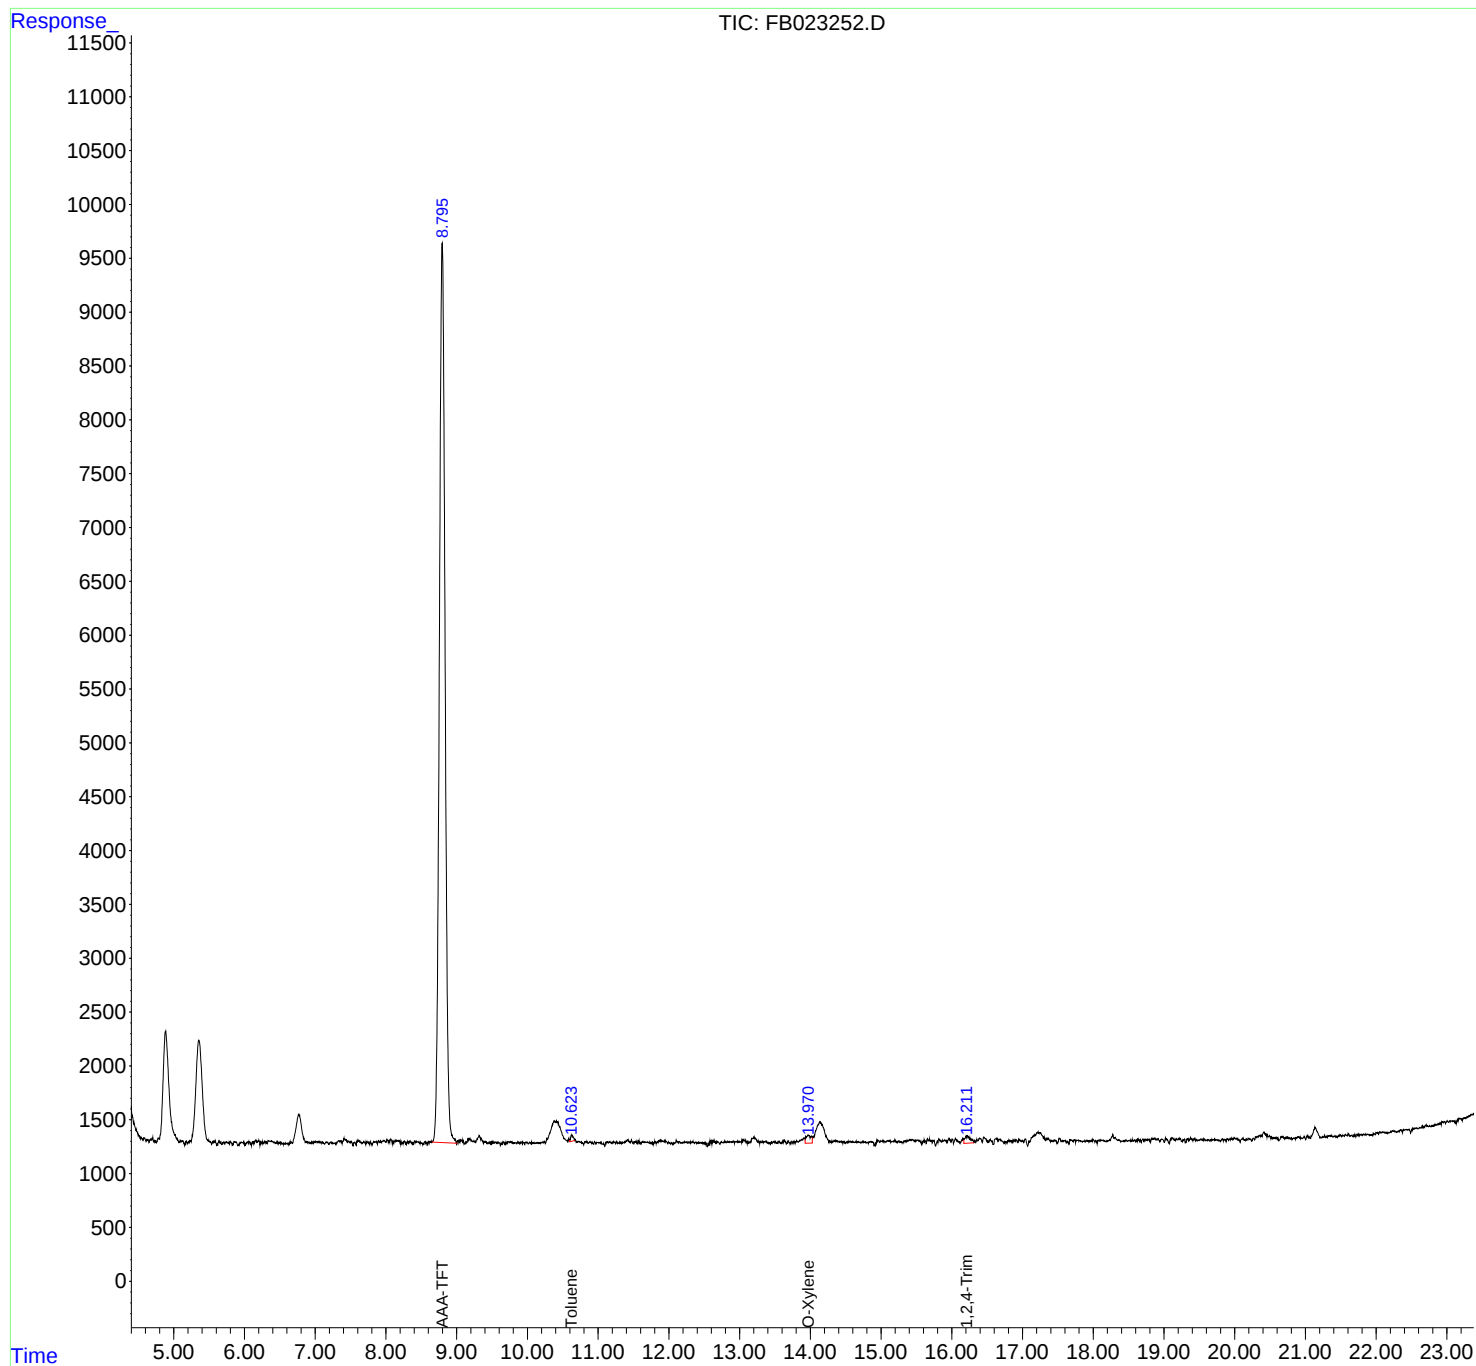


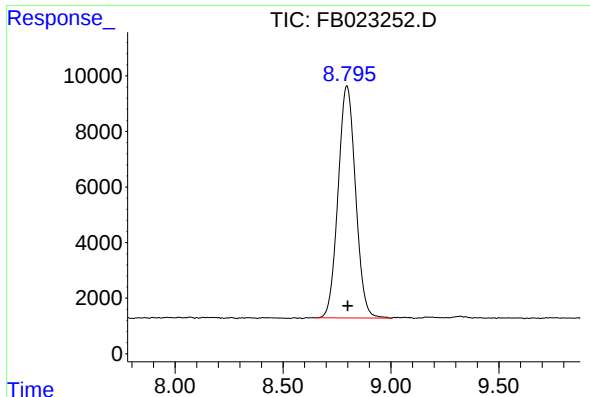

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 469258
Conc: 19.10 ng/ml

Instrument :
FID_B
ClientSampleId :

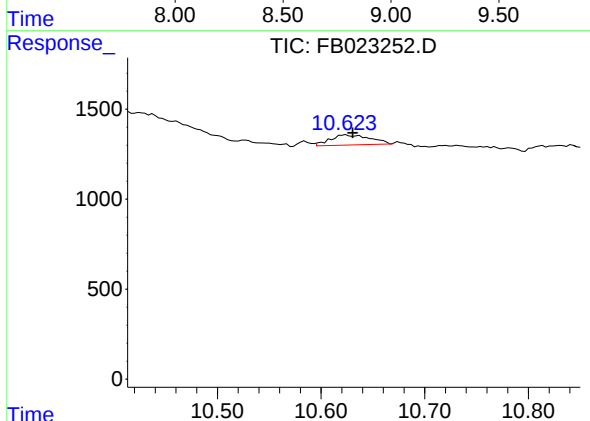


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.007 min
Response: 1493
Conc: 0.04 ng/ml

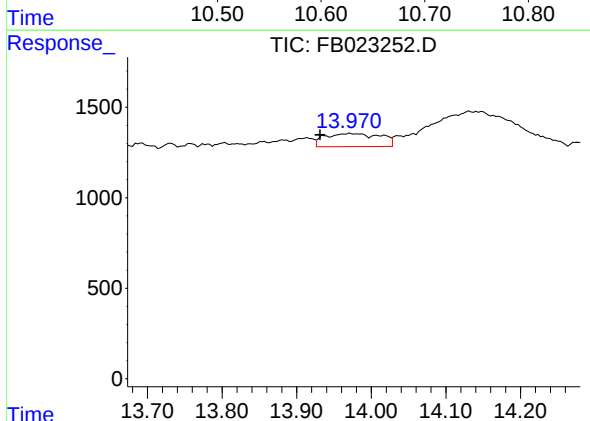

#9 O-Xylene

R.T.: 13.972 min
Delta R.T.: 0.041 min
Response: 3712
Conc: 0.11 ng/ml

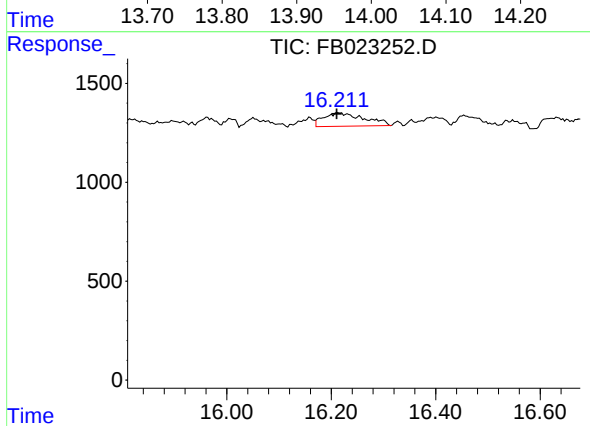

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.003 min
Response: 3657
Conc: 0.13 ng/ml