

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121719\
 Data File : FB023262.D
 Signal(s) : FID2B.CH
 Acq On : 17 Dec 2019 16:21
 Operator : DD/AJ
 Sample : K6325-05
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 RT-3425

Integration File: Calibration.e
 Quant Time: Dec 18 00:58:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	539824	21.976 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.691	7130	0.218 ng/ml
6) t	Toluene	10.634	17004	0.422 ng/ml
7) t	Ethylbenzene	13.071	98190	2.545 ng/ml
8) t	m-Xylene	13.201	162626	4.469 ng/ml
9) t	O-Xylene	13.937	132599	3.819 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	390340	13.919 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121719\
Data File : FB023262.D
Signal(s) : FID2B.CH
Acq On : 17 Dec 2019 16:21
Operator : DD/AJ
Sample : K6325-05
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RT-3425

Integration File: Calibration.e
Quant Time: Dec 18 00:58:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

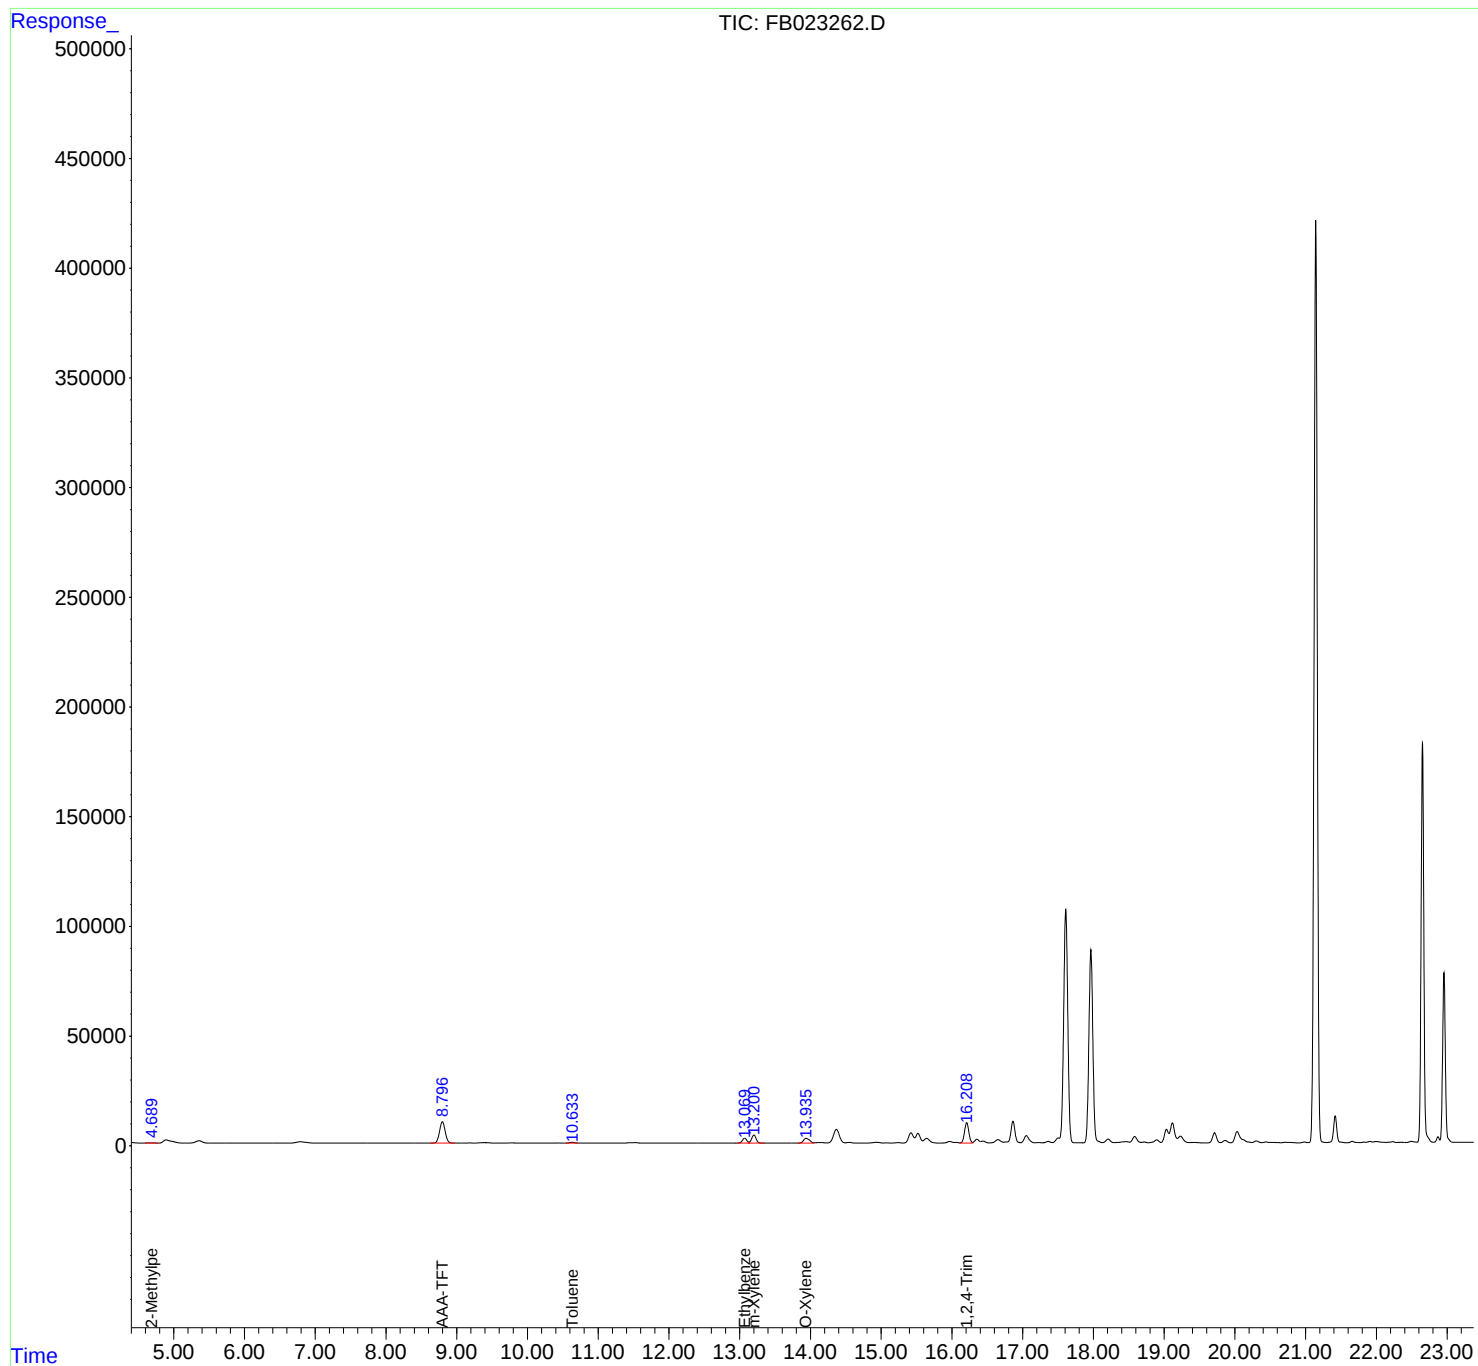


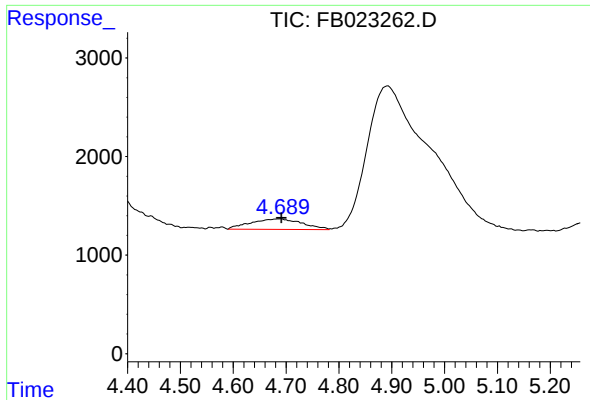

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 7130
Conc: 0.22 ng/ml

Instrument :
FID_B
ClientSampleId :
RT-3425

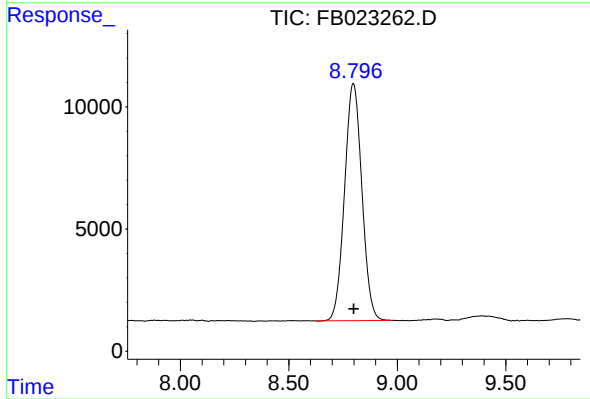


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: -0.001 min
Response: 539824
Conc: 21.98 ng/ml

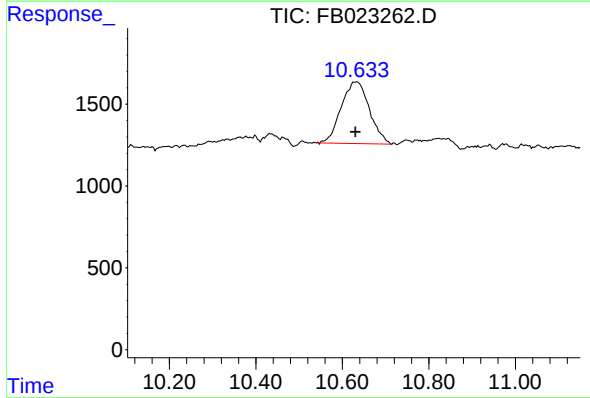


#6 Toluene

R.T.: 10.634 min
Delta R.T.: 0.004 min
Response: 17004
Conc: 0.42 ng/ml

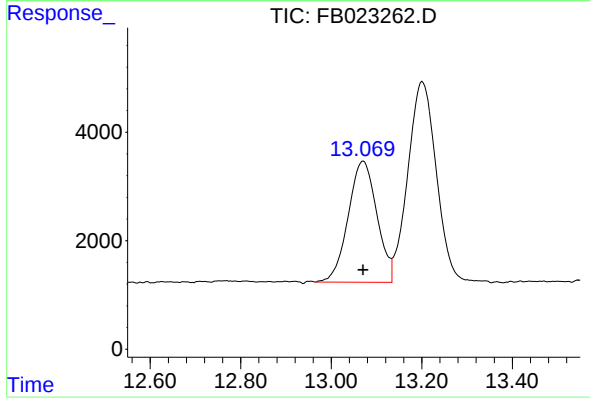

#7 Ethylbenzene


R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 98190
Conc: 2.54 ng/ml

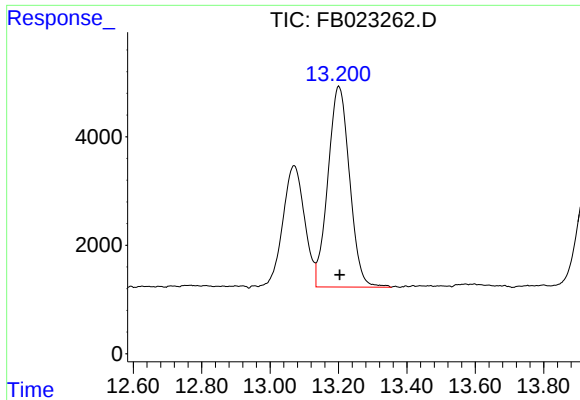

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.002 min
Response: 162626
Conc: 4.47 ng/ml

Instrument :
FID_B
ClientSampleId :
RT-3425

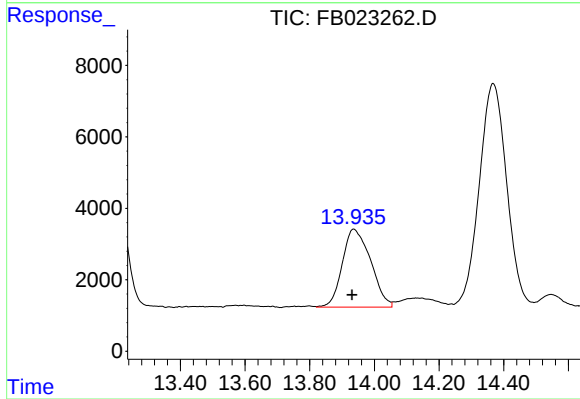

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.005 min
Response: 132599
Conc: 3.82 ng/ml

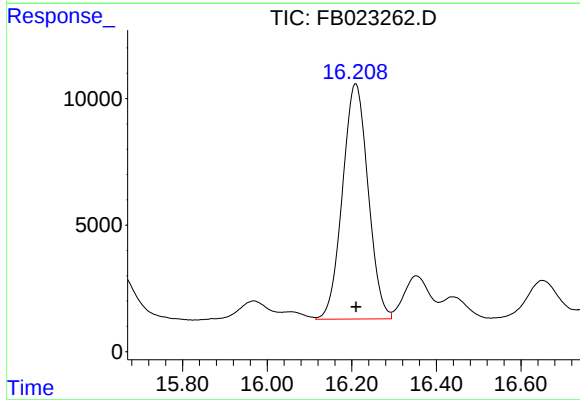

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 390340
Conc: 13.92 ng/ml