

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121719\
 Data File : FB023267.D
 Signal(s) : FID2B.CH
 Acq On : 17 Dec 2019 18:53
 Operator : DD/AJ
 Sample : K6333-04MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-1A-COMPMSD

Integration File: Calibration.e
 Quant Time: Dec 18 00:59:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	411895	16.768 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	710961	21.756 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	805018	23.086 ng/ml
3) t n-Heptane	7.756	257864	7.500 ng/ml
4) t Benzene	7.891	330248	7.926 ng/ml
6) t Toluene	10.629	971109	24.107 ng/ml
7) t Ethylbenzene	13.070	312070	8.087 ng/ml
8) t m-Xylene	13.203	597548	16.421 ng/ml
9) t O-Xylene	13.931	583467	16.805 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	495161	17.657 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121719\
Data File : FB023267.D
Signal(s) : FID2B.CH
Acq On : 17 Dec 2019 18:53
Operator : DD/AJ
Sample : K6333-04MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-1A-COMPMSD

Integration File: Calibration.e
Quant Time: Dec 18 00:59:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

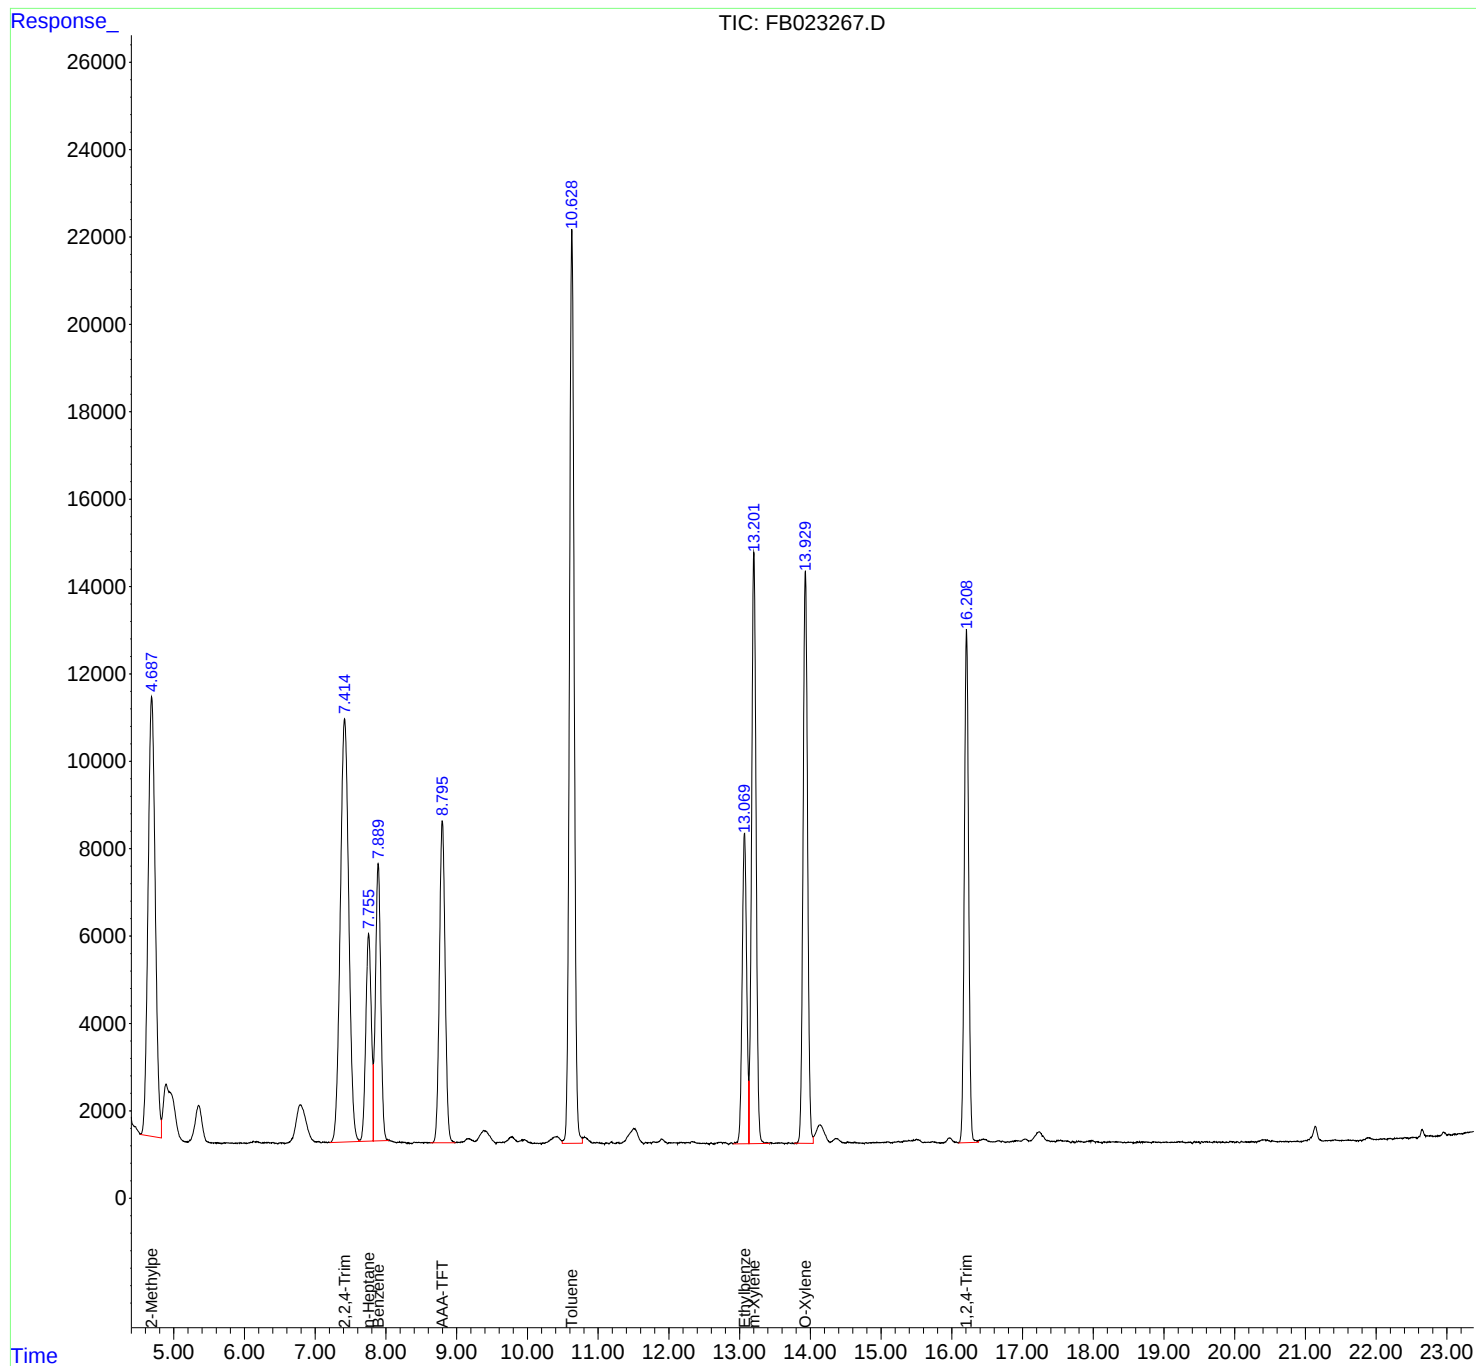


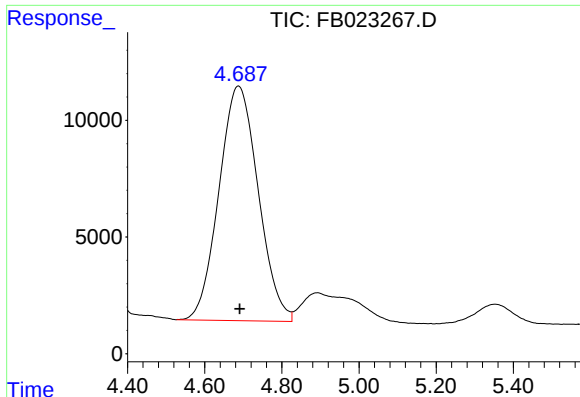

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 710961
Conc: 21.76 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1A-COMPMSD

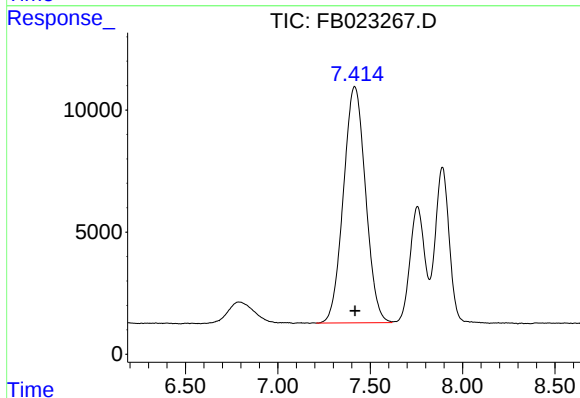


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 805018
Conc: 23.09 ng/ml

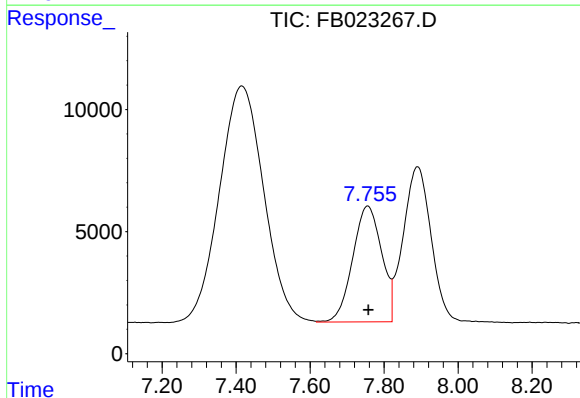


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 257864
Conc: 7.50 ng/ml

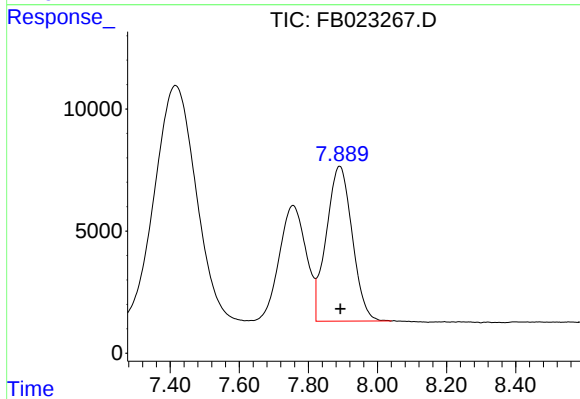

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.001 min
Response: 330248
Conc: 7.93 ng/ml

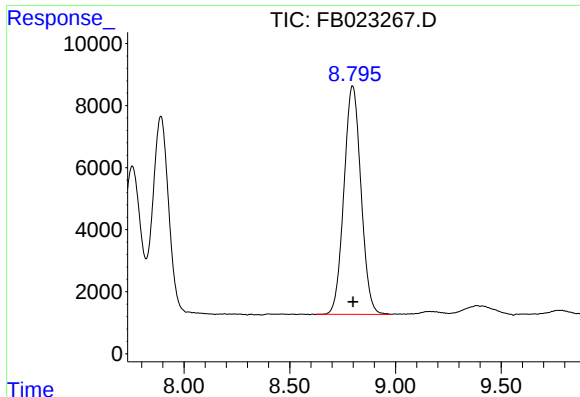

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 411895
Conc: 16.77 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1A-COMPMSD

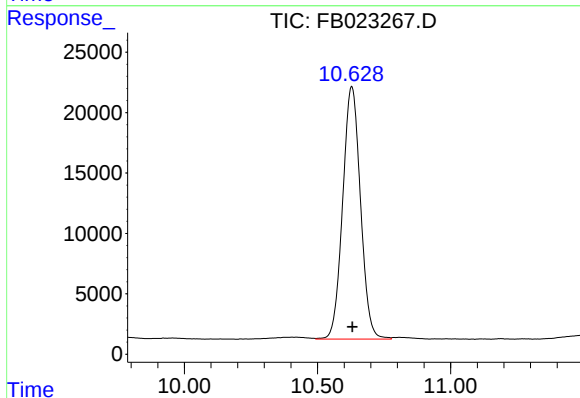


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 971109
Conc: 24.11 ng/ml

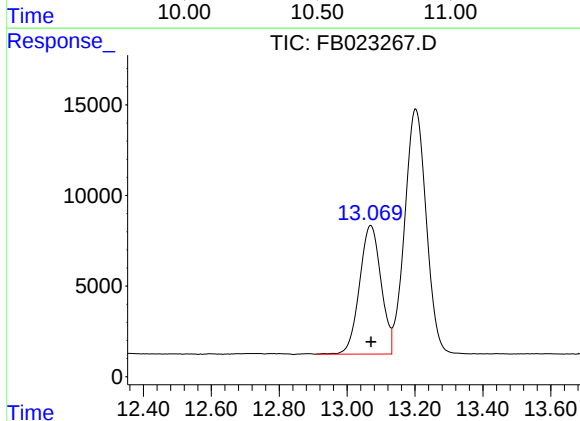


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.000 min
Response: 312070
Conc: 8.09 ng/ml

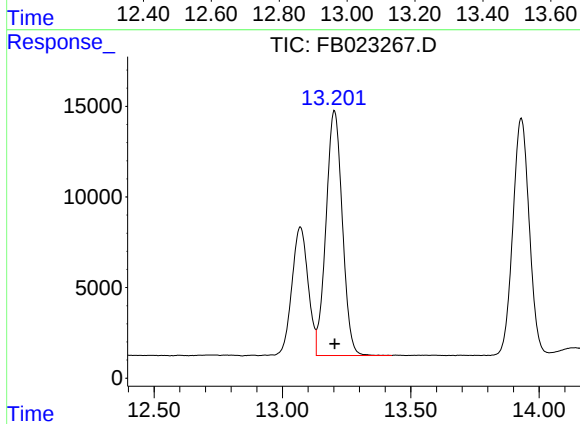

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.000 min
Response: 597548
Conc: 16.42 ng/ml

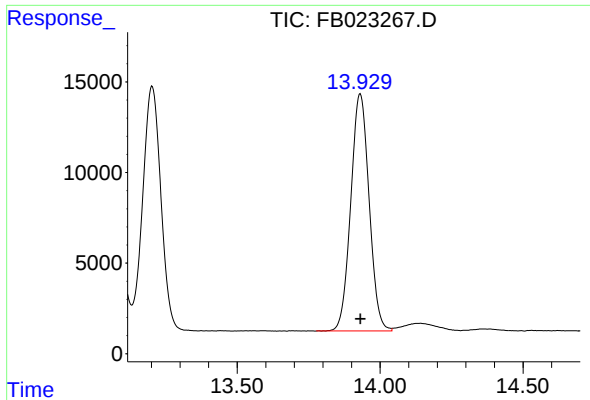

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 583467
Conc: 16.80 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1A-COMPMSD

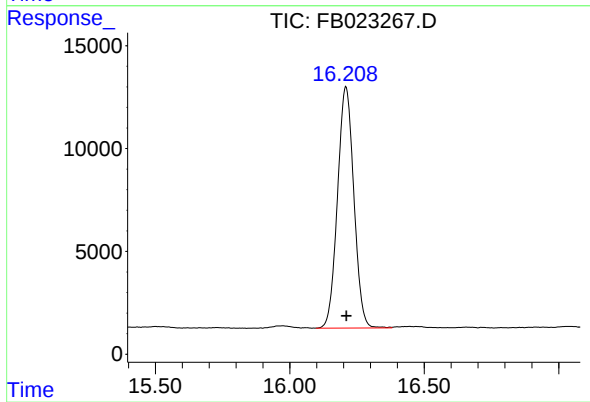

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.002 min
Response: 495161
Conc: 17.66 ng/ml