

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121721\
 Data File : FB026529.D
 Signal(s) : FID2B.CH
 Acq On : 17 Dec 2021 11:10
 Operator : AJ/MA
 Sample : BSF1217S1
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1217S1

Integration File: SAMPLE.e
 Quant Time: Dec 17 21:44:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	263184	23.426 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	482970	27.746 ng/ml
2) t 2,2,4-Trimethylpentane	7.435	562985	28.388 ng/ml
3) t n-Heptane	7.750	178546	9.327 ng/ml
4) t Benzene	7.886	208035	9.357 ng/ml
6) t Toluene	10.619	603601	28.288 ng/ml
7) t Ethylbenzene	13.056	187514	9.499 ng/ml
8) t m-Xylene	13.189	374188	18.979 ng/ml
9) t O-Xylene	13.916	366714	19.202 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	375202	19.313 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121721\
Data File : FB026529.D
Signal(s) : FID2B.CH
Acq On : 17 Dec 2021 11:10
Operator : AJ/MA
Sample : BSF1217S1
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1217S1

Integration File: SAMPLE.e
Quant Time: Dec 17 21:44:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

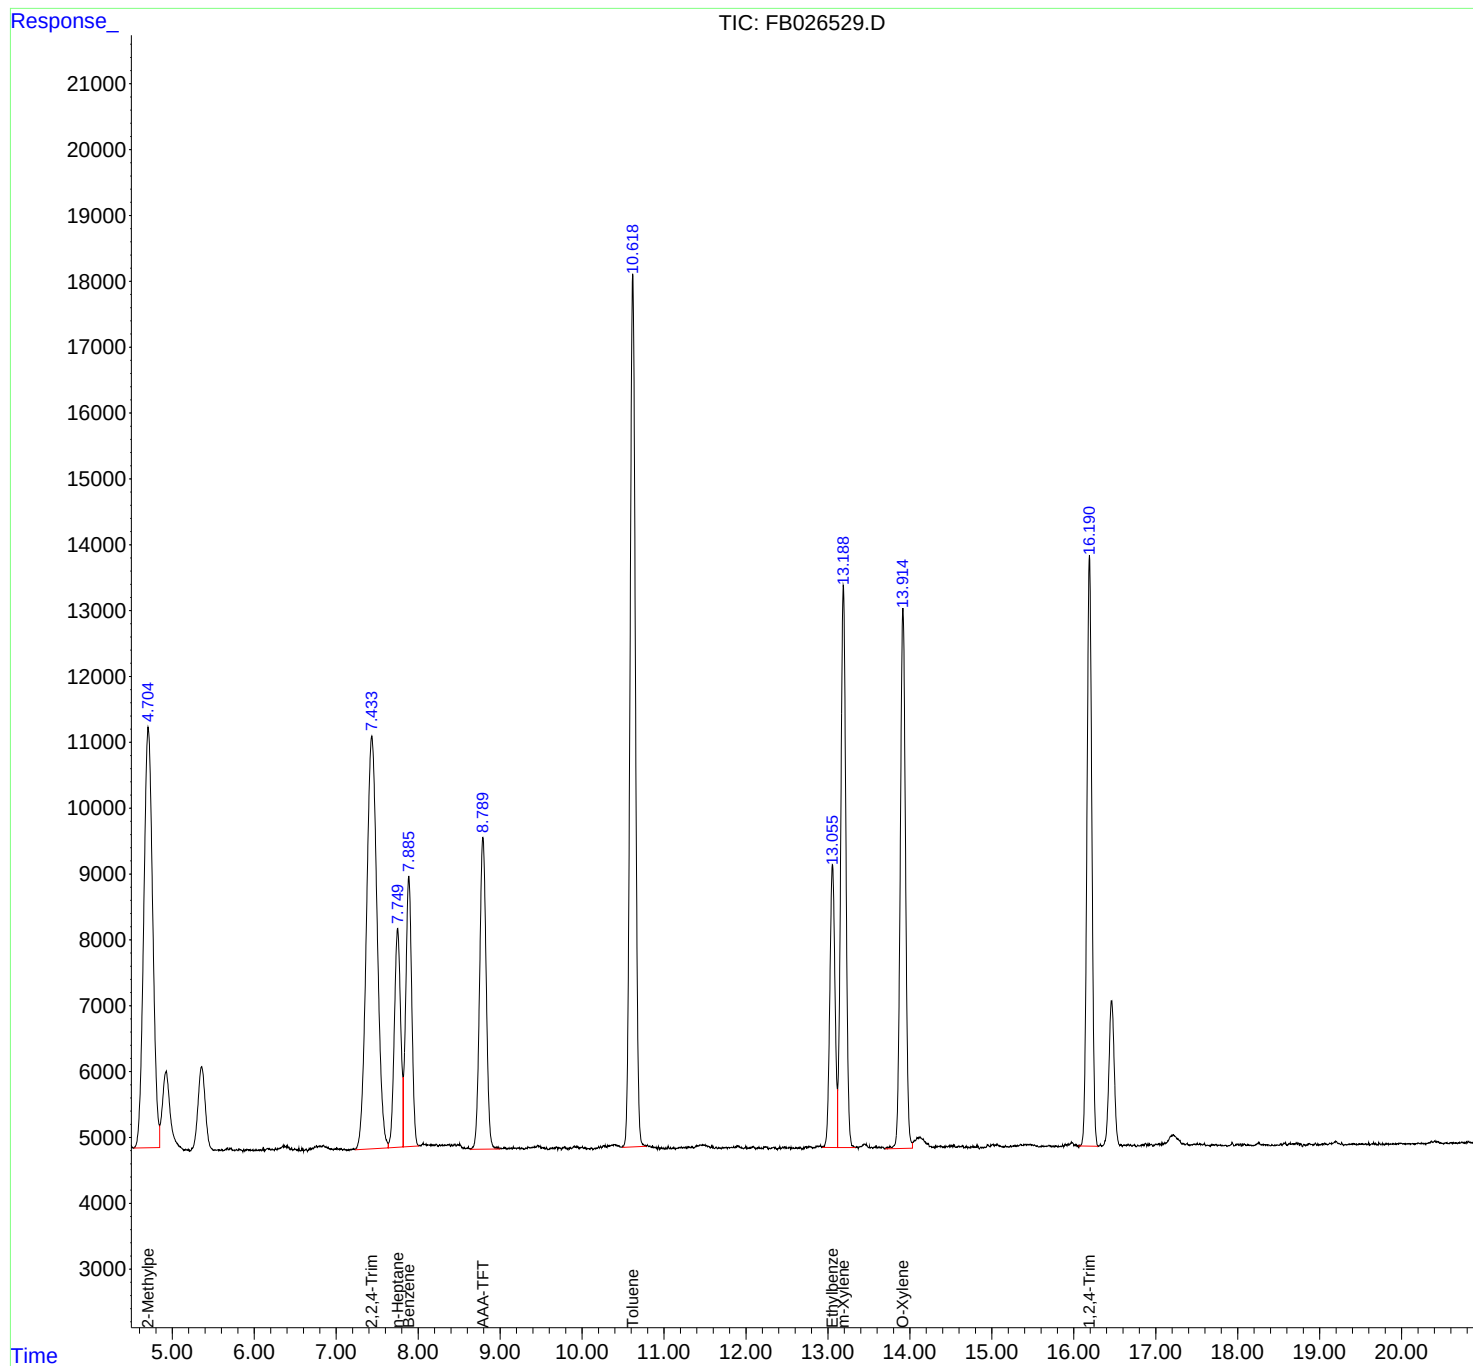


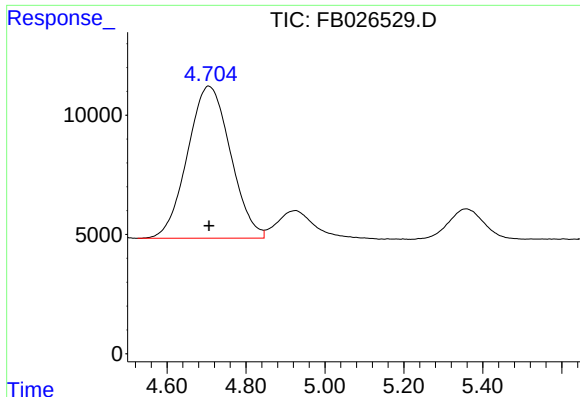

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: 0.000 min
Response: 482970
Conc: 27.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1217S1

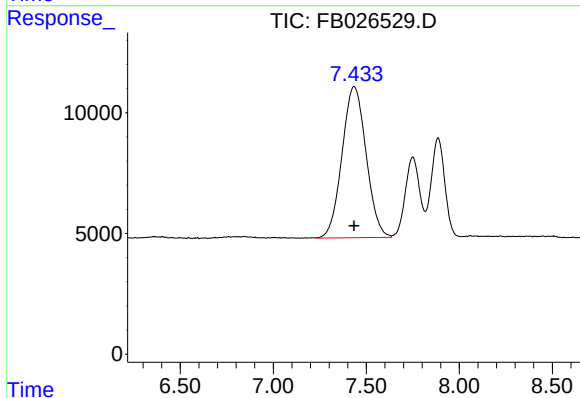


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.000 min
Response: 562985
Conc: 28.39 ng/ml

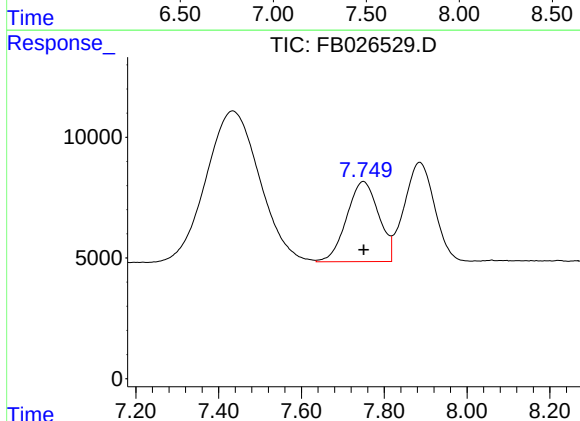


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 178546
Conc: 9.33 ng/ml

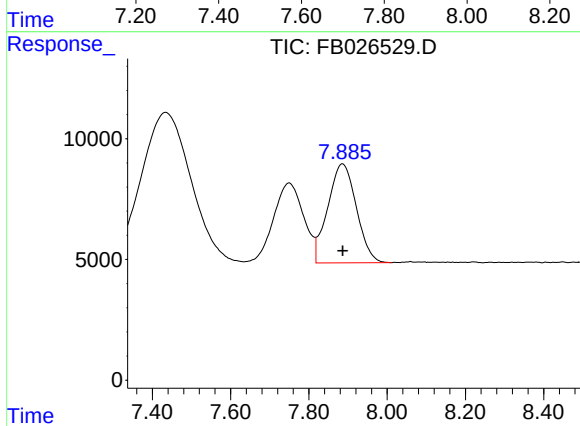

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 208035
Conc: 9.36 ng/ml

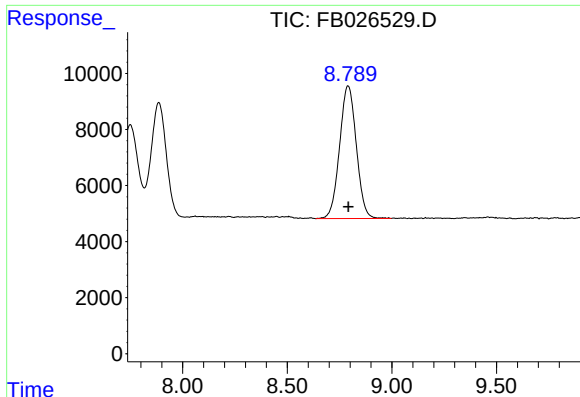

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.001 min
Response: 263184
Conc: 23.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1217S1

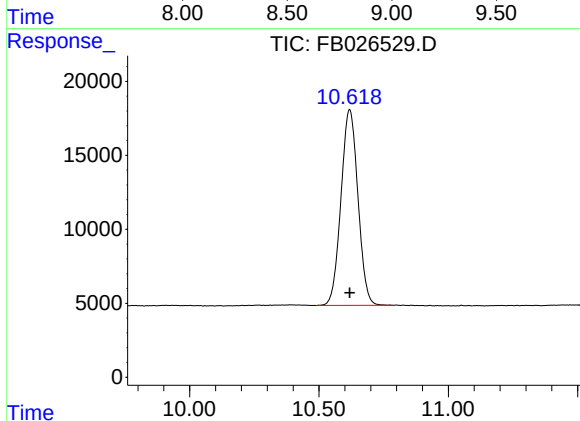


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 603601
Conc: 28.29 ng/ml

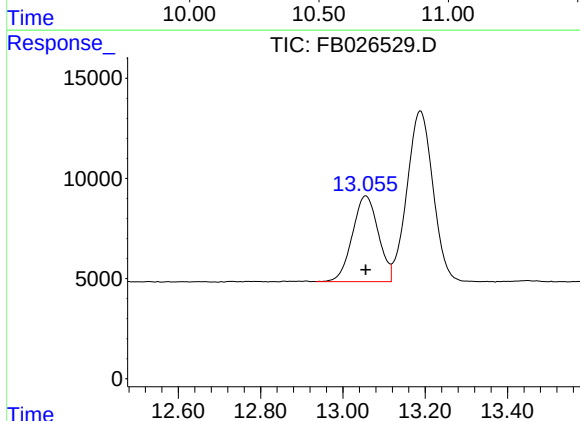


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 187514
Conc: 9.50 ng/ml

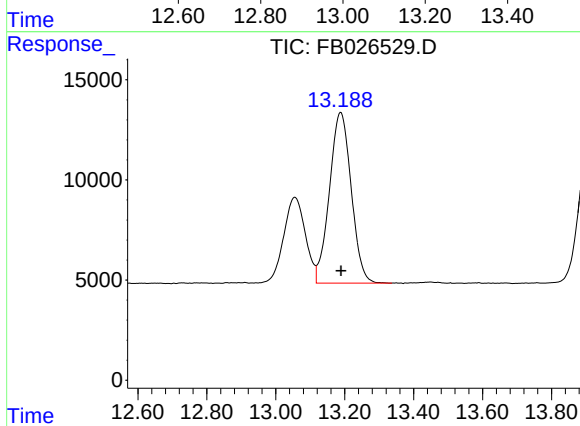

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 374188
Conc: 18.98 ng/ml

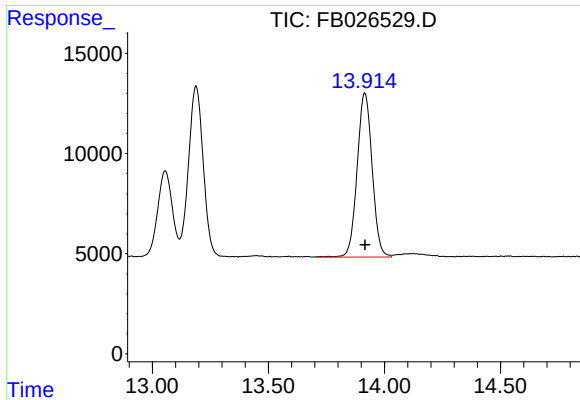

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 366714
Conc: 19.20 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1217S1

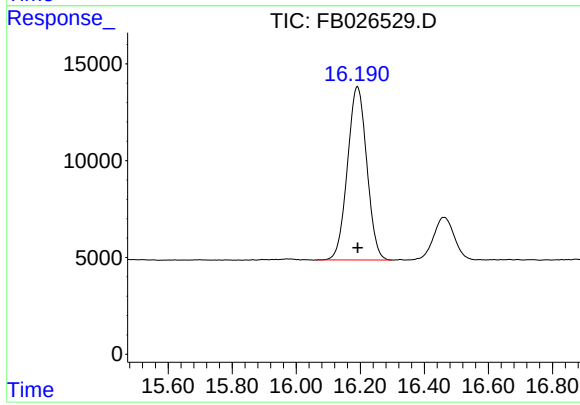

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 375202
Conc: 19.31 ng/ml