

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121721\
 Data File : FB026536.D
 Signal(s) : FID2B.CH
 Acq On : 17 Dec 2021 15:28
 Operator : AJ/MA
 Sample : M5082-03MS
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-121-1(65-77.7)MS

Integration File: SAMPLE.e
 Quant Time: Dec 17 21:45:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	241662	21.510 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	510651	29.336 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	589332	29.717 ng/ml
3) t n-Heptane	7.750	193138	10.090 ng/ml
4) t Benzene	7.886	225561	10.145 ng/ml
6) t Toluene	10.619	646589	30.302 ng/ml
7) t Ethylbenzene	13.056	200762	10.170 ng/ml
8) t m-Xylene	13.189	398810	20.228 ng/ml
9) t O-Xylene	13.916	386012	20.213 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	380602	19.591 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121721\
Data File : FB026536.D
Signal(s) : FID2B.CH
Acq On : 17 Dec 2021 15:28
Operator : AJ/MA
Sample : M5082-03MS
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-121-1(65-77.7)MS

Integration File: SAMPLE.e
Quant Time: Dec 17 21:45:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

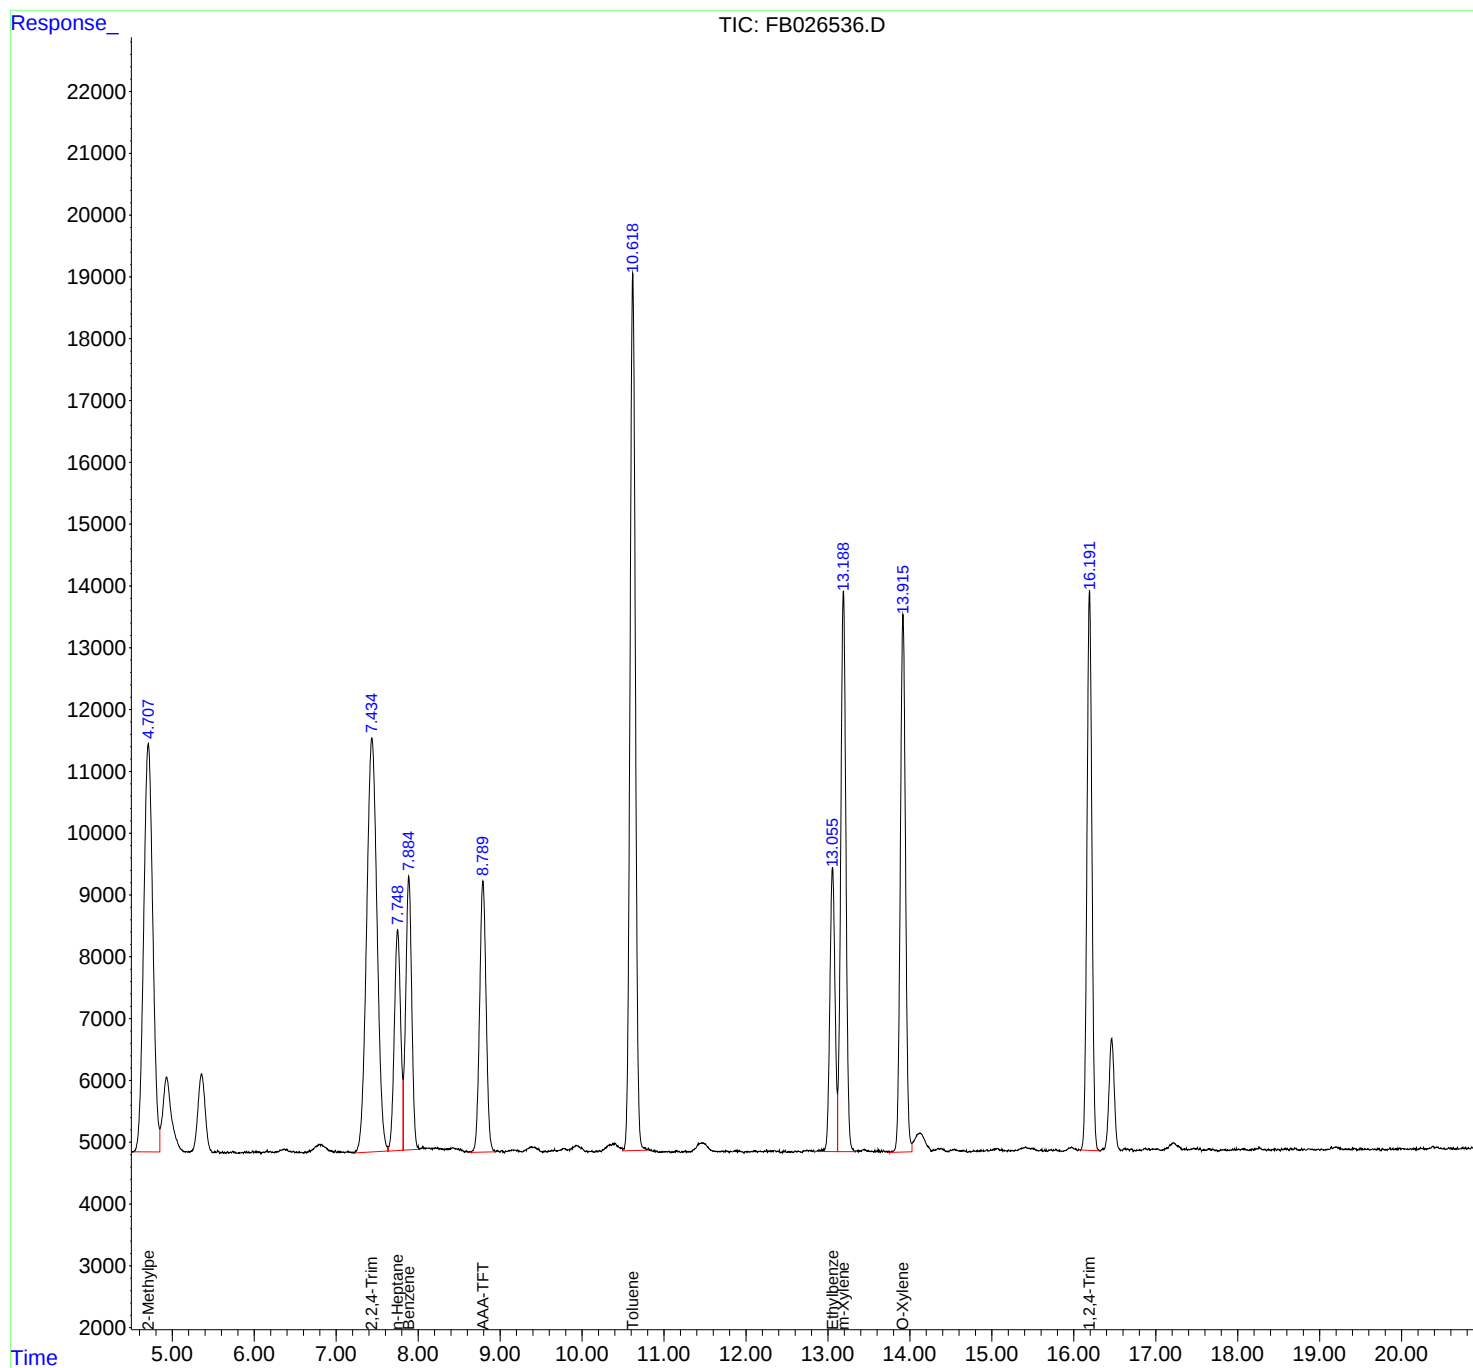


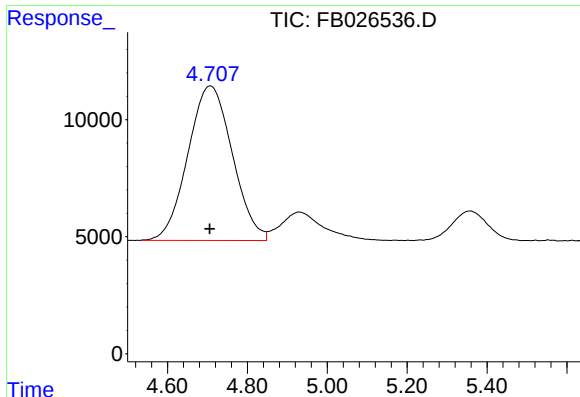

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.002 min
Response: 510651
Conc: 29.34 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-121-1(65-77.7)MS

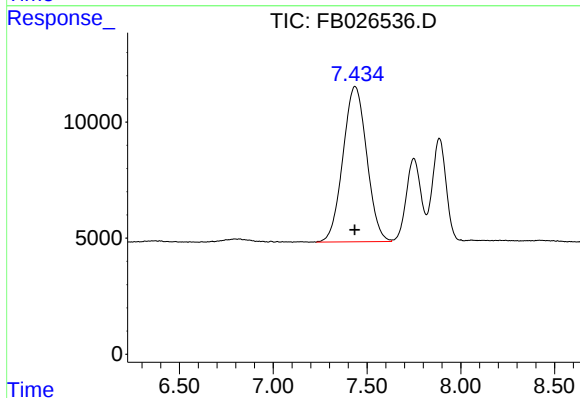


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: 0.000 min
Response: 589332
Conc: 29.72 ng/ml

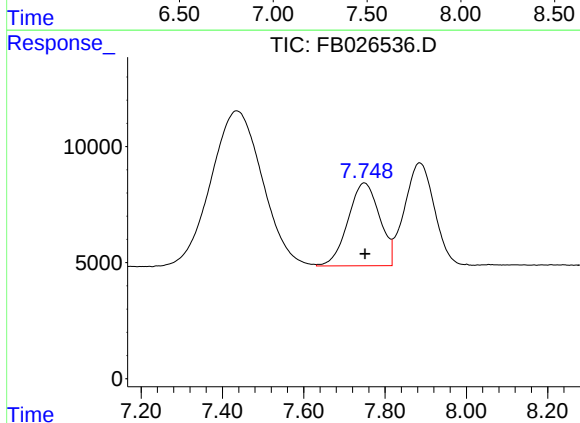


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.001 min
Response: 193138
Conc: 10.09 ng/ml

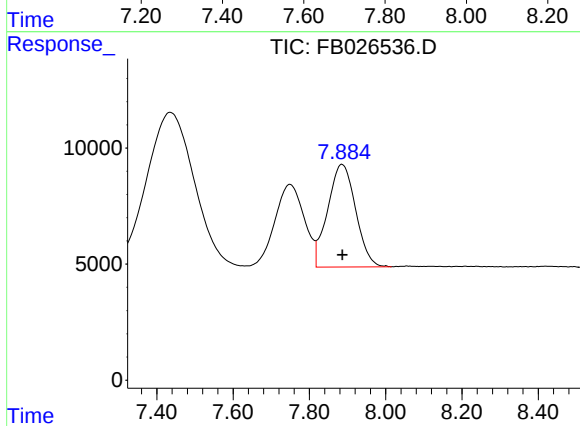

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.001 min
Response: 225561
Conc: 10.14 ng/ml

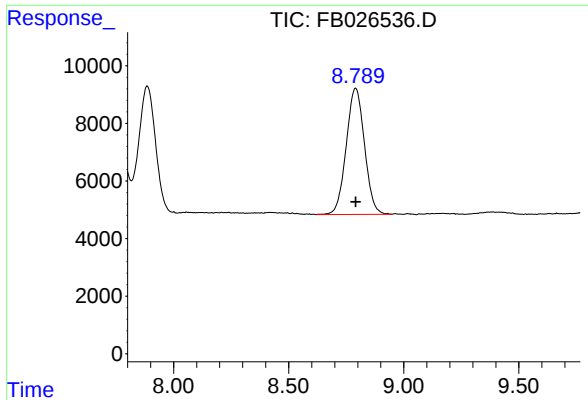

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 241662
Conc: 21.51 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-121-1(65-77.7)MS

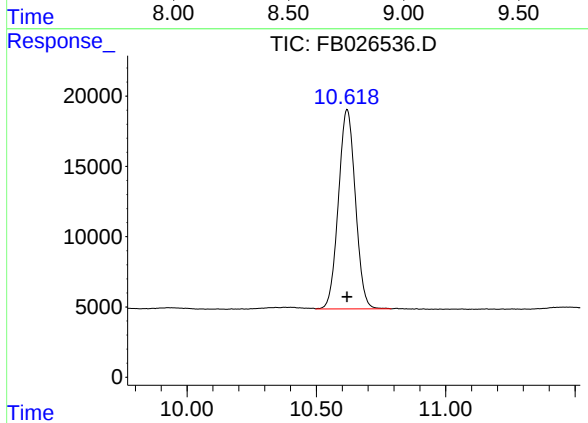


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 646589
Conc: 30.30 ng/ml

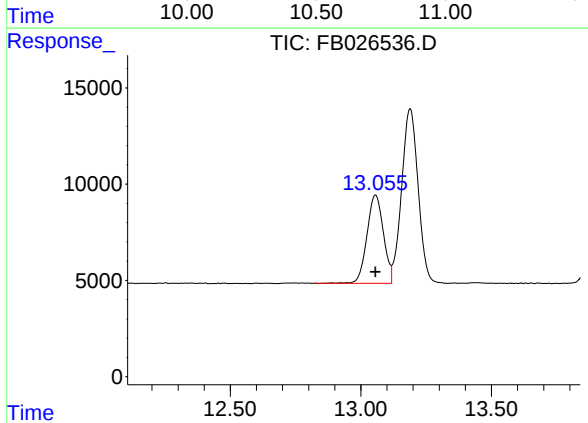


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 200762
Conc: 10.17 ng/ml

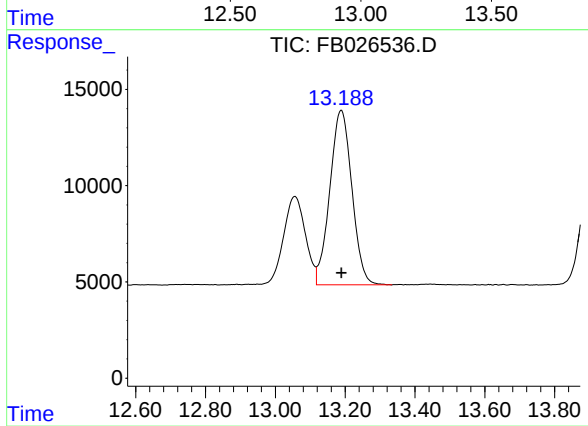

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 398810
Conc: 20.23 ng/ml

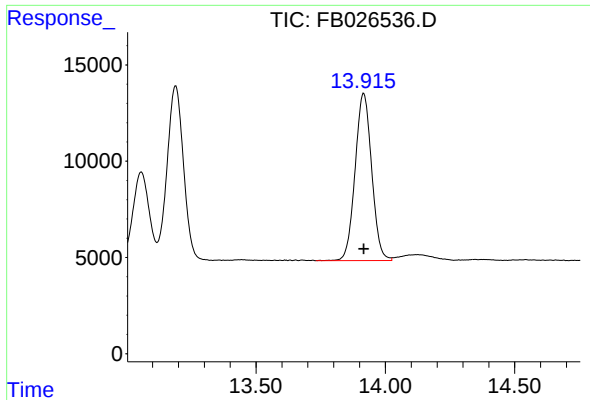

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 386012
Conc: 20.21 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-121-1(65-77.7)MS

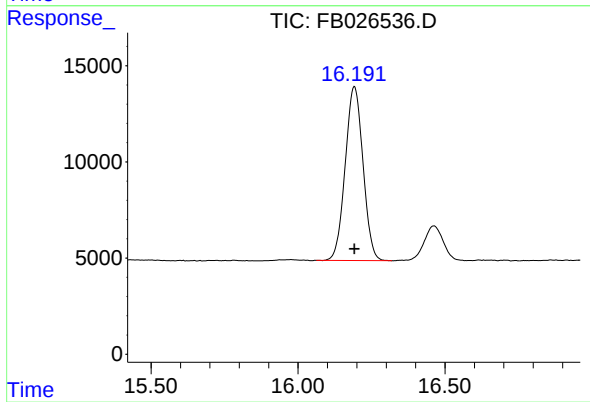

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 380602
Conc: 19.59 ng/ml