

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121721\
 Data File : FB026537.D
 Signal(s) : FID2B.CH
 Acq On : 17 Dec 2021 16:05
 Operator : AJ/MA
 Sample : M5082-03MSD
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-121-1(65-77.7)MSD

Integration File: SAMPLE.e
 Quant Time: Dec 17 21:45:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	218063	19.409 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	480999	27.633 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	586571	29.578 ng/ml
3) t n-Heptane	7.749	173924	9.086 ng/ml
4) t Benzene	7.886	205665	9.250 ng/ml
6) t Toluene	10.619	612079	28.685 ng/ml
7) t Ethylbenzene	13.057	194452	9.850 ng/ml
8) t m-Xylene	13.190	391366	19.850 ng/ml
9) t O-Xylene	13.916	385820	20.203 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	405980	20.898 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121721\
Data File : FB026537.D
Signal(s) : FID2B.CH
Acq On : 17 Dec 2021 16:05
Operator : AJ/MA
Sample : M5082-03MSD
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-121-1(65-77.7)MSD

Integration File: SAMPLE.e
Quant Time: Dec 17 21:45:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

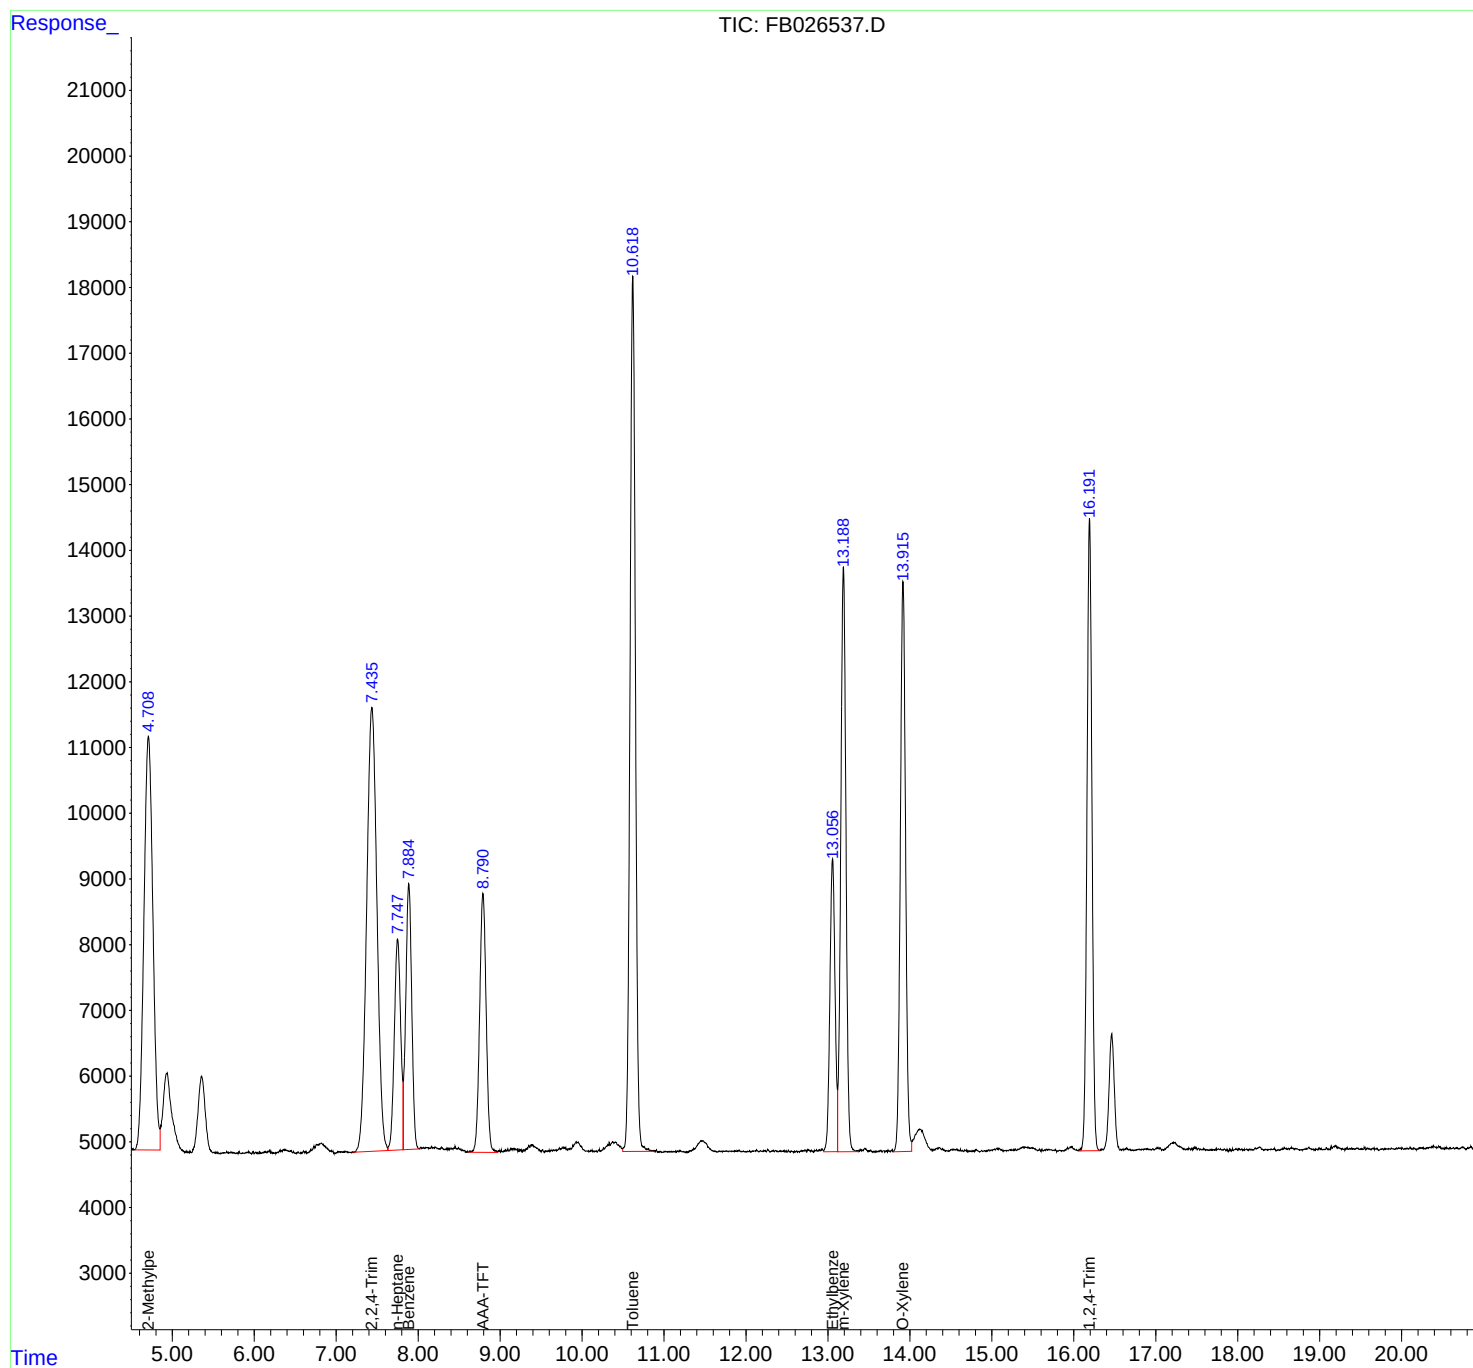


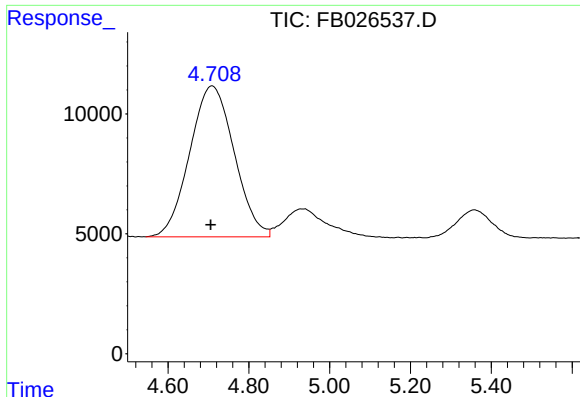

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.004 min
Response: 480999
Conc: 27.63 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-121-1(65-77.7)MSD

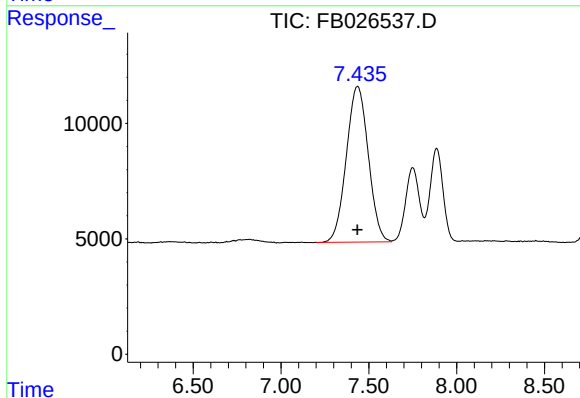


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: 0.001 min
Response: 586571
Conc: 29.58 ng/ml

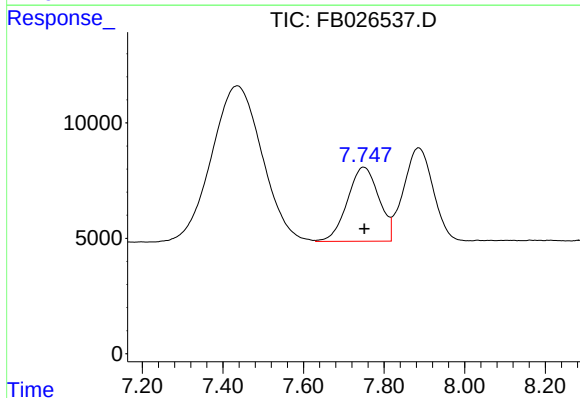


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 173924
Conc: 9.09 ng/ml

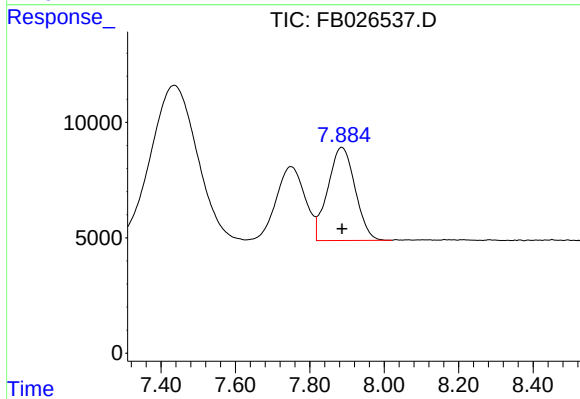

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 205665
Conc: 9.25 ng/ml

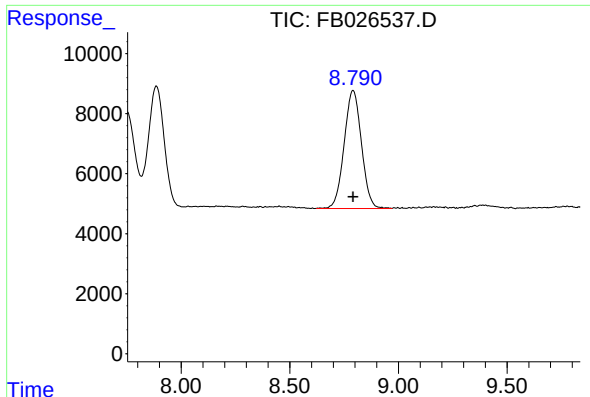

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 218063
Conc: 19.41 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-121-1(65-77.7)MSD

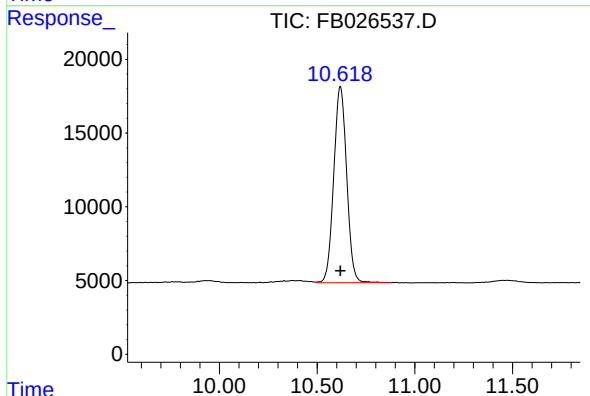


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 612079
Conc: 28.68 ng/ml

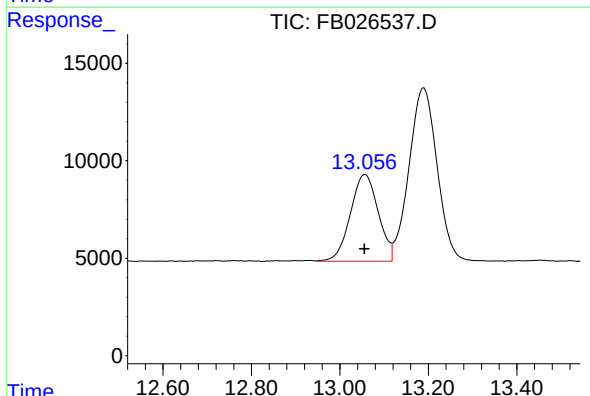


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.002 min
Response: 194452
Conc: 9.85 ng/ml

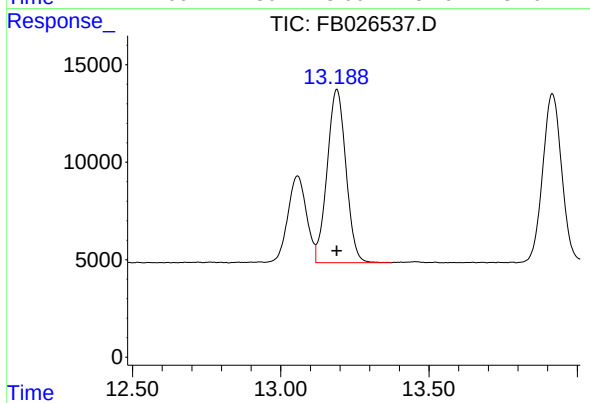

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 391366
Conc: 19.85 ng/ml

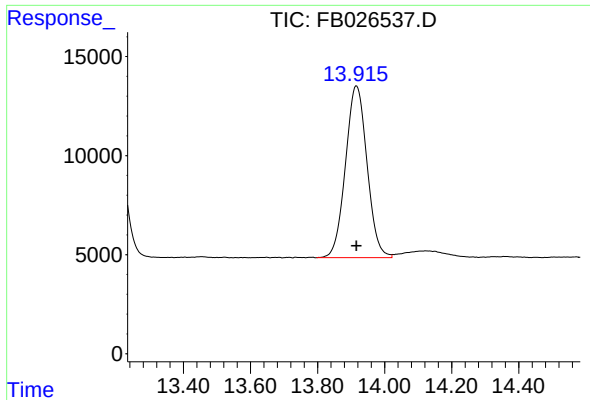

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 385820
Conc: 20.20 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-121-1(65-77.7)MSD

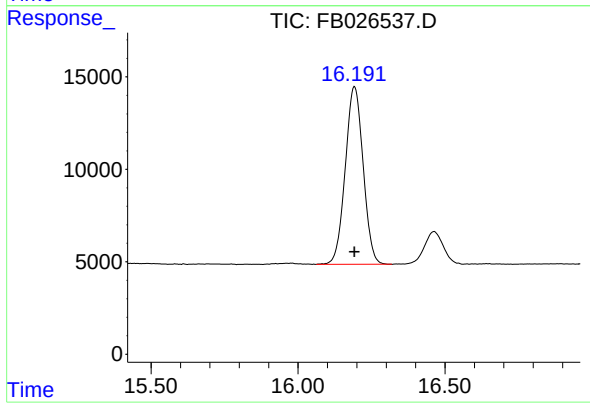

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 405980
Conc: 20.90 ng/ml