

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121819\
Data File : FB023273.D
Signal(s) : FID2B.CH
Acq On : 18 Dec 2019 11:47
Operator : DD/AJ
Sample : VBF1218S2
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 19 00:12:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	474647	19.323 ng/ml
Target Compounds			
6) t Toluene	10.615	3182	0.079 ng/ml
7) t Ethylbenzene	13.028	2194	0.057 ng/ml
8) t m-Xylene	13.193	349	0.010 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	1563	0.056 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121819\
Data File : FB023273.D
Signal(s) : FID2B.CH
Acq On : 18 Dec 2019 11:47
Operator : DD/AJ
Sample : VBF1218S2
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 19 00:12:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

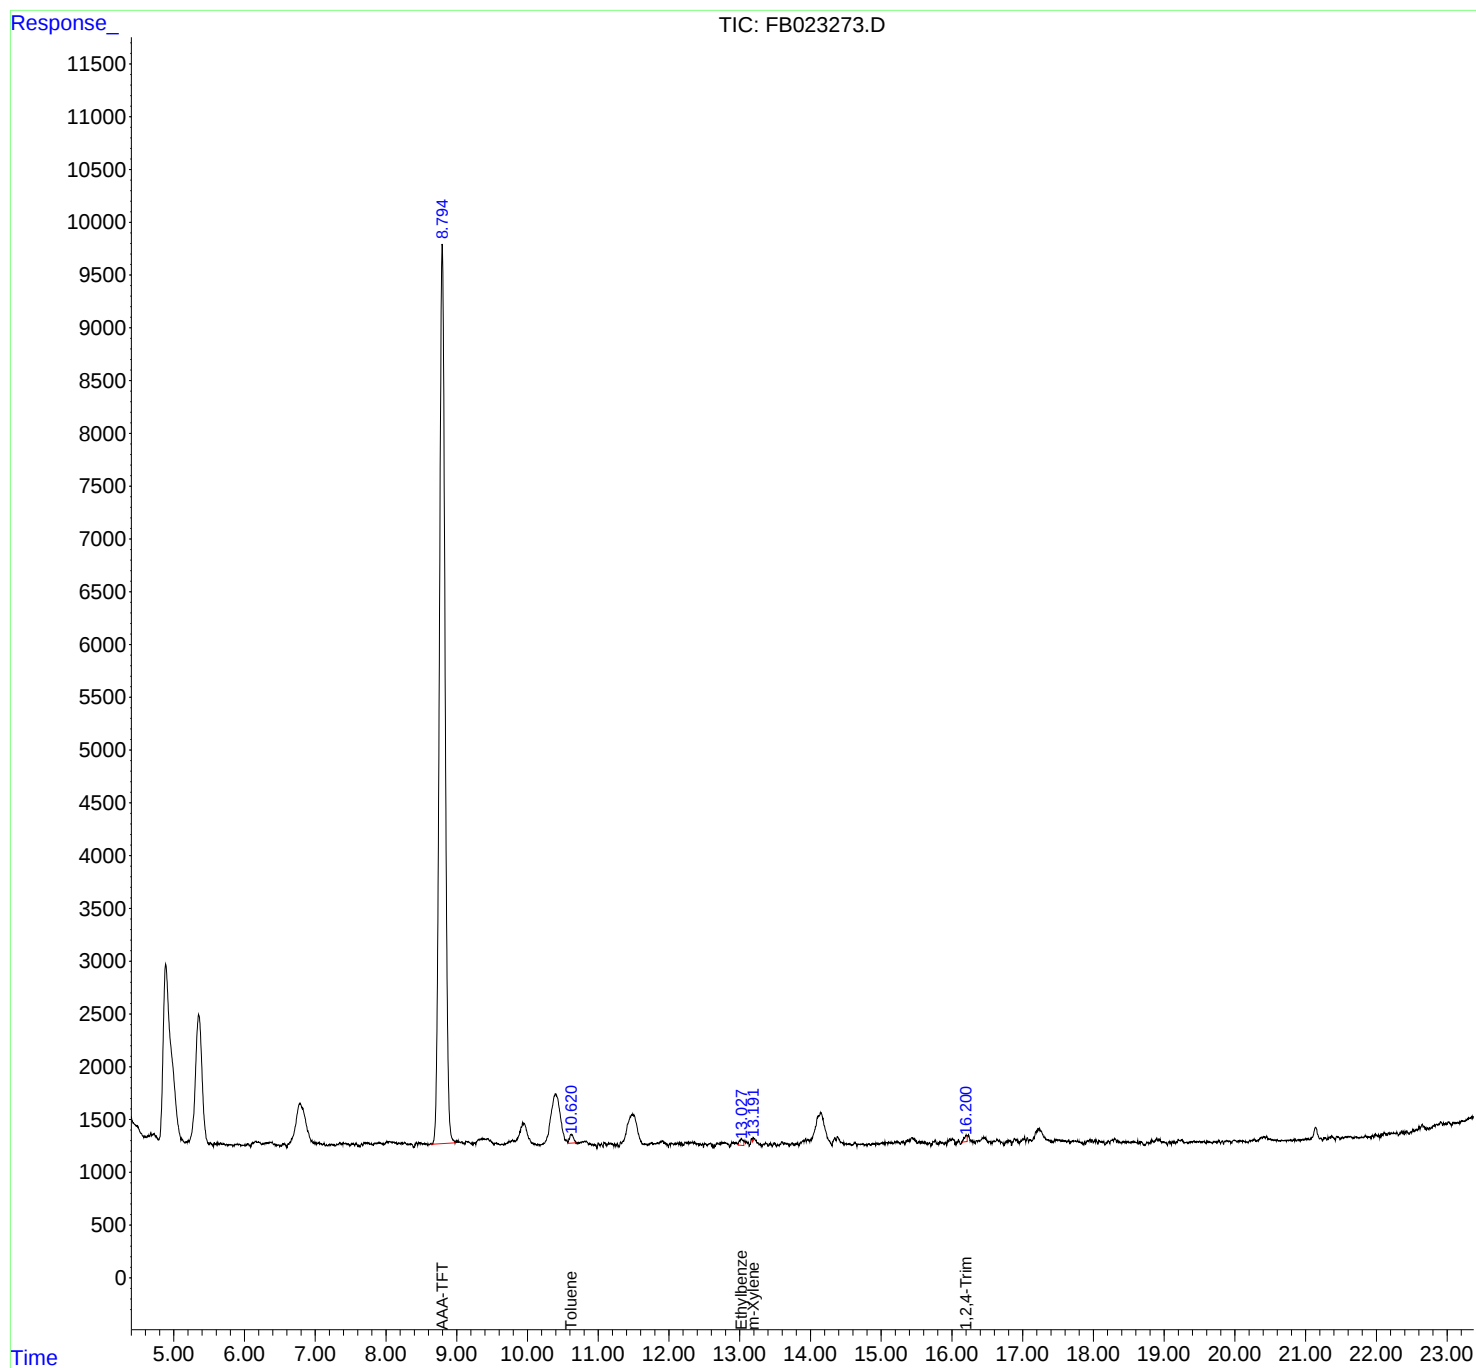

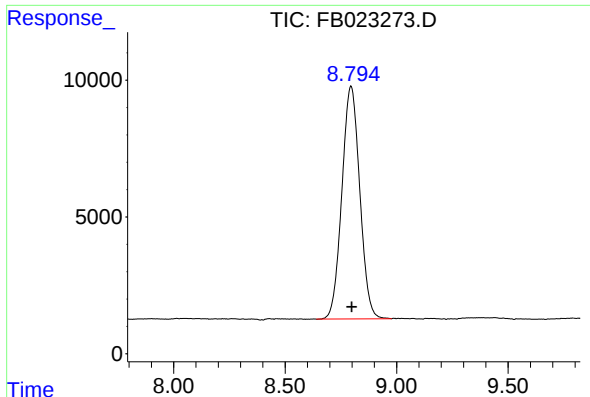


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: -0.003 min
Response: 474647
Conc: 19.32 ng/ml

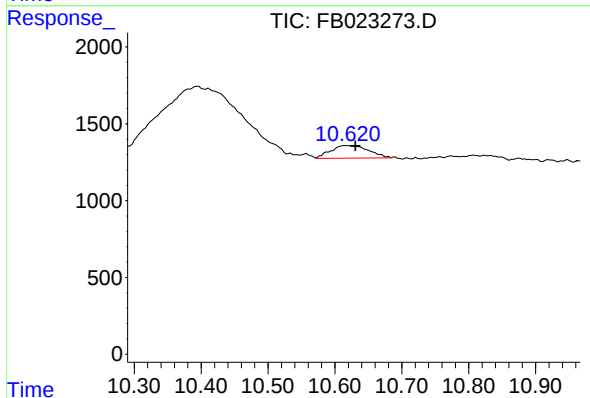


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.015 min
Response: 3182
Conc: 0.08 ng/ml

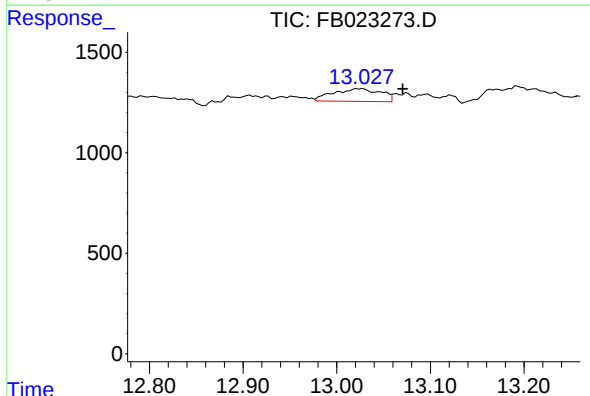


#7 Ethylbenzene

R.T.: 13.028 min
Delta R.T.: -0.042 min
Response: 2194
Conc: 0.06 ng/ml

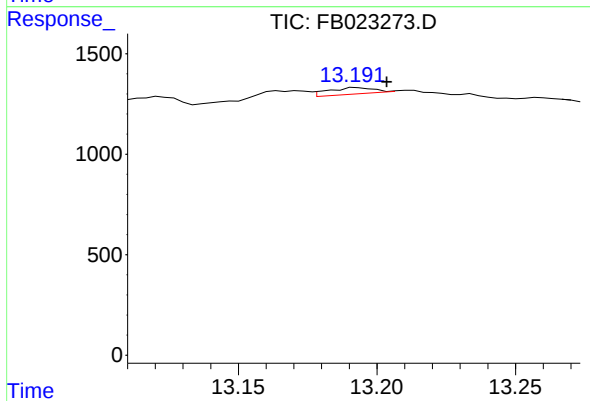

#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: -0.010 min
Response: 349
Conc: 0.01 ng/ml

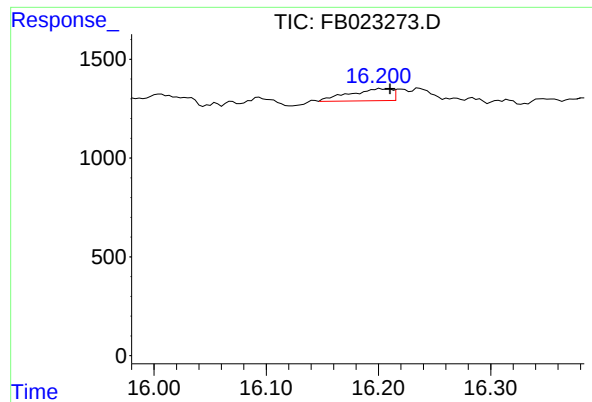

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.009 min
Response: 1563
Conc: 0.06 ng/ml