

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121819\
 Data File : FB023275.D
 Signal(s) : FID2B.CH
 Acq On : 18 Dec 2019 16:16
 Operator : DD/AJ
 Sample : BSF1218S2
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 19 00:12:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
 Quant Title :
 QLast Update : Fri Nov 22 12:34:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	464667	18.917 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	797366	24.401 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	952339	27.311 ng/ml
3) t n-Heptane	7.751	306616	8.918 ng/ml
4) t Benzene	7.887	372547	8.942 ng/ml
6) t Toluene	10.625	1076744	26.729 ng/ml
7) t Ethylbenzene	13.065	343834	8.910 ng/ml
8) t m-Xylene	13.198	648412	17.819 ng/ml
9) t O-Xylene	13.926	629008	18.116 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	534712	19.067 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121819\
Data File : FB023275.D
Signal(s) : FID2B.CH
Acq On : 18 Dec 2019 16:16
Operator : DD/AJ
Sample : BSF1218S2
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 19 00:12:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB112219.M
Quant Title :
QLast Update : Fri Nov 22 12:34:56 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

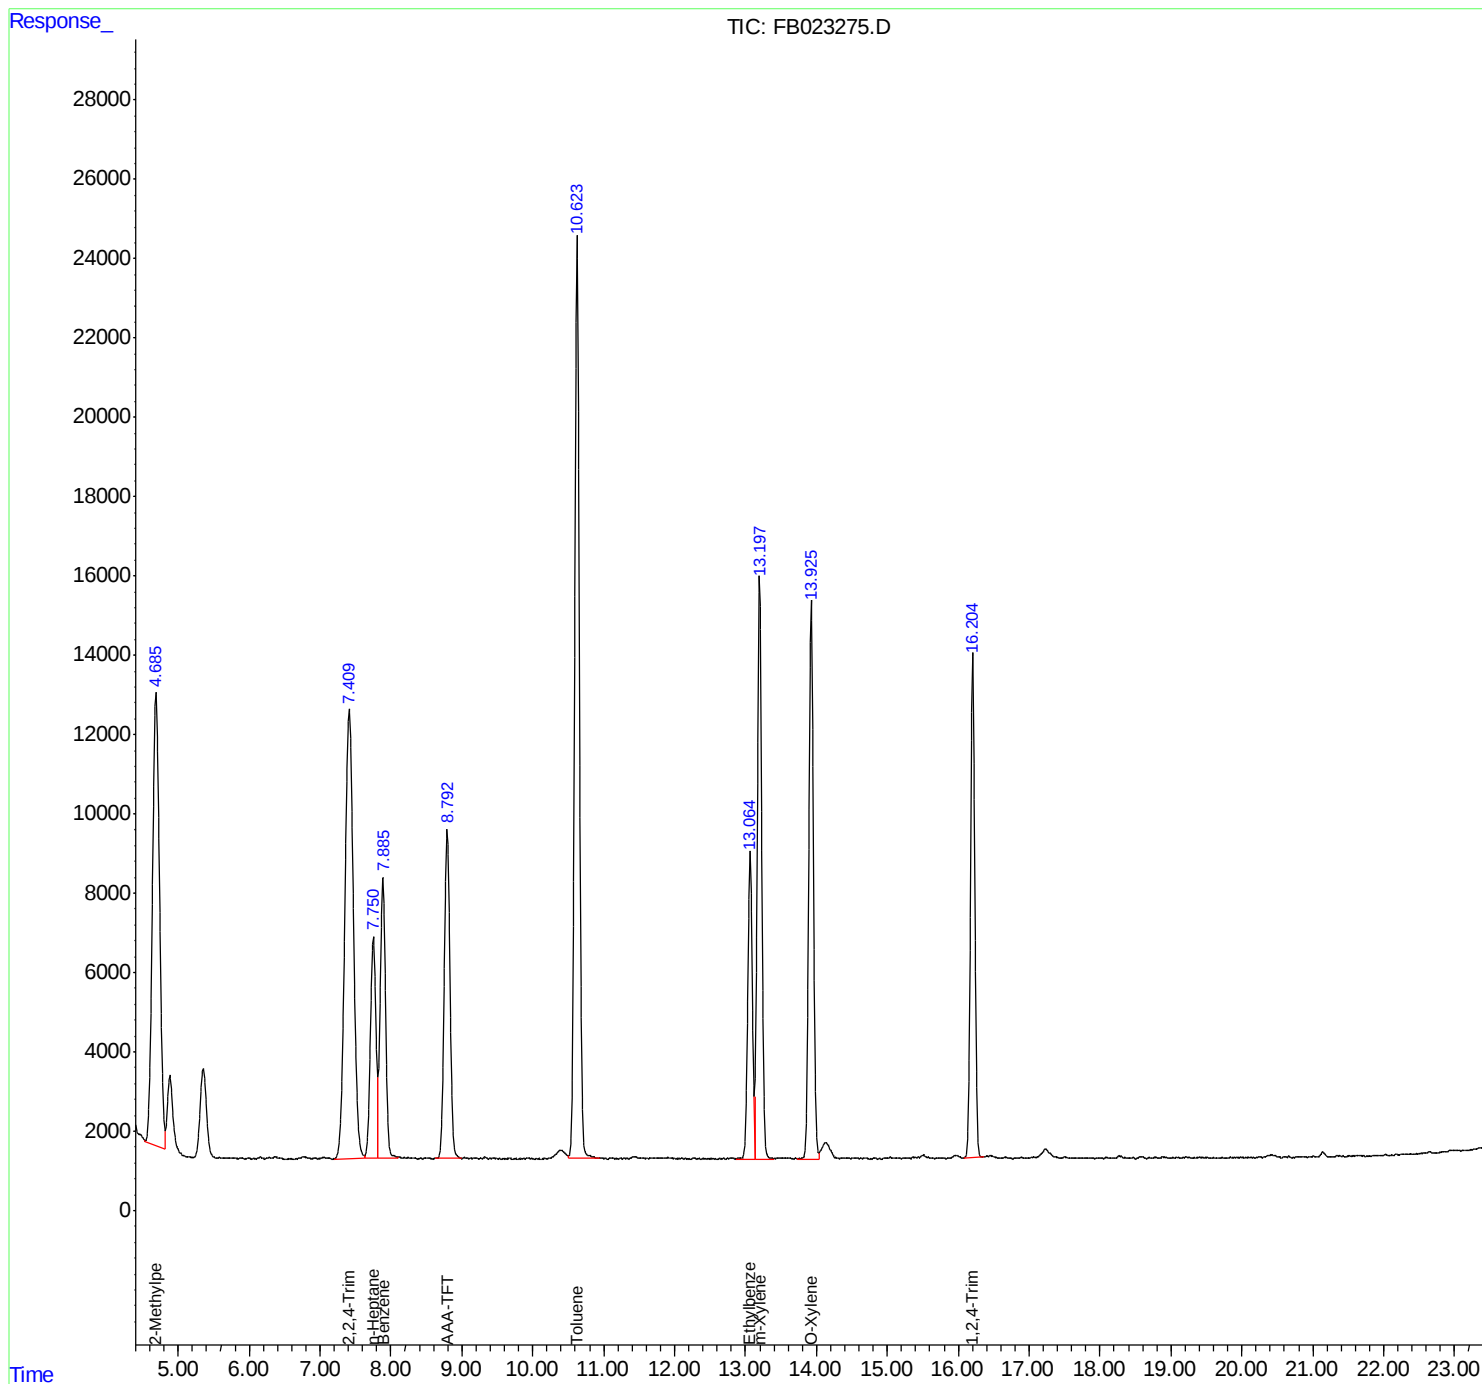

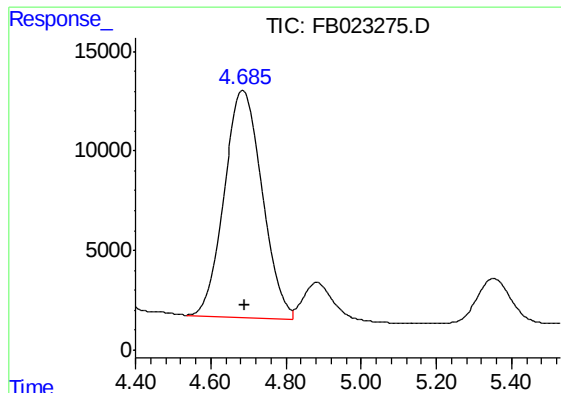


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: -0.005 min
Response: 797366
Conc: 24.40 ng/ml

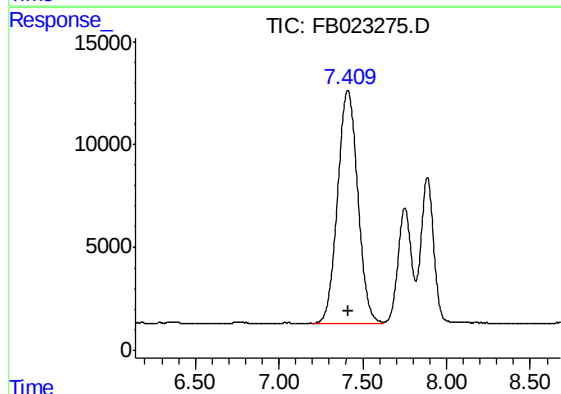


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.007 min
Response: 952339
Conc: 27.31 ng/ml

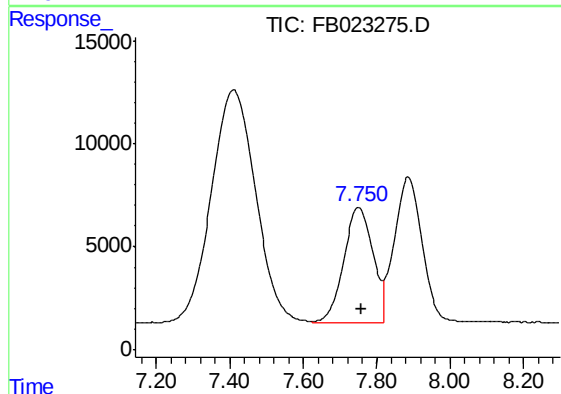


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.007 min
Response: 306616
Conc: 8.92 ng/ml

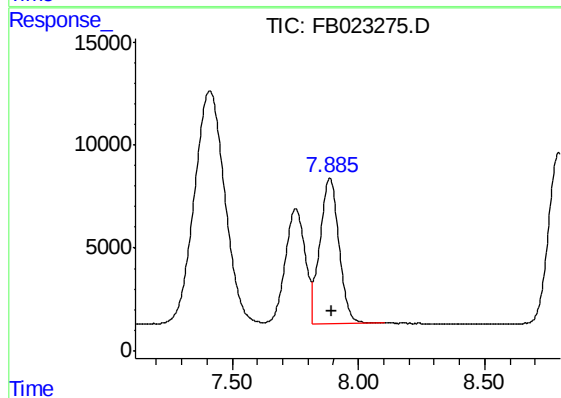


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.006 min
Response: 372547
Conc: 8.94 ng/ml

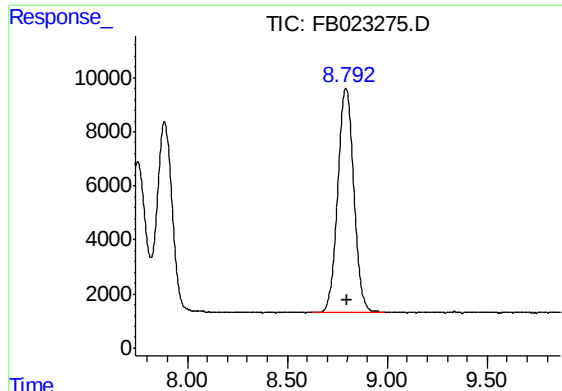


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: -0.006 min
Response: 464667
Conc: 18.92 ng/ml

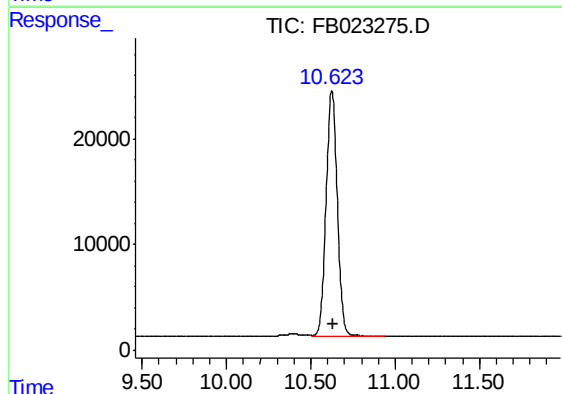


#6 Toluene

R.T.: 10.625 min
Delta R.T.: -0.006 min
Response: 1076744
Conc: 26.73 ng/ml

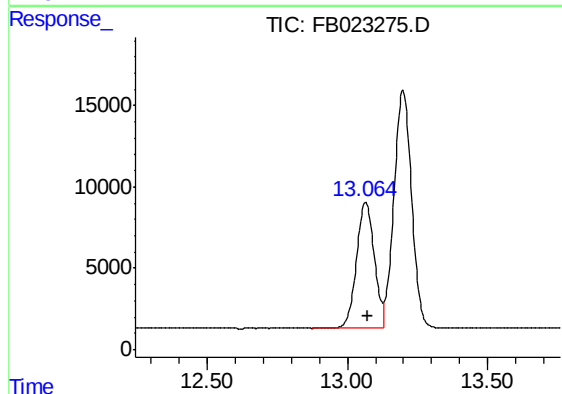


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.005 min
Response: 343834
Conc: 8.91 ng/ml

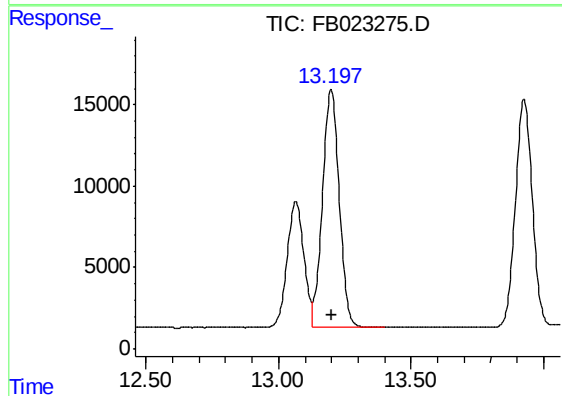


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: -0.005 min
Response: 648412
Conc: 17.82 ng/ml

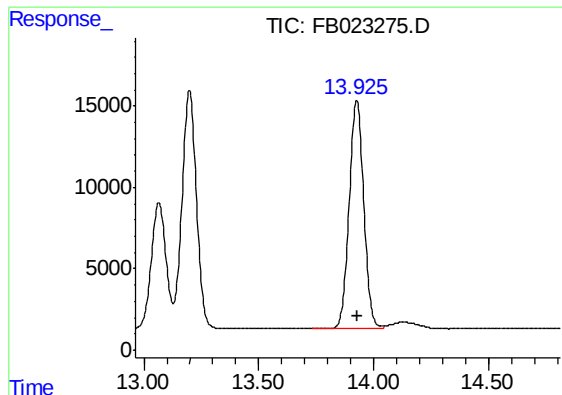

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: -0.005 min
Response: 629008
Conc: 18.12 ng/ml

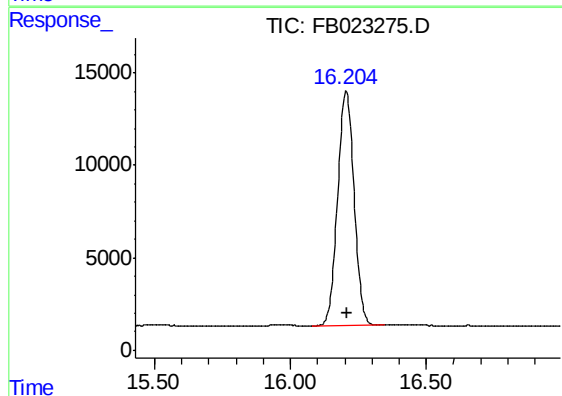

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.005 min
Response: 534712
Conc: 19.07 ng/ml