

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121918\
 Data File : FE029334.D
 Signal(s) : FID1B.CH
 Acq On : 19 Dec 2018 11:10
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 20 04:00:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE120718.M
 Quant Title :
 QLast Update : Fri Dec 07 23:47:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
5) N-DODECANE	6.574	7270388	40.356 ug/ml
11) N-OCTACOSANE	17.024	7283611	39.195 ug/ml
12) N-DOTRIACONTANE	18.737	644812	3.541 ug/ml
14) N-HEXATRIACONTANE	20.264	285236	1.592 ug/ml
15) N-TETRACONTANE	21.992	110798	0.711 ug/ml
16) N-TETRTETRACOCANE	24.917	150432	1.283 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121918\
Data File : FE029334.D
Signal(s) : FID1B.CH
Acq On : 19 Dec 2018 11:10
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 20 04:00:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE120718.M
Quant Title :
QLast Update : Fri Dec 07 23:47:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

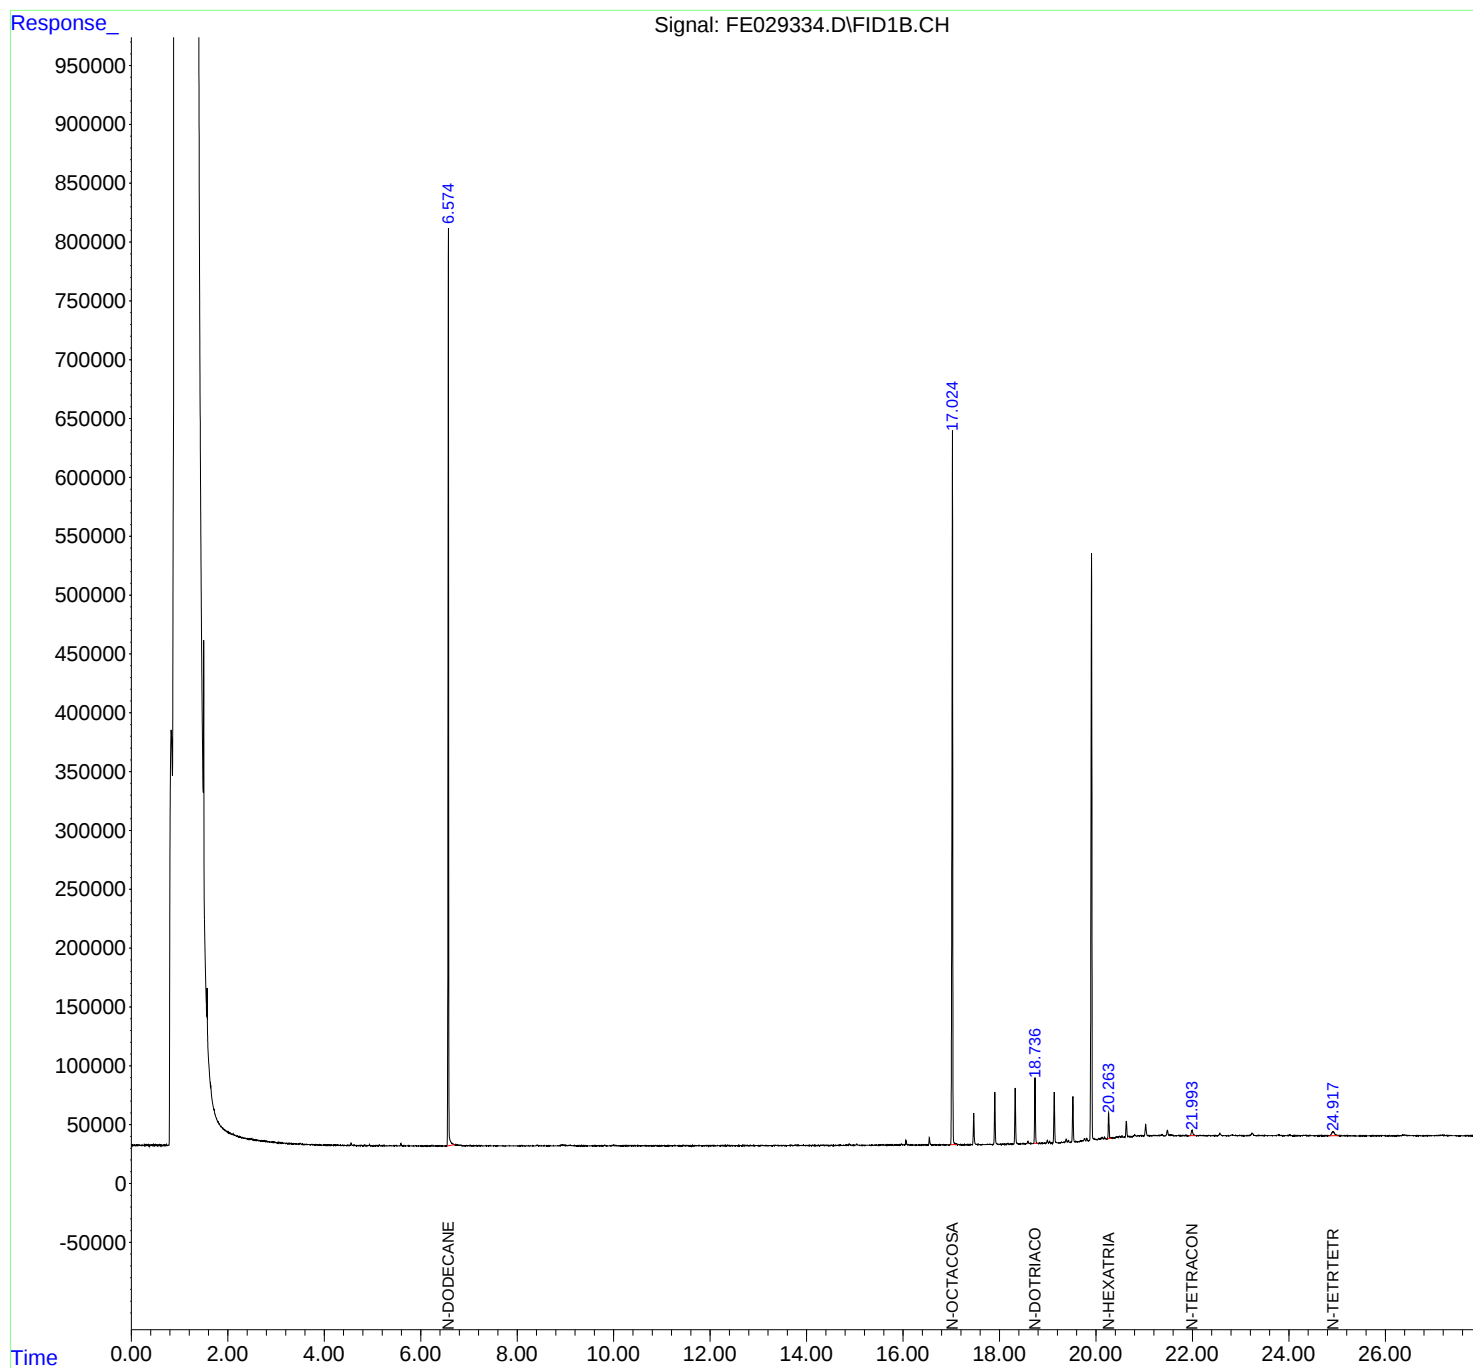


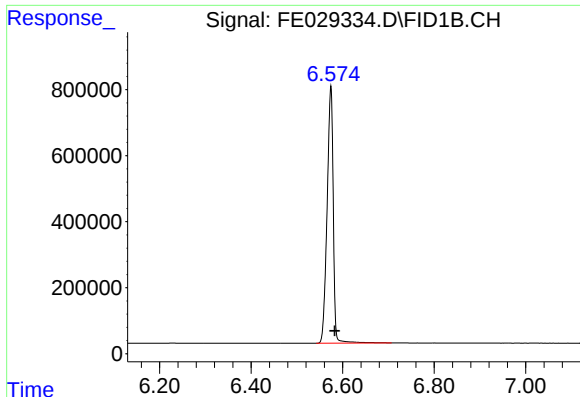

#5 N-DODECANE


R.T.: 6.574 min
Delta R.T.: -0.008 min
Response: 7270388
Conc: 40.36 ug/ml

Instrument :
FID_B
ClientSampleId :

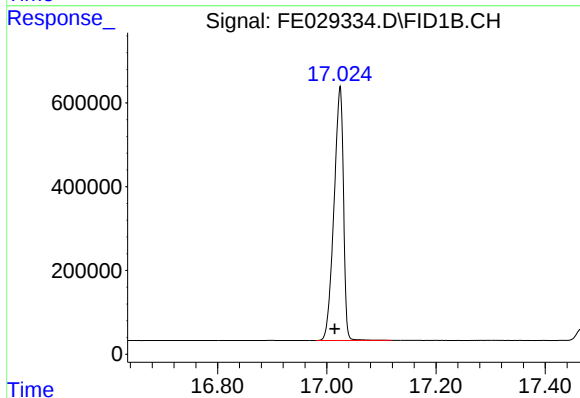


#11 N-OCTACOSANE

R.T.: 17.024 min
Delta R.T.: 0.010 min
Response: 7283611
Conc: 39.19 ug/ml

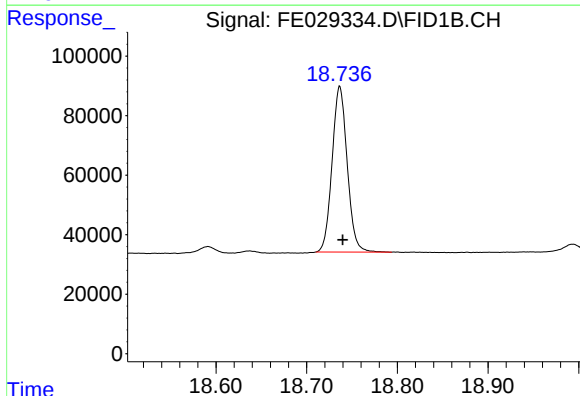


#12 N-DOTRIACONTANE

R.T.: 18.737 min
Delta R.T.: -0.003 min
Response: 644812
Conc: 3.54 ug/ml

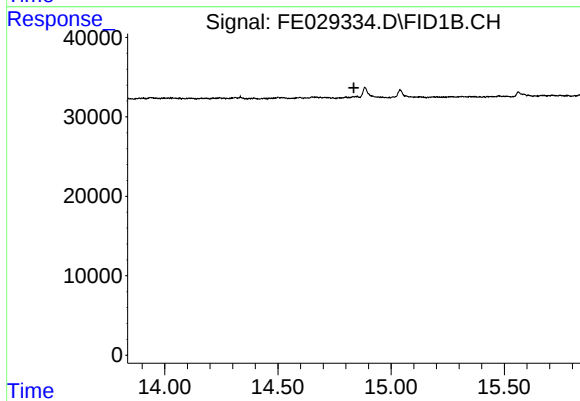

#13 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.835 min
Response: 0
Conc: N.D.

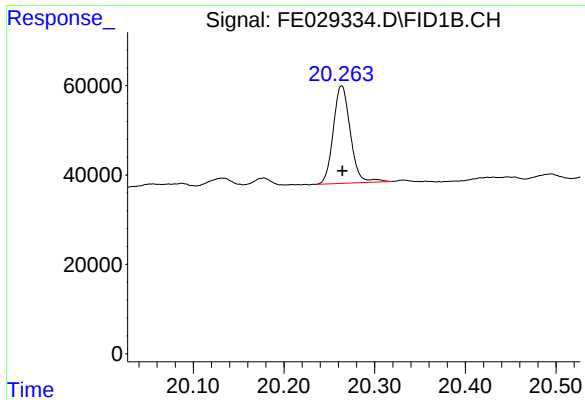

#14 N-HEXATRIACONTANE


R.T.: 20.264 min
Delta R.T.: 0.000 min
Response: 285236
Conc: 1.59 ug/ml

Instrument :
FID_B
ClientSampleId :

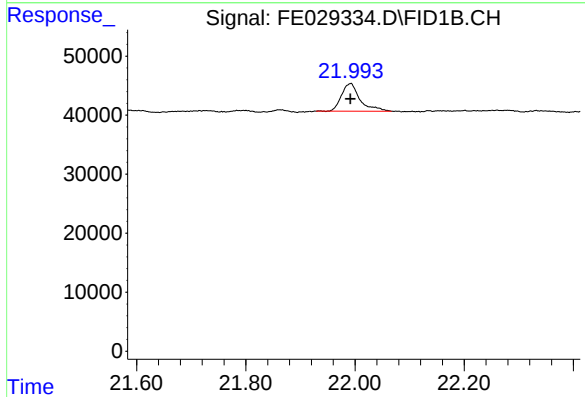

#15 N-TETRACONTANE

R.T.: 21.992 min
Delta R.T.: 0.000 min
Response: 110798
Conc: 0.71 ug/ml

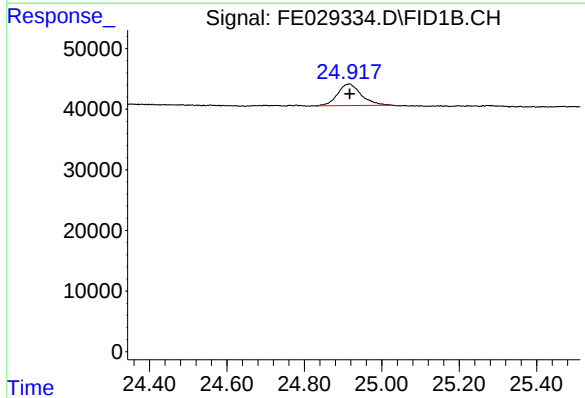

#16 N-TETRTETRACONTANE

R.T.: 24.917 min
Delta R.T.: 0.000 min
Response: 150432
Conc: 1.28 ug/ml