

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121918\
 Data File : FB019116.D
 Signal(s) : FID2B.CH
 Acq On : 19 Dec 2018 9:11
 Operator : MJ/SJ
 Sample : BSF1219S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1219S1

Integration File: Calibration.e
 Quant Time: Dec 20 02:44:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.107	157825	18.056 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.959	406222	26.572 ng/ml
2) t 2,2,4-Trimethylpentane	7.722	424997	27.587 ng/ml
3) t n-Heptane	8.061	140846	9.476 ng/ml
4) t Benzene	8.202	177293	9.843 ng/ml
6) t Toluene	10.956	438675	28.900 ng/ml
7) t Ethylbenzene	13.405	146573	9.434 ng/ml
8) t m-Xylene	13.538	314510	19.305 ng/ml
9) t O-Xylene	14.270	338045	19.993 ng/ml
10) t 1,2,4-Trimethylbenzene	16.553	396891	19.611 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121918\
Data File : FB019116.D
Signal(s) : FID2B.CH
Acq On : 19 Dec 2018 9:11
Operator : MJ/SJ
Sample : BSF1219S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1219S1

Integration File: Calibration.e
Quant Time: Dec 20 02:44:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

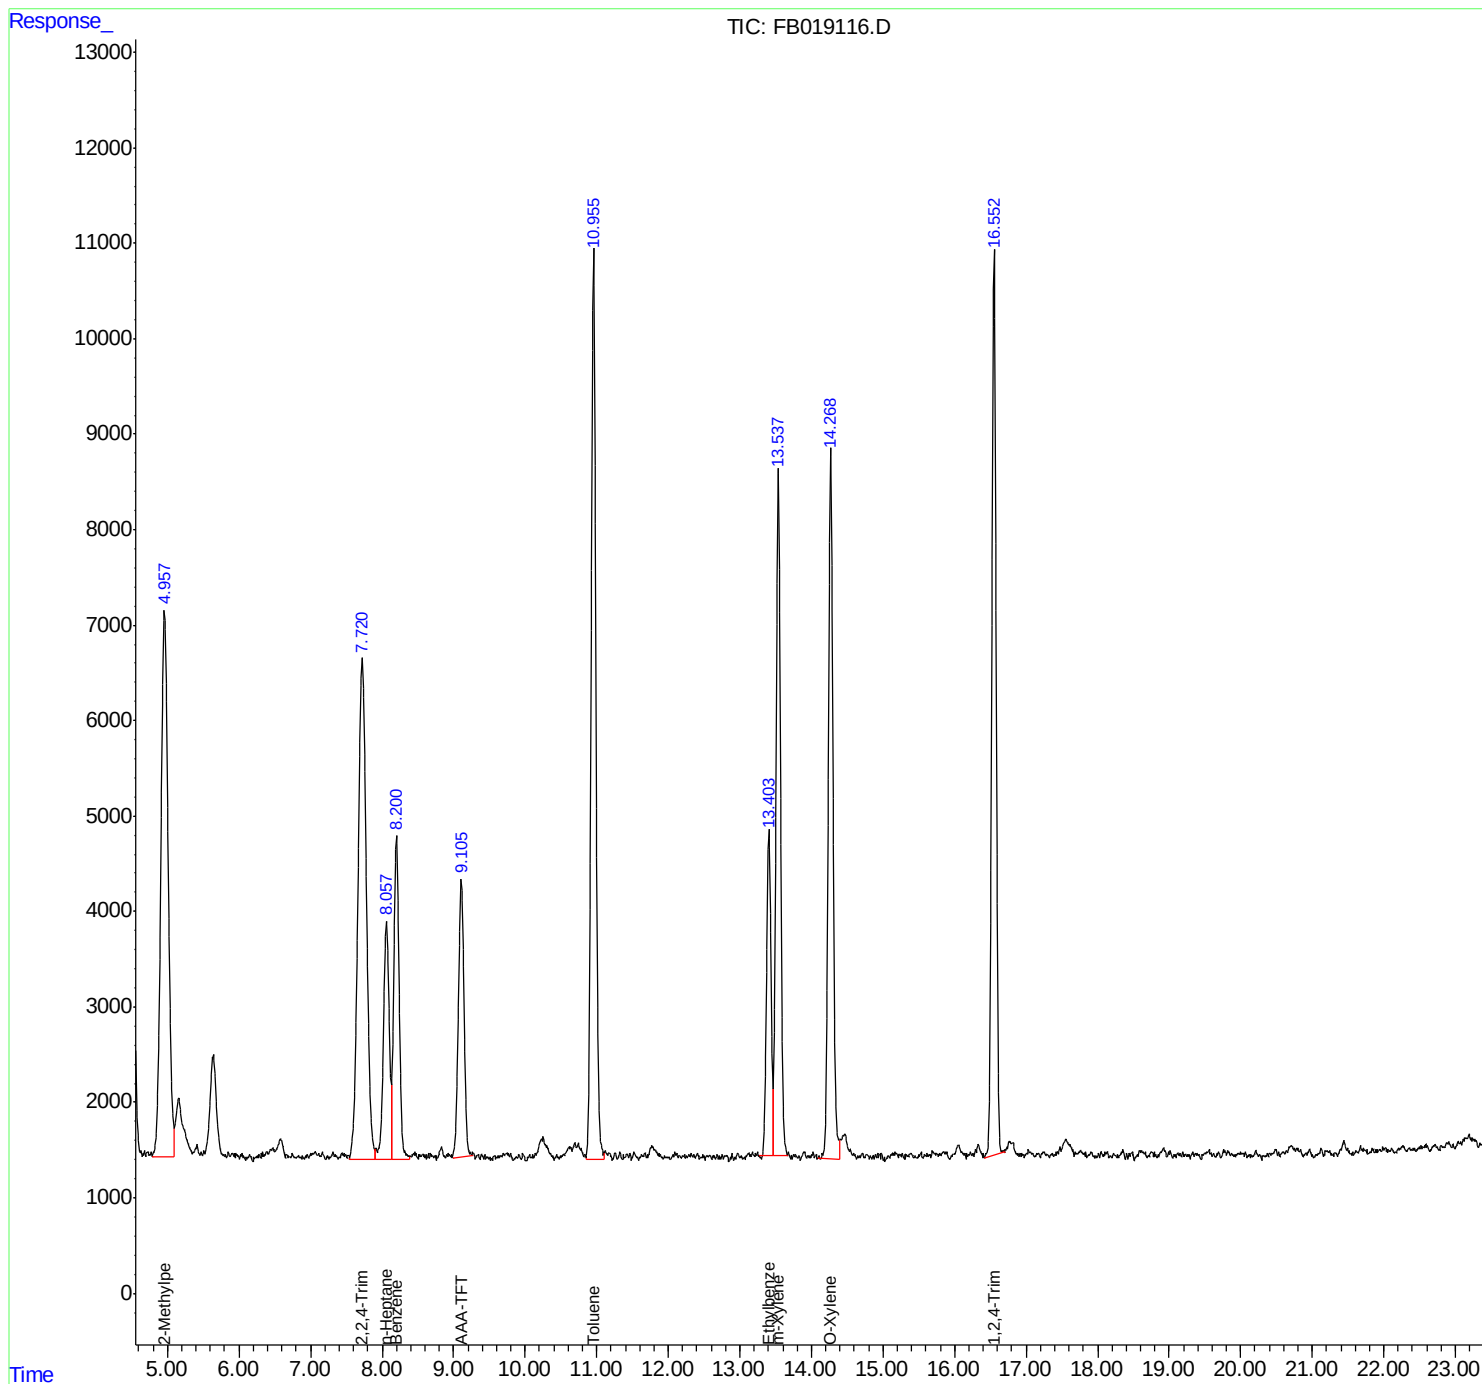


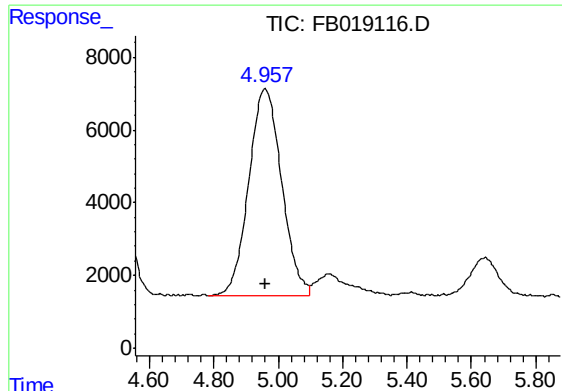

#1 2-Methylpentane


R.T.: 4.959 min
Delta R.T.: -0.002 min
Response: 406222
Conc: 26.57 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1219S1

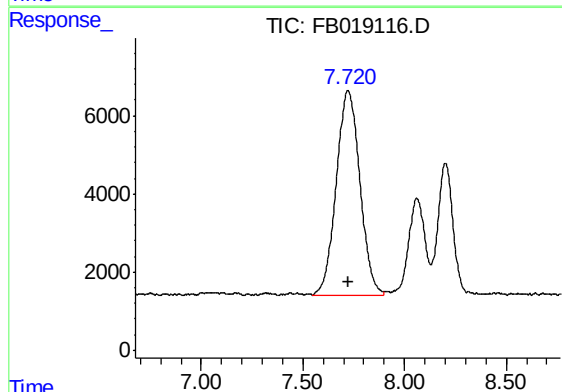


#2 2,2,4-Trimethylpentane

R.T.: 7.722 min
Delta R.T.: 0.000 min
Response: 424997
Conc: 27.59 ng/ml

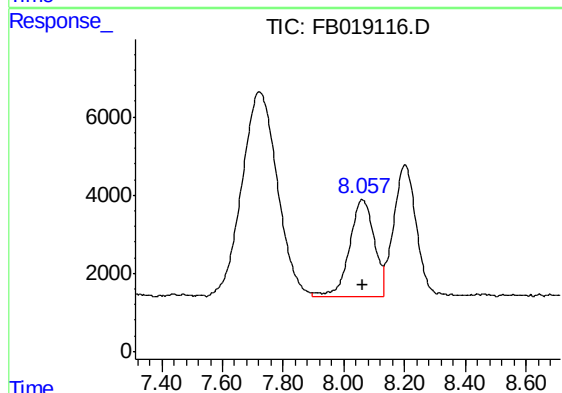


#3 n-Heptane

R.T.: 8.061 min
Delta R.T.: -0.002 min
Response: 140846
Conc: 9.48 ng/ml

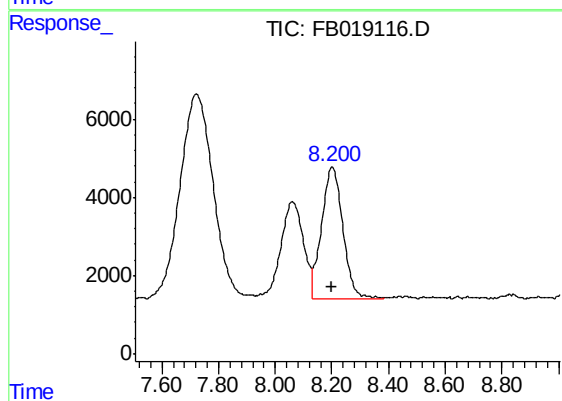

#4 Benzene


R.T.: 8.202 min
Delta R.T.: 0.000 min
Response: 177293
Conc: 9.84 ng/ml

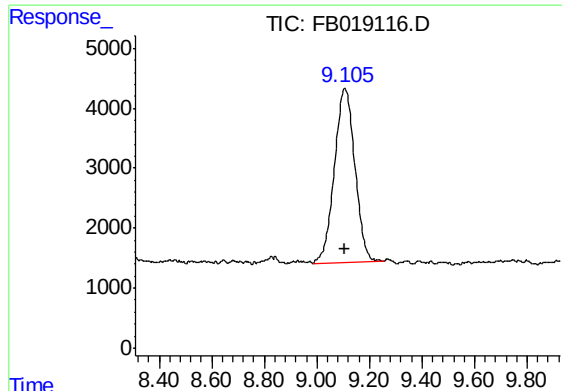

#5 AAA-TFT


R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 157825
Conc: 18.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1219S1

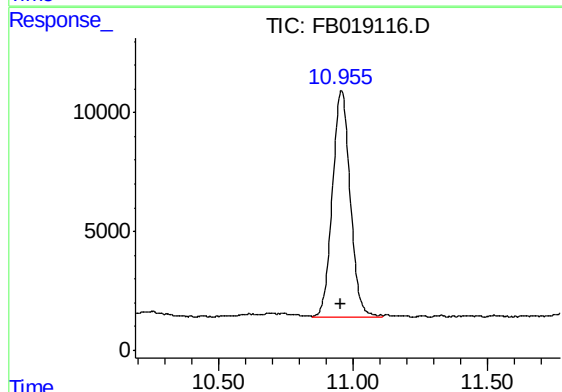


#6 Toluene

R.T.: 10.956 min
Delta R.T.: 0.000 min
Response: 438675
Conc: 28.90 ng/ml

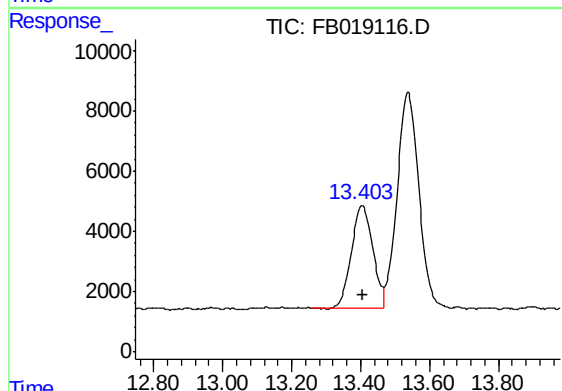


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: 0.000 min
Response: 146573
Conc: 9.43 ng/ml

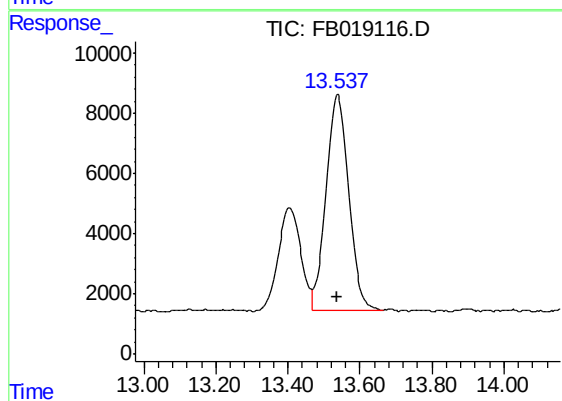

#8 m-Xylene


R.T.: 13.538 min
Delta R.T.: 0.000 min
Response: 314510
Conc: 19.30 ng/ml

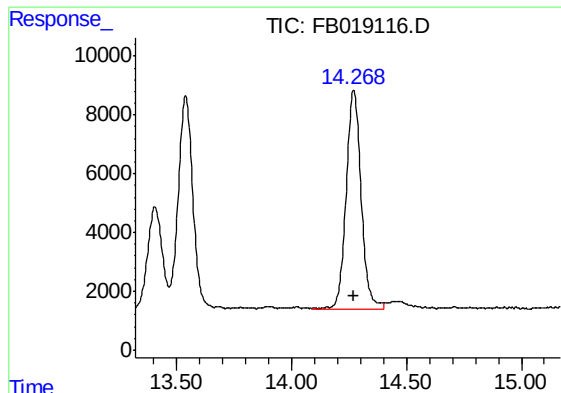

#9 O-Xylene

R.T.: 14.270 min
Delta R.T.: 0.000 min
Response: 338045
Conc: 19.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1219S1

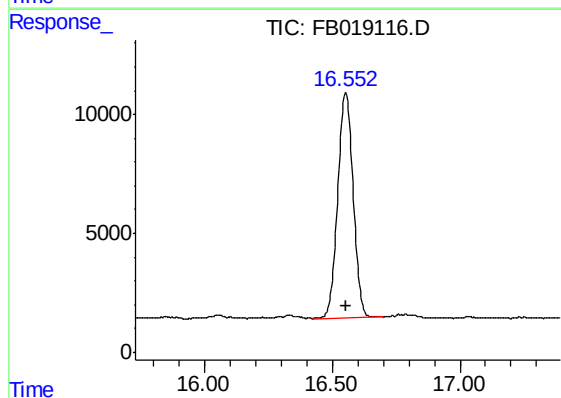

#10 1,2,4-Trimethylbenzene

R.T.: 16.553 min
Delta R.T.: 0.000 min
Response: 396891
Conc: 19.61 ng/ml