

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121918\
 Data File : FB019132.D
 Signal(s) : FID2B.CH
 Acq On : 19 Dec 2018 17:18
 Operator : MJ/SJ
 Sample : J6196-07MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 EO-01-121818-AMSD

Integration File: Calibration.e
 Quant Time: Dec 20 02:50:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.109	146659	16.779 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.961	334468	21.878 ng/ml
2) t 2,2,4-Trimethylpentane	7.726	289592	18.797 ng/ml
3) t n-Heptane	8.068	92710	6.237 ng/ml
4) t Benzene	8.205	162043	8.996 ng/ml
6) t Toluene	10.960	393267	25.909 ng/ml
7) t Ethylbenzene	13.410	131169	8.443 ng/ml
8) t m-Xylene	13.543	267571	16.424 ng/ml
9) t O-Xylene	14.274	290842	17.201 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	307267	15.183 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB121918\
Data File : FB019132.D
Signal(s) : FID2B.CH
Acq On : 19 Dec 2018 17:18
Operator : MJ/SJ
Sample : J6196-07MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
EO-01-121818-AMSD

Integration File: Calibration.e
Quant Time: Dec 20 02:50:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

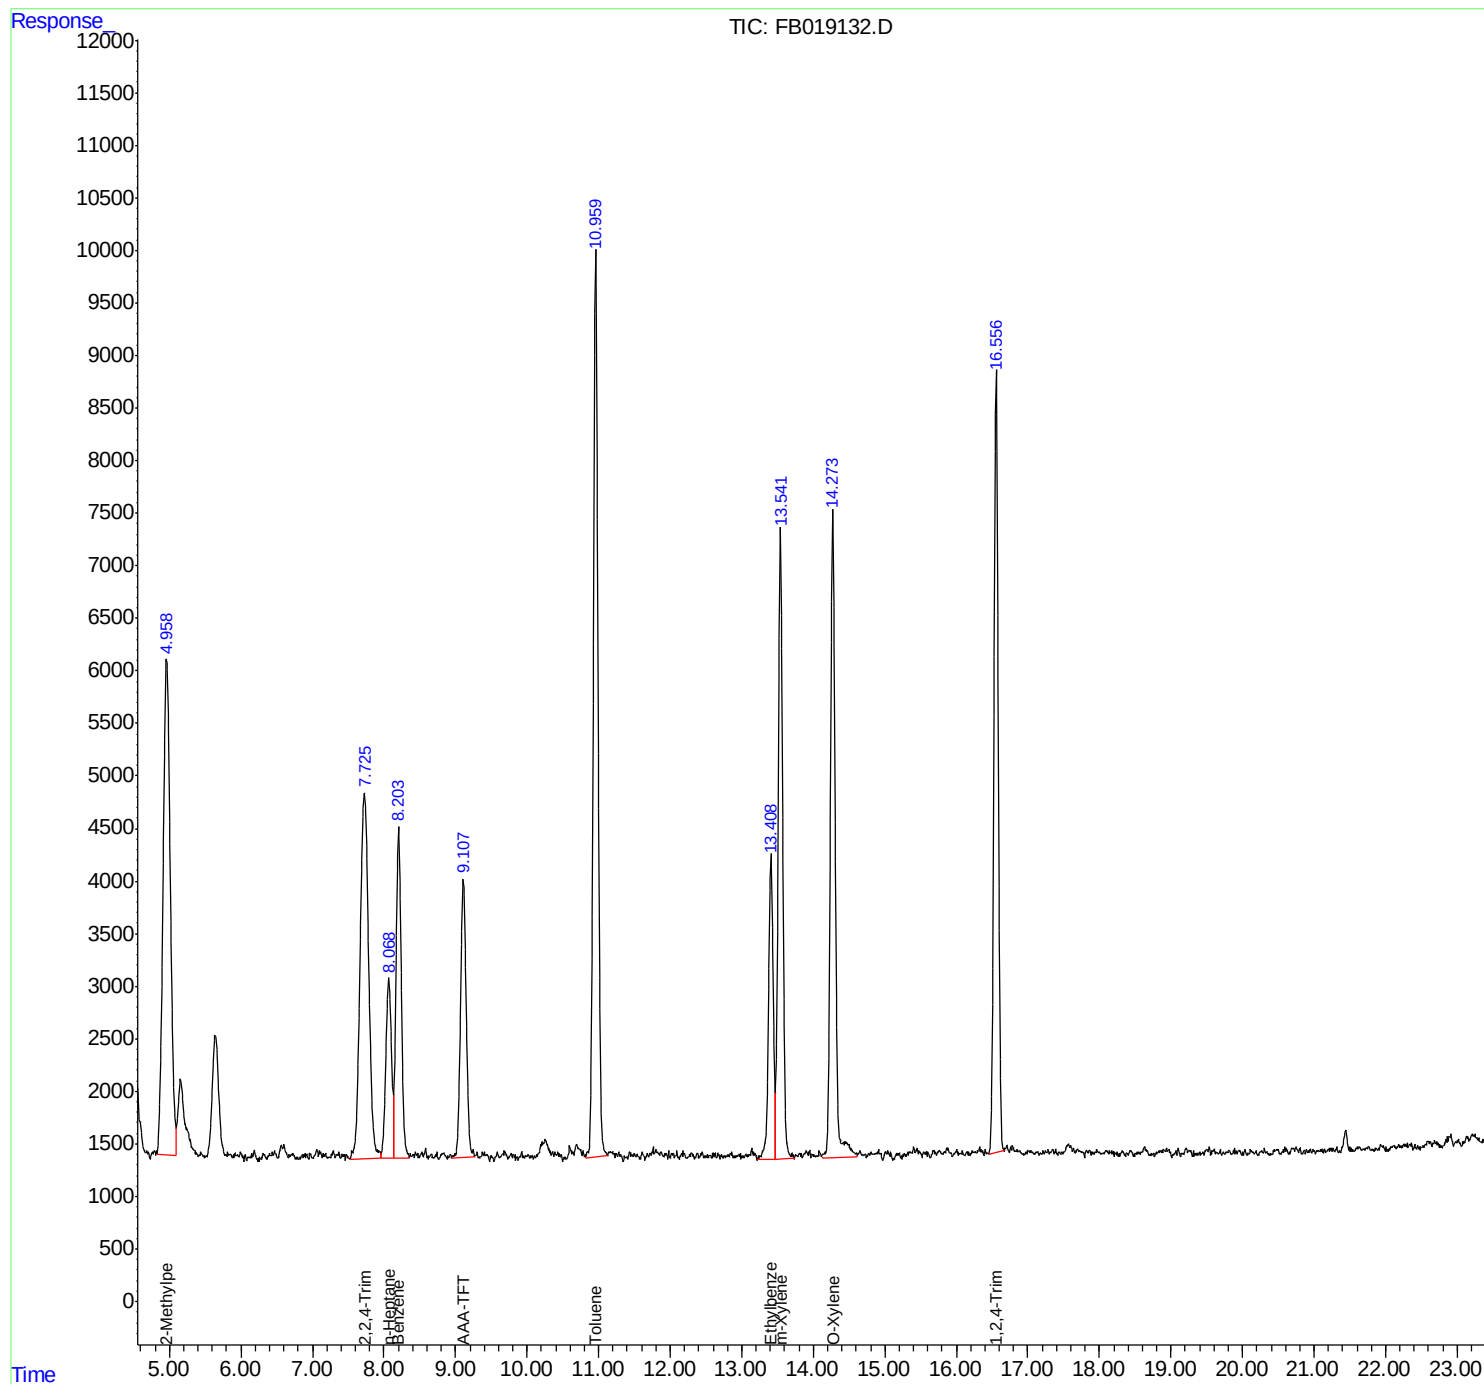


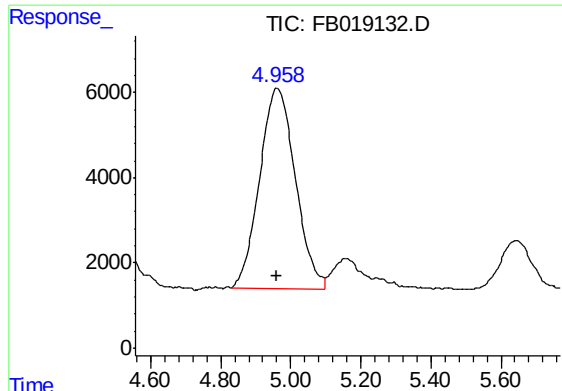

#1 2-Methylpentane


R.T.: 4.961 min
Delta R.T.: 0.000 min
Response: 334468
Conc: 21.88 ng/ml

Instrument :
FID_B
ClientSampleId :
EO-01-121818-AMSD

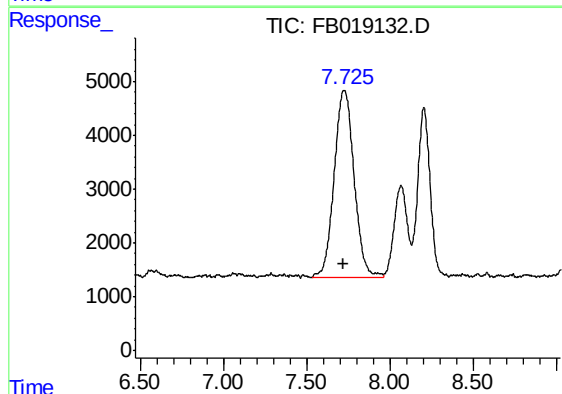


#2 2,2,4-Trimethylpentane

R.T.: 7.726 min
Delta R.T.: 0.003 min
Response: 289592
Conc: 18.80 ng/ml

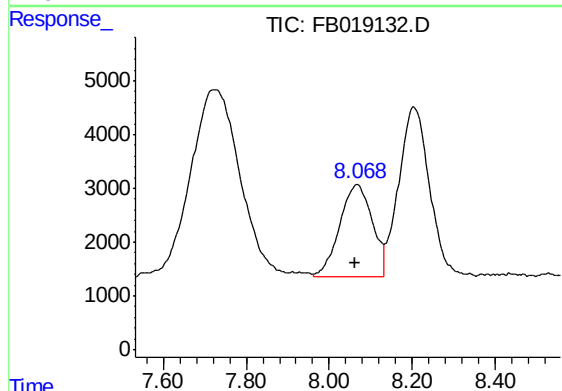


#3 n-Heptane

R.T.: 8.068 min
Delta R.T.: 0.006 min
Response: 92710
Conc: 6.24 ng/ml

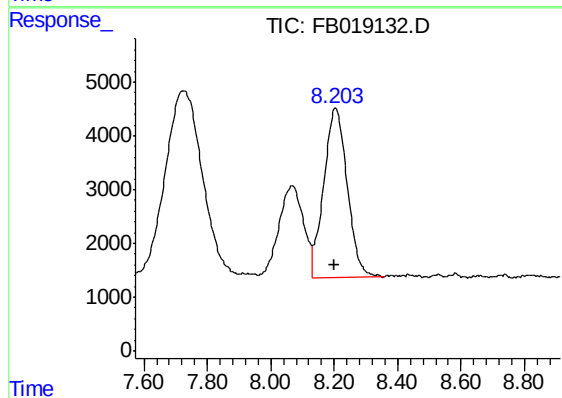

#4 Benzene


R.T.: 8.205 min
Delta R.T.: 0.004 min
Response: 162043
Conc: 9.00 ng/ml

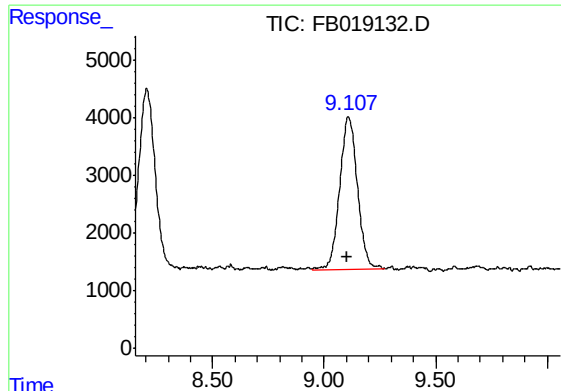

#5 AAA-TFT


R.T.: 9.109 min
Delta R.T.: 0.003 min
Response: 146659
Conc: 16.78 ng/ml

Instrument :
FID_B
ClientSampleId :
EO-01-121818-AMSD

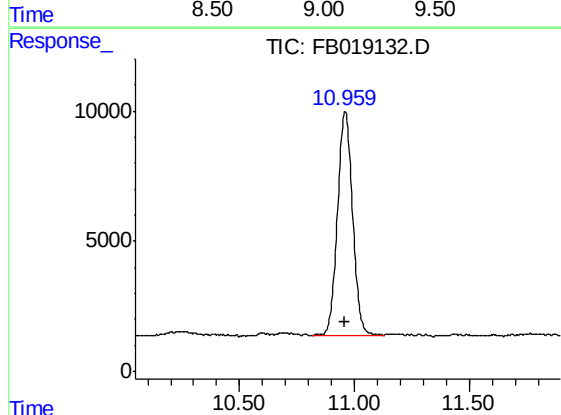


#6 Toluene

R.T.: 10.960 min
Delta R.T.: 0.004 min
Response: 393267
Conc: 25.91 ng/ml

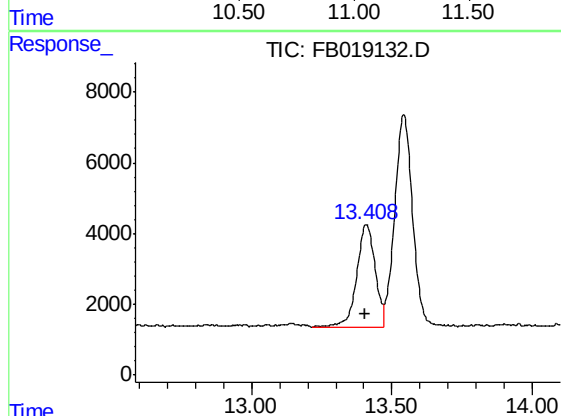


#7 Ethylbenzene

R.T.: 13.410 min
Delta R.T.: 0.004 min
Response: 131169
Conc: 8.44 ng/ml

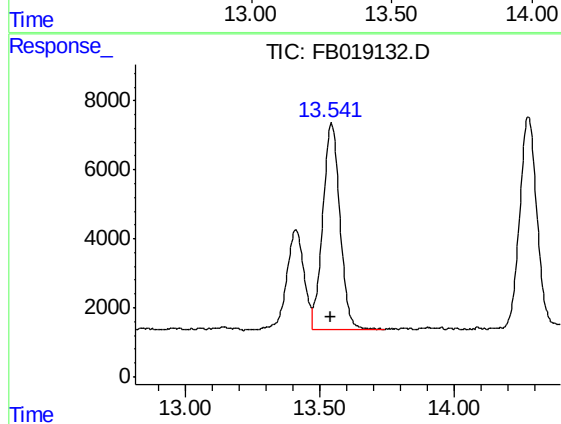

#8 m-Xylene


R.T.: 13.543 min
Delta R.T.: 0.005 min
Response: 267571
Conc: 16.42 ng/ml

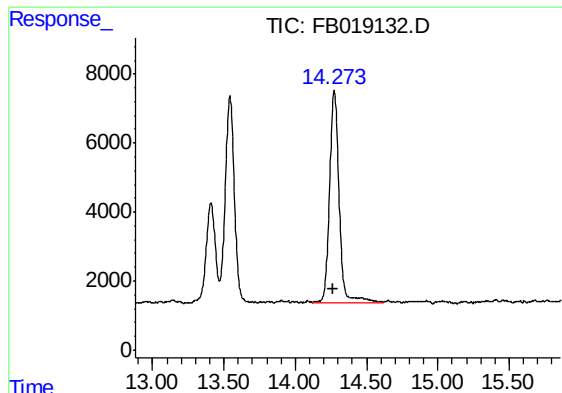

#9 O-Xylene

R.T.: 14.274 min
Delta R.T.: 0.005 min
Response: 290842
Conc: 17.20 ng/ml

Instrument :
FID_B
ClientSampleId :
EO-01-121818-AMSD

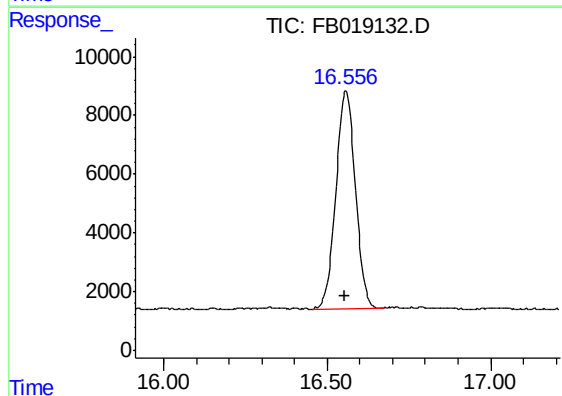

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.005 min
Response: 307267
Conc: 15.18 ng/ml